

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021040.D
 Acq On : 16 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2031-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG534

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	105	rVB	164274	182422	11.27%	1.402%
2	1.571	159	165	183	rVB	130238	166052	10.26%	1.276%
3	2.108	323	332	355	rBV	361578	520312	32.15%	3.999%
4	2.387	416	419	421	rBV2	399	291	0.02%	0.002%
5	2.452	436	439	444	rBV3	644	528	0.03%	0.004%
6	2.478	444	447	449	rBV2	635	331	0.02%	0.003%
7	2.616	488	490	491	rBV2	672	286	0.02%	0.002%
8	2.741	527	529	531	rVB	745	357	0.02%	0.003%
9	2.767	532	537	538	rBV2	684	431	0.03%	0.003%
10	3.381	725	728	731	rVB	381	291	0.02%	0.002%
11	3.407	731	736	739	rBV	505	369	0.02%	0.003%
12	3.648	808	811	814	rBV	408	328	0.02%	0.003%
13	3.899	878	889	932	rBV	85569	309929	19.15%	2.382%
14	4.349	1013	1029	1064	rBV	290594	733254	45.30%	5.635%
15	4.638	1116	1119	1124	rVV3	496	505	0.03%	0.004%
16	4.741	1147	1151	1157	rBV3	621	775	0.05%	0.006%
17	4.793	1164	1167	1170	rBV3	529	338	0.02%	0.003%
18	4.860	1184	1188	1192	rBV	473	382	0.02%	0.003%
19	4.915	1202	1205	1208	rBB3	484	309	0.02%	0.002%
20	4.944	1211	1214	1217	rBV	465	392	0.02%	0.003%
21	5.047	1229	1246	1276	rBV2	621552	1618598	100.00%	12.439%
22	5.368	1343	1346	1354	rBV3	680	641	0.04%	0.005%
23	5.400	1354	1356	1358	rBV	741	407	0.03%	0.003%
24	5.497	1383	1386	1388	rVB3	515	300	0.02%	0.002%
25	5.545	1397	1401	1406	rVB4	421	340	0.02%	0.003%
26	5.619	1411	1424	1447	rBV	530122	1064086	65.74%	8.178%
27	5.838	1486	1492	1499	rBV5	896	1248	0.08%	0.010%
28	5.915	1509	1516	1525	rVB8	2383	3681	0.23%	0.028%
29	5.953	1526	1528	1531	rVB2	643	287	0.02%	0.002%
30	5.982	1535	1537	1541	rBV	639	434	0.03%	0.003%
31	6.072	1551	1565	1588	rBV	346645	702581	43.41%	5.399%
32	6.210	1604	1608	1617	rBV4	1683	2350	0.15%	0.018%
33	6.278	1628	1629	1635	rVB3	718	453	0.03%	0.003%
34	6.365	1653	1656	1658	rBV2	461	310	0.02%	0.002%
35	6.423	1669	1674	1677	rBV2	478	590	0.04%	0.005%
36	6.516	1697	1703	1704	rBV2	1181	719	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021040.D
 Acq On : 16 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2031-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG534

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.645	1740	1743	1745	rBV2	534	309	0.02%	0.002%
38	6.677	1750	1753	1758	rVV3	502	425	0.03%	0.003%
39	6.805	1791	1793	1796	rVB2	649	362	0.02%	0.003%
40	6.870	1811	1813	1816	rBV	512	364	0.02%	0.003%
41	6.989	1839	1850	1869	rBV	212315	381286	23.56%	2.930%
42	7.162	1899	1904	1907	rBV2	857	741	0.05%	0.006%
43	7.252	1926	1932	1936	rBV4	1160	1218	0.08%	0.009%
44	7.317	1940	1952	1968	rBV	758520	1330371	82.19%	10.224%
45	7.625	2037	2048	2064	rBV	153844	261779	16.17%	2.012%
46	7.828	2105	2111	2116	rBV2	530	713	0.04%	0.005%
47	7.863	2116	2122	2130	rVB6	2405	3574	0.22%	0.027%
48	7.937	2134	2145	2147	rBV5	3109	3625	0.22%	0.028%
49	8.021	2168	2171	2174	rBV2	509	436	0.03%	0.003%
50	8.091	2181	2193	2226	rBV	419514	757908	46.82%	5.825%
51	8.435	2298	2300	2303	rBV	719	352	0.02%	0.003%
52	8.458	2303	2307	2309	rBV3	630	521	0.03%	0.004%
53	8.506	2319	2322	2326	rBV2	1048	569	0.04%	0.004%
54	8.593	2345	2349	2351	rBV	445	361	0.02%	0.003%
55	8.616	2354	2356	2359	rBV2	509	342	0.02%	0.003%
56	8.661	2368	2370	2374	rBV2	535	368	0.02%	0.003%
57	8.680	2374	2376	2380	rVB	510	346	0.02%	0.003%
58	8.808	2414	2416	2419	rBV2	426	319	0.02%	0.002%
59	8.853	2419	2430	2454	rBV	795719	1298974	80.25%	9.983%
60	9.149	2512	2522	2523	rBV6	4383	4758	0.29%	0.037%
61	9.291	2563	2566	2571	rBV2	550	469	0.03%	0.004%
62	9.410	2598	2603	2607	rBV	523	605	0.04%	0.005%
63	9.554	2639	2648	2662	rBV3	9497	16138	1.00%	0.124%
64	9.651	2675	2678	2682	rBV2	494	419	0.03%	0.003%
65	9.699	2687	2693	2696	rBV3	680	601	0.04%	0.005%
66	9.728	2699	2702	2703	rBV2	1141	620	0.04%	0.005%
67	9.837	2731	2736	2739	rBV3	538	584	0.04%	0.004%
68	9.940	2762	2768	2774	rBV3	1305	1442	0.09%	0.011%
69	10.133	2821	2828	2836	rBV5	2768	3748	0.23%	0.029%
70	10.220	2844	2855	2875	rBV2	577281	902332	55.75%	6.934%
71	10.332	2887	2890	2893	rBV2	833	594	0.04%	0.005%
72	10.387	2902	2907	2915	rVB5	3794	5568	0.34%	0.043%
73	10.439	2920	2923	2926	rBV2	688	565	0.03%	0.004%
74	10.670	2993	2995	2998	rBV	585	326	0.02%	0.003%
75	10.738	3013	3016	3017	rBV	509	273	0.02%	0.002%
76	10.847	3044	3050	3051	rBV3	634	655	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021040.D
 Acq On : 16 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2031-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG534

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

77	10.921	3064	3073	3083	rBV6	5809	7681	0.47%	0.059%
78	11.040	3106	3110	3115	rBV5	843	931	0.06%	0.007%
79	11.120	3128	3135	3137	rBV2	673	878	0.05%	0.007%
80	11.255	3165	3177	3196	rBV	816943	1260723	77.89%	9.689%
81	11.535	3254	3264	3276	rBV2	20013	31870	1.97%	0.245%
82	11.631	3282	3294	3311	rBV	870097	1378420	85.16%	10.593%
83	11.831	3352	3356	3357	rBV2	567	396	0.02%	0.003%
84	11.931	3385	3387	3390	rVB2	692	293	0.02%	0.002%
85	12.040	3418	3421	3425	rBV2	679	527	0.03%	0.004%
86	12.062	3425	3428	3430	rVV2	480	353	0.02%	0.003%
87	12.258	3480	3489	3493	rBV4	2278	2713	0.17%	0.021%
88	12.464	3550	3553	3557	rVV2	460	372	0.02%	0.003%
89	12.654	3607	3612	3614	rBV2	742	557	0.03%	0.004%
90	12.673	3614	3618	3619	rBV3	516	399	0.02%	0.003%
91	12.718	3630	3632	3635	rVB2	746	372	0.02%	0.003%
92	13.371	3833	3835	3838	rBV2	710	435	0.03%	0.003%
93	13.406	3843	3846	3849	rBV3	726	489	0.03%	0.004%
94	13.516	3873	3880	3891	rVB2	14398	22191	1.37%	0.171%
95	13.622	3911	3913	3915	rBV2	803	419	0.03%	0.003%
96	14.110	4063	4065	4069	rBV3	728	429	0.03%	0.003%
97	14.397	4151	4154	4161	rBV3	663	685	0.04%	0.005%
98	14.876	4300	4303	4304	rBV2	804	453	0.03%	0.003%
99	15.043	4353	4355	4358	rBV2	1026	487	0.03%	0.004%
100	15.082	4365	4367	4369	rBV2	847	369	0.02%	0.003%




Sum of corrected areas: 13012309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021040.D
Acq On : 16 Apr 2021 12:18
Operator : SY/MD
Sample : M2031-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG534

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

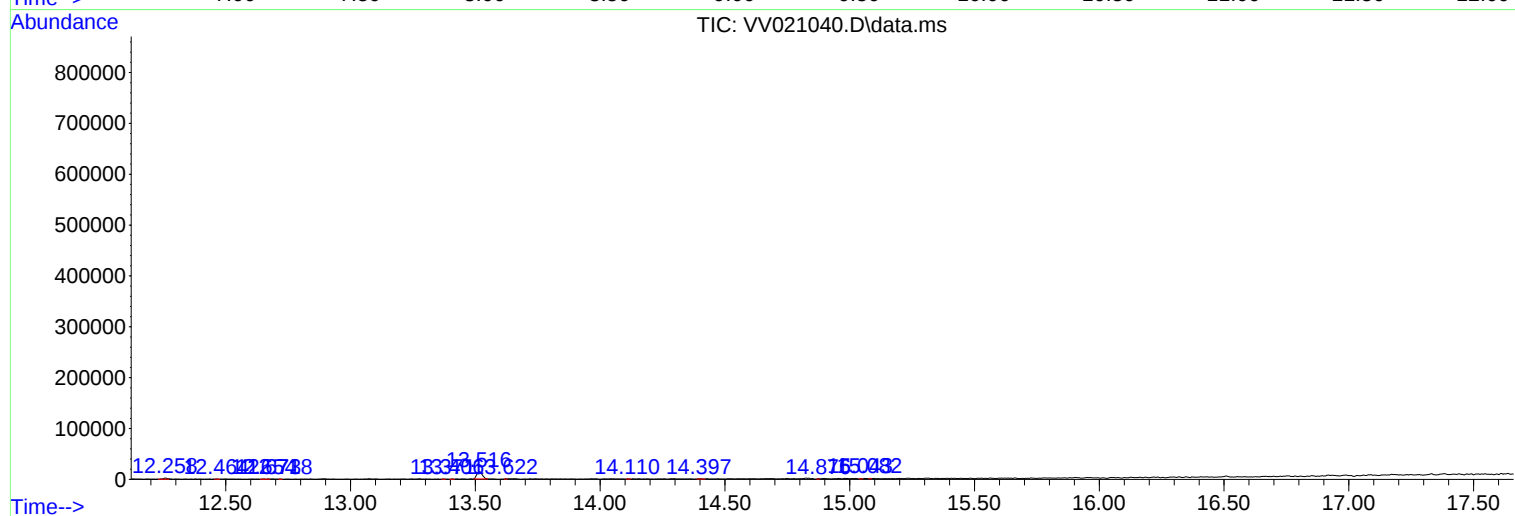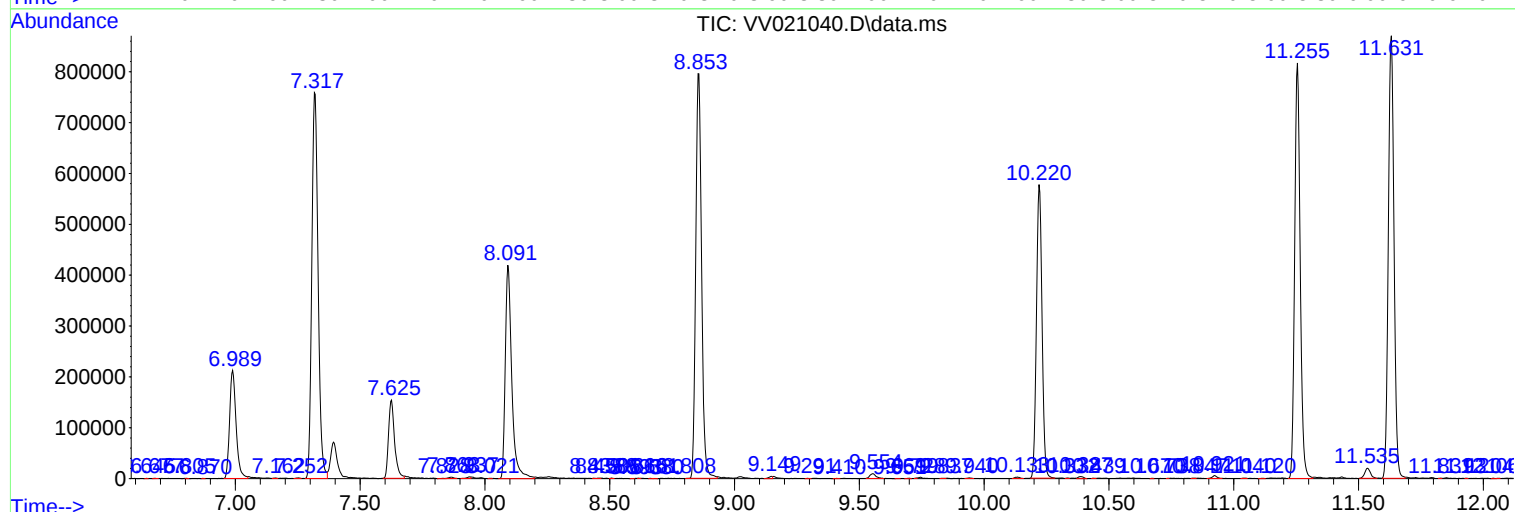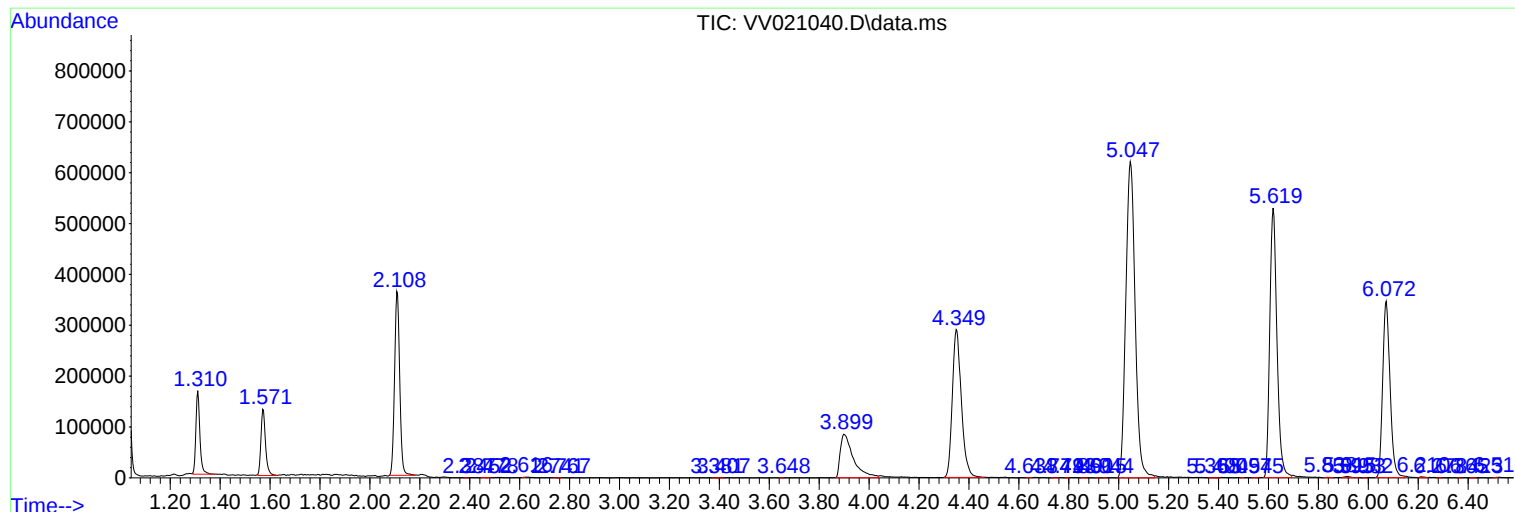

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021040.D
Acq On : 16 Apr 2021 12:18
Operator : SY/MD
Sample : M2031-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG534

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021040.D
Acq On : 16 Apr 2021 12:18
Operator : SY/MD
Sample : M2031-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG534

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
