

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021041.D
 Acq On : 16 Apr 2021 12:41
 Operator : SY/MD
 Sample : M2031-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	154465	174779	10.67%	1.357%
2	1.571	158	165	180	rVB	134309	166512	10.17%	1.293%
3	2.108	322	332	349	rBV	362974	527122	32.18%	4.092%
4	2.436	431	434	436	rBV2	764	493	0.03%	0.004%
5	2.513	451	458	466	rVB5	1402	1750	0.11%	0.014%
6	2.629	489	494	497	rBV2	568	517	0.03%	0.004%
7	2.709	517	519	522	rVB	543	289	0.02%	0.002%
8	2.725	522	524	530	rBV2	413	433	0.03%	0.003%
9	2.761	530	535	539	rBV3	717	716	0.04%	0.006%
10	2.863	565	567	572	rBV2	611	461	0.03%	0.004%
11	2.928	585	587	592	rVB2	703	382	0.02%	0.003%
12	3.240	681	684	686	rBV	527	366	0.02%	0.003%
13	3.587	788	792	796	rBB2	406	316	0.02%	0.002%
14	3.616	799	801	806	rBV2	500	455	0.03%	0.004%
15	3.751	839	843	845	rBV2	927	727	0.04%	0.006%
16	3.812	860	862	865	rBV2	636	427	0.03%	0.003%
17	3.905	879	891	932	rBV2	71944	282864	17.27%	2.196%
18	4.236	991	994	999	rVB3	743	578	0.04%	0.004%
19	4.355	1014	1031	1059	rBV	287901	723679	44.18%	5.618%
20	4.587	1097	1103	1107	rVB3	787	851	0.05%	0.007%
21	4.783	1160	1164	1166	rBV2	459	347	0.02%	0.003%
22	4.912	1203	1204	1208	rVB2	524	293	0.02%	0.002%
23	4.937	1208	1212	1215	rBB2	646	519	0.03%	0.004%
24	4.957	1215	1218	1220	rBV2	461	324	0.02%	0.003%
25	5.050	1230	1247	1275	rBV2	643752	1637954	100.00%	12.716%
26	5.323	1330	1332	1336	rBV2	490	384	0.02%	0.003%
27	5.378	1344	1349	1352	rVB3	627	473	0.03%	0.004%
28	5.400	1352	1356	1359	rBV2	546	412	0.03%	0.003%
29	5.461	1371	1375	1378	rBV2	459	313	0.02%	0.002%
30	5.551	1400	1403	1405	rBV3	426	290	0.02%	0.002%
31	5.622	1410	1425	1455	rBV	549203	1095280	66.87%	8.503%
32	5.912	1510	1515	1517	rBV5	1730	1450	0.09%	0.011%
33	6.002	1538	1543	1546	rBV2	612	696	0.04%	0.005%
34	6.076	1552	1566	1586	rBV	349508	711400	43.43%	5.523%
35	6.330	1642	1645	1646	rBV2	708	378	0.02%	0.003%
36	6.375	1656	1659	1663	rVB5	637	404	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021041.D
 Acq On : 16 Apr 2021 12:41
 Operator : SY/MD
 Sample : M2031-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.420	1671	1673	1678	rVV2	533	365	0.02%	0.003%
38	6.523	1699	1705	1708	rBV4	923	936	0.06%	0.007%
39	6.555	1713	1715	1721	rVB3	642	615	0.04%	0.005%
40	6.580	1721	1723	1724	rBV2	731	324	0.02%	0.003%
41	6.715	1761	1765	1770	rBV2	607	652	0.04%	0.005%
42	6.934	1829	1833	1838	rBV3	784	814	0.05%	0.006%
43	6.989	1839	1850	1871	rBV	209634	380035	23.20%	2.950%
44	7.207	1912	1918	1919	rBV3	498	518	0.03%	0.004%
45	7.320	1941	1953	1971	rBV	802731	1354673	82.71%	10.516%
46	7.625	2036	2048	2069	rBV	153064	266111	16.25%	2.066%
47	7.802	2100	2103	2104	rBV3	969	608	0.04%	0.005%
48	7.841	2110	2115	2116	rBV	948	565	0.03%	0.004%
49	7.895	2130	2132	2136	rBV2	527	366	0.02%	0.003%
50	7.947	2138	2148	2156	rVB4	3096	6185	0.38%	0.048%
51	8.095	2183	2194	2233	rBV	365799	663810	40.53%	5.153%
52	8.481	2309	2314	2318	rBV2	863	971	0.06%	0.008%
53	8.503	2319	2321	2324	rVV2	653	366	0.02%	0.003%
54	8.667	2367	2372	2377	rBV2	756	682	0.04%	0.005%
55	8.770	2402	2404	2408	rVB	635	336	0.02%	0.003%
56	8.789	2408	2410	2415	rBV2	465	473	0.03%	0.004%
57	8.857	2419	2431	2450	rBV	816242	1323483	80.80%	10.274%
58	9.088	2501	2503	2508	rBV3	587	515	0.03%	0.004%
59	9.381	2591	2594	2599	rVB2	451	342	0.02%	0.003%
60	9.548	2642	2646	2647	rBV	836	555	0.03%	0.004%
61	9.661	2677	2681	2683	rBV2	521	384	0.02%	0.003%
62	9.828	2730	2733	2736	rBV3	594	548	0.03%	0.004%
63	10.024	2792	2794	2799	rVB2	432	356	0.02%	0.003%
64	10.059	2804	2805	2810	rVB2	642	324	0.02%	0.003%
65	10.091	2810	2815	2817	rBV2	531	476	0.03%	0.004%
66	10.130	2821	2827	2838	rVB6	3366	4568	0.28%	0.035%
67	10.220	2844	2855	2883	rVB	564049	880253	53.74%	6.833%
68	10.329	2883	2889	2892	rBV2	1166	1115	0.07%	0.009%
69	10.352	2892	2896	2899	rVV3	809	689	0.04%	0.005%
70	10.391	2899	2908	2918	rVB4	3426	5899	0.36%	0.046%
71	10.506	2942	2944	2947	rVB2	740	353	0.02%	0.003%
72	10.526	2947	2950	2951	rBV	473	286	0.02%	0.002%
73	10.577	2962	2966	2969	rBV3	679	699	0.04%	0.005%
74	10.612	2974	2977	2986	rVB4	699	740	0.05%	0.006%
75	10.828	3042	3044	3050	rBV3	378	347	0.02%	0.003%
76	10.863	3052	3055	3057	rVB	651	384	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021041.D
 Acq On : 16 Apr 2021 12:41
 Operator : SY/MD
 Sample : M2031-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.924	3067	3074	3083	rVB7	3237	4183	0.26%	0.032%
78	11.149	3140	3144	3147	rBV3	1197	1184	0.07%	0.009%
79	11.255	3165	3177	3195	rBV	809330	1249670	76.29%	9.701%
80	11.481	3243	3247	3249	rBV2	564	461	0.03%	0.004%
81	11.542	3257	3266	3279	rBV5	7779	14608	0.89%	0.113%
82	11.632	3282	3294	3315	rBV	874444	1365126	83.34%	10.598%
83	11.857	3361	3364	3367	rBV3	831	614	0.04%	0.005%
84	11.918	3379	3383	3391	rBV	488	745	0.05%	0.006%
85	12.255	3481	3488	3490	rBV5	1424	1677	0.10%	0.013%
86	12.326	3507	3510	3514	rBV3	790	626	0.04%	0.005%
87	12.407	3530	3535	3538	rBV2	489	512	0.03%	0.004%
88	12.535	3569	3575	3576	rBV3	637	562	0.03%	0.004%
89	12.722	3632	3633	3636	rBV	526	330	0.02%	0.003%
90	12.831	3664	3667	3671	rVB2	885	609	0.04%	0.005%
91	12.886	3680	3684	3686	rBV	495	403	0.02%	0.003%
92	13.053	3733	3736	3738	rBV3	686	380	0.02%	0.003%
93	13.268	3801	3803	3805	rBV2	946	485	0.03%	0.004%
94	13.310	3814	3816	3818	rBV	496	285	0.02%	0.002%
95	13.361	3829	3832	3834	rBV	585	425	0.03%	0.003%
96	13.435	3850	3855	3858	rBV2	648	746	0.05%	0.006%
97	13.657	3920	3924	3927	rBV	770	514	0.03%	0.004%
98	13.680	3930	3931	3934	rVB2	653	338	0.02%	0.003%
99	14.365	4142	4144	4146	rBV2	628	338	0.02%	0.003%
100	14.812	4281	4283	4285	rBV	698	311	0.02%	0.002%




Sum of corrected areas: 12881487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021041.D
Acq On : 16 Apr 2021 12:41
Operator : SY/MD
Sample : M2031-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

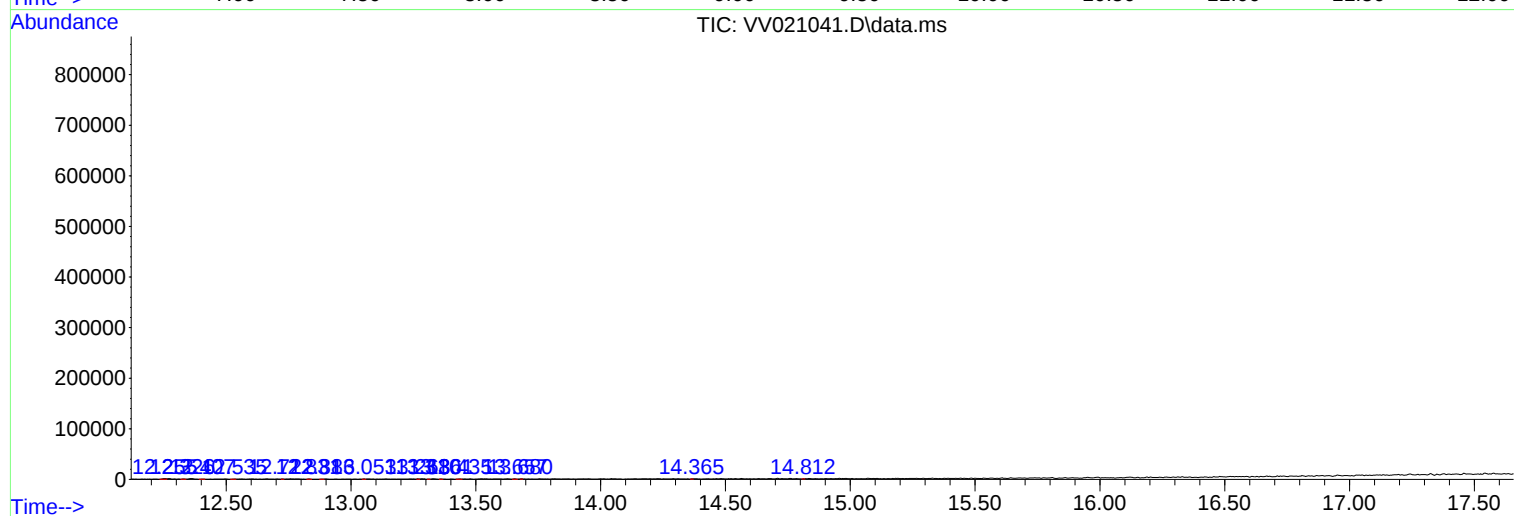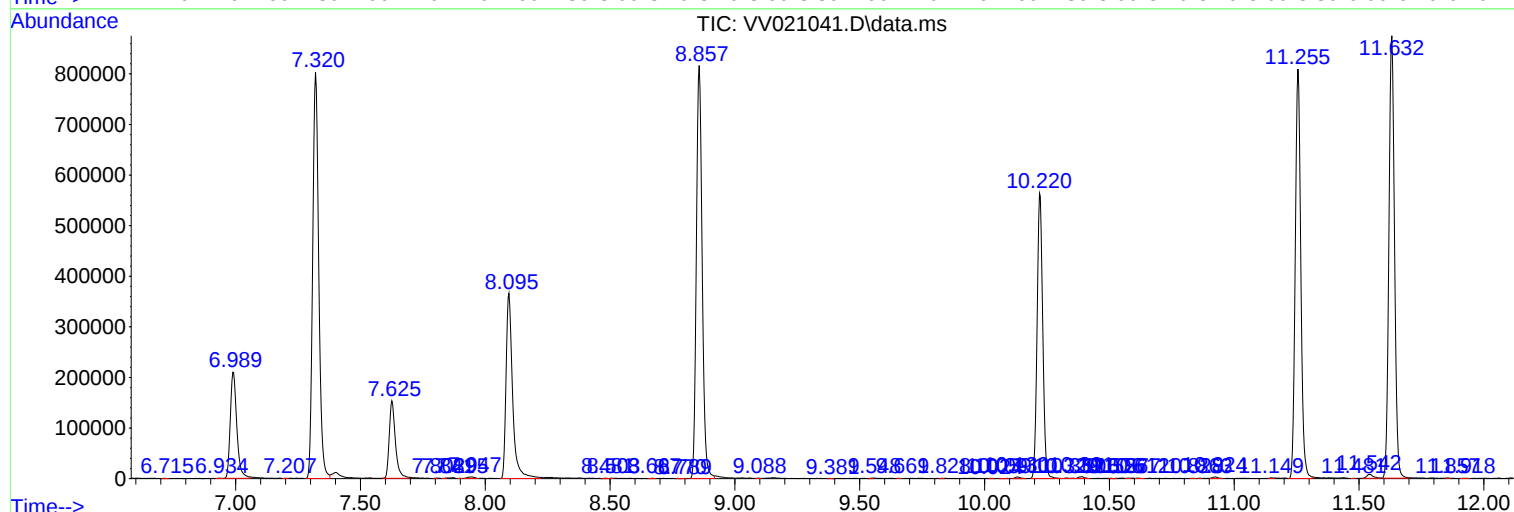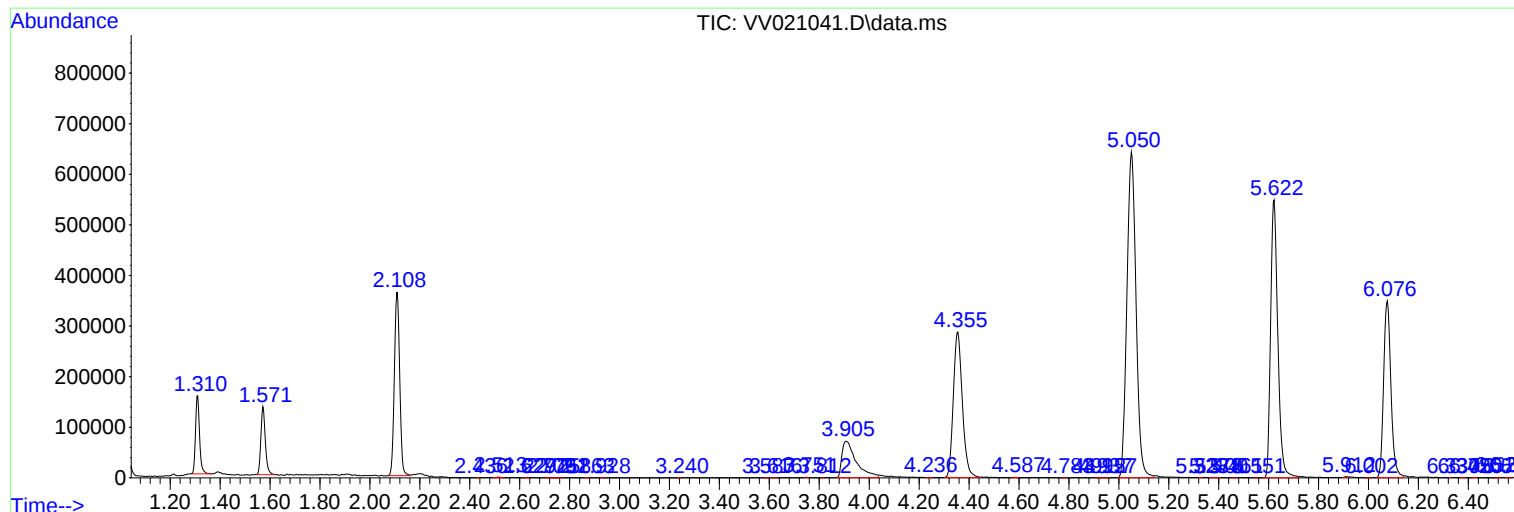

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021041.D
Acq On : 16 Apr 2021 12:41
Operator : SY/MD
Sample : M2031-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021041.D
Acq On : 16 Apr 2021 12:41
Operator : SY/MD
Sample : M2031-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
