

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021042.D
 Acq On : 16 Apr 2021 13:04
 Operator : SY/MD
 Sample : M2031-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG545

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	96	rBV	151758	168463	10.62%	1.365%
2	1.571	159	165	184	rVB	132811	167714	10.58%	1.358%
3	2.111	322	333	352	rBV	352043	522473	32.95%	4.232%
4	2.410	423	426	428	rBV	405	231	0.01%	0.002%
5	2.600	483	485	490	rBV3	326	338	0.02%	0.003%
6	2.748	529	531	534	rVB2	553	302	0.02%	0.002%
7	2.873	567	570	574	rBV2	601	451	0.03%	0.004%
8	3.082	631	635	637	rBV2	352	258	0.02%	0.002%
9	3.137	647	652	654	rBV2	373	336	0.02%	0.003%
10	3.204	669	673	675	rBV	464	399	0.03%	0.003%
11	3.346	713	717	719	rVB2	429	218	0.01%	0.002%
12	3.416	735	739	740	rBV	461	323	0.02%	0.003%
13	3.426	740	742	746	rVB2	725	419	0.03%	0.003%
14	3.474	753	757	758	rBV2	372	325	0.02%	0.003%
15	3.613	797	800	803	rVB	528	329	0.02%	0.003%
16	3.632	803	806	809	rBV2	456	278	0.02%	0.002%
17	3.725	832	835	836	rBV	487	231	0.01%	0.002%
18	3.767	846	848	854	rVB3	969	618	0.04%	0.005%
19	3.912	877	893	921	rBV	73514	269842	17.02%	2.186%
20	4.355	1014	1031	1057	rBV	280346	711312	44.85%	5.762%
21	4.539	1084	1088	1094	rVB4	615	681	0.04%	0.006%
22	4.606	1107	1109	1111	rVB2	846	362	0.02%	0.003%
23	4.706	1136	1140	1143	rBV3	691	546	0.03%	0.004%
24	4.831	1177	1179	1184	rBV	315	310	0.02%	0.003%
25	4.966	1219	1221	1224	rBV	323	237	0.01%	0.002%
26	5.050	1231	1247	1276	rBV2	619127	1585831	100.00%	12.845%
27	5.307	1325	1327	1334	rVB3	730	513	0.03%	0.004%
28	5.397	1352	1355	1356	rBV2	531	220	0.01%	0.002%
29	5.532	1391	1397	1401	rBV3	549	655	0.04%	0.005%
30	5.622	1413	1425	1448	rBV	502644	997511	62.90%	8.080%
31	5.876	1502	1504	1507	rBV3	396	218	0.01%	0.002%
32	6.075	1553	1566	1590	rBV	341443	687935	43.38%	5.572%
33	6.262	1620	1624	1629	rVB6	1163	983	0.06%	0.008%
34	6.304	1635	1637	1640	rVB3	690	359	0.02%	0.003%
35	6.326	1641	1644	1645	rBV	710	308	0.02%	0.002%
36	6.336	1645	1647	1654	rVB4	723	721	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021042.D
 Acq On : 16 Apr 2021 13:04
 Operator : SY/MD
 Sample : M2031-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 BG545

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1667	rVB4	773	483	0.03%	0.004%
38	6.490	1692	1695	1698	rBV2	726	618	0.04%	0.005%
39	6.561	1714	1717	1721	rBV3	602	495	0.03%	0.004%
40	6.657	1743	1747	1751	rVB2	450	308	0.02%	0.002%
41	6.690	1754	1757	1758	rBV2	485	305	0.02%	0.002%
42	6.770	1779	1782	1785	rBV2	500	369	0.02%	0.003%
43	6.873	1808	1814	1816	rBV	259	306	0.02%	0.002%
44	6.902	1821	1823	1826	rVB2	566	267	0.02%	0.002%
45	6.940	1829	1835	1839	rBV2	814	841	0.05%	0.007%
46	6.992	1839	1851	1867	rBV2	203481	367835	23.20%	2.979%
47	7.153	1899	1901	1905	rVB4	894	490	0.03%	0.004%
48	7.233	1921	1926	1929	rVB5	547	486	0.03%	0.004%
49	7.252	1929	1932	1937	rVB3	707	471	0.03%	0.004%
50	7.320	1941	1953	1971	rBV	752146	1306115	82.36%	10.579%
51	7.625	2037	2048	2071	rBV	146966	260024	16.40%	2.106%
52	7.773	2092	2094	2096	rBV2	605	349	0.02%	0.003%
53	7.944	2138	2147	2148	rBV3	3918	4515	0.28%	0.037%
54	8.050	2178	2180	2184	rBV	727	376	0.02%	0.003%
55	8.095	2184	2194	2224	rBV	376214	683775	43.12%	5.538%
56	8.403	2286	2290	2295	rVB4	605	558	0.04%	0.005%
57	8.429	2295	2298	2301	rBV	432	252	0.02%	0.002%
58	8.448	2301	2304	2308	rVB2	528	379	0.02%	0.003%
59	8.603	2350	2352	2353	rBV	481	214	0.01%	0.002%
60	8.760	2399	2401	2404	rVB	623	315	0.02%	0.003%
61	8.792	2406	2411	2415	rBV2	396	326	0.02%	0.003%
62	8.857	2419	2431	2458	rBV	750320	1213767	76.54%	9.831%
63	9.236	2547	2549	2551	rBV	456	250	0.02%	0.002%
64	9.397	2594	2599	2601	rBV2	420	379	0.02%	0.003%
65	9.474	2619	2623	2626	rBV2	442	416	0.03%	0.003%
66	9.545	2639	2645	2646	rBV	405	374	0.02%	0.003%
67	9.677	2683	2686	2688	rBV2	485	226	0.01%	0.002%
68	9.693	2688	2691	2692	rBV	360	215	0.01%	0.002%
69	9.924	2760	2763	2764	rBV2	452	221	0.01%	0.002%
70	9.988	2779	2783	2785	rBV	451	381	0.02%	0.003%
71	10.056	2801	2804	2806	rBV	427	283	0.02%	0.002%
72	10.133	2818	2828	2837	rBV7	3475	5268	0.33%	0.043%
73	10.223	2843	2856	2878	rBV	561739	878296	55.38%	7.114%
74	10.554	2956	2959	2962	rVB	1049	648	0.04%	0.005%
75	10.580	2962	2967	2968	rBV3	988	862	0.05%	0.007%
76	10.677	2996	2997	3002	rBV2	365	305	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021042.D
 Acq On : 16 Apr 2021 13:04
 Operator : SY/MD
 Sample : M2031-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG545

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.718	3006	3010	3012	rBV	449	336	0.02%	0.003%
78	10.747	3017	3019	3021	rBV	709	292	0.02%	0.002%
79	10.786	3025	3031	3033	rBV2	560	519	0.03%	0.004%
80	10.818	3038	3041	3044	rVB	530	291	0.02%	0.002%
81	10.860	3051	3054	3057	rVV2	885	514	0.03%	0.004%
82	11.046	3106	3112	3115	rBV3	833	957	0.06%	0.008%
83	11.149	3139	3144	3150	rBV4	1546	1886	0.12%	0.015%
84	11.191	3155	3157	3162	rVB3	743	450	0.03%	0.004%
85	11.255	3166	3177	3201	rBV	736298	1158548	73.06%	9.384%
86	11.631	3282	3294	3311	rBV	842341	1320484	83.27%	10.696%
87	11.840	3356	3359	3364	rBV3	656	573	0.04%	0.005%
88	11.988	3403	3405	3407	rBV	573	400	0.03%	0.003%
89	12.657	3610	3613	3619	rBV2	1175	1048	0.07%	0.008%
90	12.975	3710	3712	3715	rBV3	645	443	0.03%	0.004%
91	13.082	3741	3745	3747	rBV2	812	606	0.04%	0.005%
92	13.130	3757	3760	3763	rBV3	671	550	0.03%	0.004%
93	13.371	3833	3835	3837	rBV	470	243	0.02%	0.002%
94	13.487	3869	3871	3873	rBV	567	346	0.02%	0.003%
95	13.644	3918	3920	3923	rBV3	502	338	0.02%	0.003%
96	14.030	4037	4040	4042	rBV	631	368	0.02%	0.003%
97	14.139	4071	4074	4077	rBV2	757	501	0.03%	0.004%
98	14.194	4087	4091	4093	rBV2	652	506	0.03%	0.004%
99	14.496	4183	4185	4188	rVB2	937	492	0.03%	0.004%
100	15.159	4389	4391	4394	rBV2	985	576	0.04%	0.005%




Sum of corrected areas: 12345880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021042.D
Acq On : 16 Apr 2021 13:04
Operator : SY/MD
Sample : M2031-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG545

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

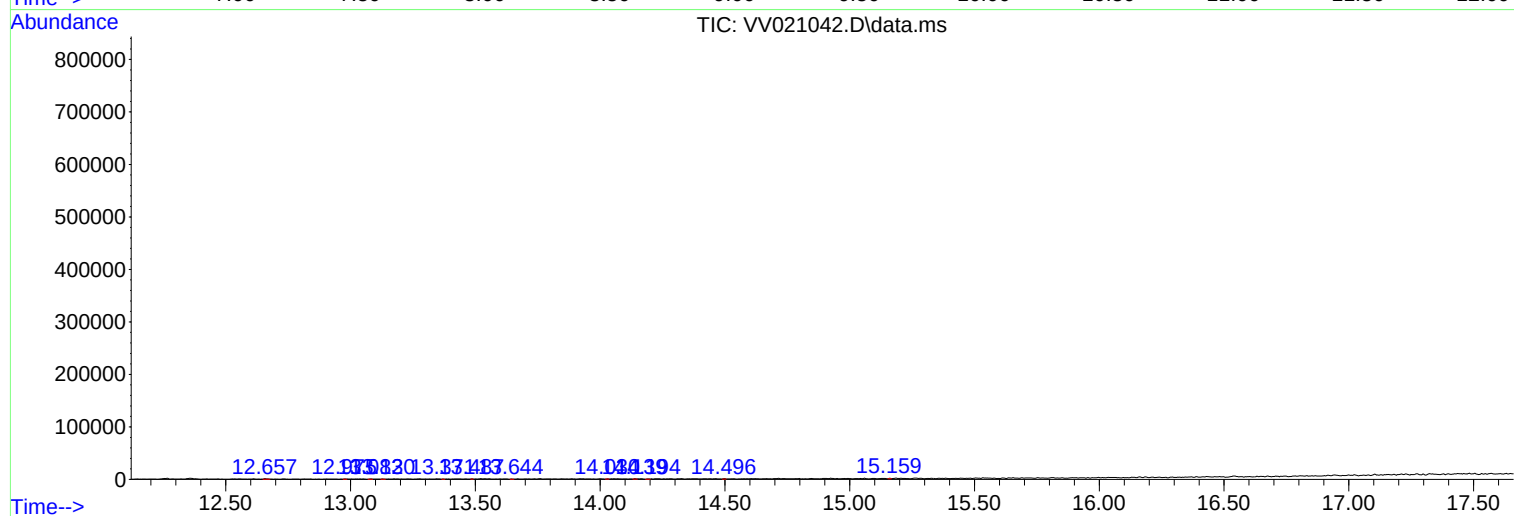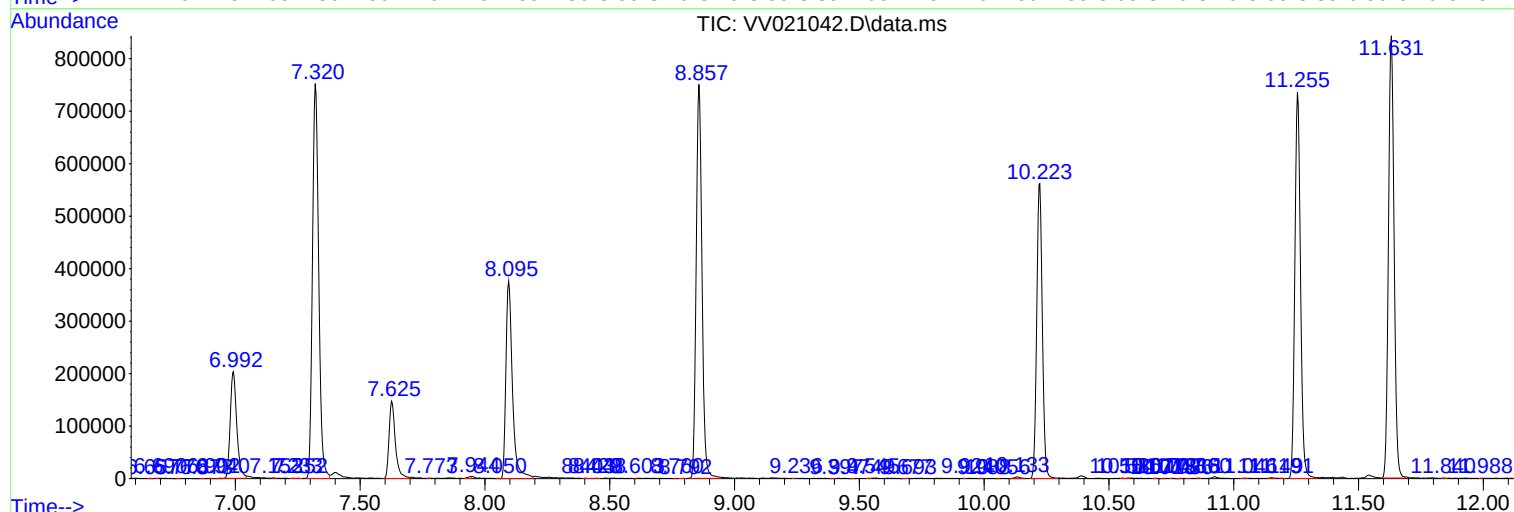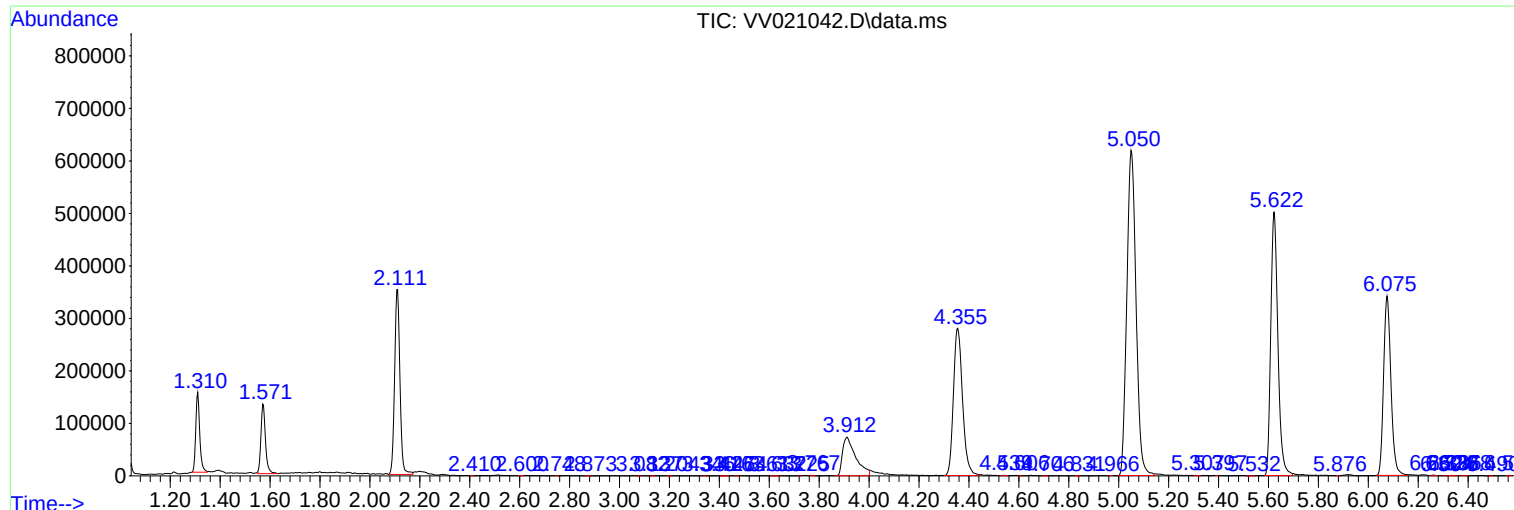

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021042.D
Acq On : 16 Apr 2021 13:04
Operator : SY/MD
Sample : M2031-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG545

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021042.D
Acq On : 16 Apr 2021 13:04
Operator : SY/MD
Sample : M2031-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG545

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
