

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041621\
 Data File : VW021045.D
 Acq On : 16 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2067-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG798

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VW021045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	32	rVB3	10577	10398	0.68%	0.085%
2	1.307	76	83	93	rBV	152656	164904	10.81%	1.343%
3	1.571	158	165	180	rVB	127525	156998	10.29%	1.279%
4	2.108	323	332	344	rBV	336058	469425	30.78%	3.824%
5	2.346	403	406	408	rBV	552	258	0.02%	0.002%
6	2.388	415	419	420	rBV2	525	303	0.02%	0.002%
7	2.449	435	438	439	rBV	575	295	0.02%	0.002%
8	2.555	469	471	475	rBV	389	304	0.02%	0.002%
9	2.638	494	497	501	rVB2	625	357	0.02%	0.003%
10	2.770	530	538	541	rBV3	929	1041	0.07%	0.008%
11	2.838	554	559	560	rBV	364	243	0.02%	0.002%
12	2.880	566	572	577	rVB2	400	548	0.04%	0.004%
13	3.047	615	624	625	rBV3	1165	1424	0.09%	0.012%
14	3.127	642	649	653	rVB2	452	450	0.03%	0.004%
15	3.166	659	661	667	rVB2	355	335	0.02%	0.003%
16	3.198	667	671	672	rBV	406	285	0.02%	0.002%
17	3.240	681	684	686	rBV	570	316	0.02%	0.003%
18	3.359	719	721	724	rVB2	741	330	0.02%	0.003%
19	3.397	729	733	738	rVV	307	320	0.02%	0.003%
20	3.487	757	761	764	rBV	393	256	0.02%	0.002%
21	3.606	795	798	800	rBV	479	332	0.02%	0.003%
22	3.626	800	804	807	rVB	377	266	0.02%	0.002%
23	3.655	810	813	817	rBV2	422	427	0.03%	0.003%
24	3.767	843	848	850	rBV2	459	410	0.03%	0.003%
25	3.909	880	892	935	rBV2	71525	269292	17.66%	2.194%
26	4.208	983	985	988	rBV2	651	377	0.02%	0.003%
27	4.352	1015	1030	1058	rBV	265933	680858	44.64%	5.547%
28	5.050	1230	1247	1283	rBV2	580275	1525105	100.00%	12.425%
29	5.365	1340	1345	1348	rBV2	636	669	0.04%	0.005%
30	5.429	1362	1365	1368	rVB3	665	441	0.03%	0.004%
31	5.487	1381	1383	1385	rBV2	437	246	0.02%	0.002%
32	5.571	1405	1409	1412	rBV2	473	405	0.03%	0.003%
33	5.622	1412	1425	1453	rBV	528326	1060347	69.53%	8.638%
34	5.822	1485	1487	1488	rBV	617	244	0.02%	0.002%
35	5.876	1500	1504	1508	rBV3	896	936	0.06%	0.008%
36	5.973	1529	1534	1541	rBV3	436	648	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021045.D
 Acq On : 16 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2067-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG798

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.005	1541	1544	1548	rVB	637	482	0.03%	0.004%
38	6.072	1552	1565	1595	rBV	321216	671684	44.04%	5.472%
39	6.317	1637	1641	1643	rBV2	470	357	0.02%	0.003%
40	6.365	1653	1656	1657	rBV2	816	464	0.03%	0.004%
41	6.474	1688	1690	1695	rVB2	410	256	0.02%	0.002%
42	6.519	1700	1704	1705	rBV	399	274	0.02%	0.002%
43	6.548	1710	1713	1717	rVB2	438	315	0.02%	0.003%
44	6.577	1718	1722	1725	rBV	506	394	0.03%	0.003%
45	6.619	1733	1735	1740	rVB3	545	413	0.03%	0.003%
46	6.645	1740	1743	1744	rBV	460	273	0.02%	0.002%
47	6.748	1772	1775	1777	rBV2	558	352	0.02%	0.003%
48	6.770	1780	1782	1785	rVV3	516	320	0.02%	0.003%
49	6.834	1798	1802	1805	rVB3	277	254	0.02%	0.002%
50	6.989	1837	1850	1874	rBV2	197147	360351	23.63%	2.936%
51	7.172	1905	1907	1910	rVB2	695	334	0.02%	0.003%
52	7.259	1931	1934	1938	rBV3	916	747	0.05%	0.006%
53	7.320	1942	1953	1970	rBV	714835	1234512	80.95%	10.057%
54	7.625	2038	2048	2077	rVV	142566	250371	16.42%	2.040%
55	7.944	2136	2147	2160	rBV2	21928	39647	2.60%	0.323%
56	8.095	2183	2194	2232	rBV	348087	640486	42.00%	5.218%
57	8.352	2271	2274	2276	rBV2	702	430	0.03%	0.004%
58	8.371	2277	2280	2282	rBV2	703	495	0.03%	0.004%
59	8.510	2318	2323	2324	rBV2	599	491	0.03%	0.004%
60	8.709	2383	2385	2387	rBV	402	246	0.02%	0.002%
61	8.802	2412	2414	2418	rBV2	379	258	0.02%	0.002%
62	8.857	2418	2431	2455	rBV	791788	1285664	84.30%	10.474%
63	9.056	2491	2493	2495	rBV2	613	290	0.02%	0.002%
64	9.140	2516	2519	2520	rBV2	686	306	0.02%	0.002%
65	9.198	2535	2537	2539	rBV	577	246	0.02%	0.002%
66	9.249	2551	2553	2556	rBV	496	410	0.03%	0.003%
67	9.722	2698	2700	2705	rVB2	407	265	0.02%	0.002%
68	9.895	2752	2754	2759	rVB	734	540	0.04%	0.004%
69	9.924	2759	2763	2765	rBV	432	344	0.02%	0.003%
70	9.937	2765	2767	2770	rBV2	424	353	0.02%	0.003%
71	10.037	2794	2798	2799	rBV2	443	277	0.02%	0.002%
72	10.137	2821	2829	2836	rBV4	2235	3238	0.21%	0.026%
73	10.223	2843	2856	2877	rBV	544804	846601	55.51%	6.897%
74	10.387	2896	2907	2919	rVB2	26656	43147	2.83%	0.352%
75	10.638	2982	2985	2986	rBV	410	248	0.02%	0.002%
76	10.786	3029	3031	3033	rBV	380	251	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021045.D
 Acq On : 16 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2067-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG798

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.860	3046	3054	3059	rBV4	801	1098	0.07%	0.009%
78	10.924	3067	3074	3082	rBV6	2651	3484	0.23%	0.028%
79	11.130	3132	3138	3140	rBV2	689	769	0.05%	0.006%
80	11.149	3140	3144	3149	rBV4	1112	1439	0.09%	0.012%
81	11.256	3165	3177	3201	rBV	795721	1222314	80.15%	9.958%
82	11.384	3215	3217	3220	rBV2	847	703	0.05%	0.006%
83	11.419	3226	3228	3231	rBV2	877	579	0.04%	0.005%
84	11.500	3247	3253	3255	rBV3	933	726	0.05%	0.006%
85	11.538	3262	3265	3267	rBV	751	485	0.03%	0.004%
86	11.632	3281	3294	3318	rBV	821186	1286956	84.38%	10.484%
87	11.780	3338	3340	3344	rVB2	546	316	0.02%	0.003%
88	11.847	3358	3361	3364	rBV2	704	510	0.03%	0.004%
89	12.059	3425	3427	3431	rBV2	464	301	0.02%	0.002%
90	12.127	3444	3448	3454	rBV2	640	503	0.03%	0.004%
91	12.259	3477	3489	3502	rBV2	6956	11589	0.76%	0.094%
92	12.365	3515	3522	3525	rVV5	1428	2048	0.13%	0.017%
93	12.468	3551	3554	3559	rBV2	638	408	0.03%	0.003%
94	12.702	3623	3627	3632	rBV3	589	487	0.03%	0.004%
95	12.921	3693	3695	3700	rVB2	557	321	0.02%	0.003%
96	13.535	3883	3886	3889	rBV2	1009	851	0.06%	0.007%
97	13.696	3934	3936	3938	rBV	743	395	0.03%	0.003%
98	13.944	4007	4013	4019	rBV4	1115	1501	0.10%	0.012%
99	14.300	4122	4124	4126	rBV	706	352	0.02%	0.003%
100	15.053	4356	4358	4360	rBV3	1113	626	0.04%	0.005%




Sum of corrected areas: 12274940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021045.D
Acq On : 16 Apr 2021 14:15
Operator : SY/MD
Sample : M2067-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG798

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

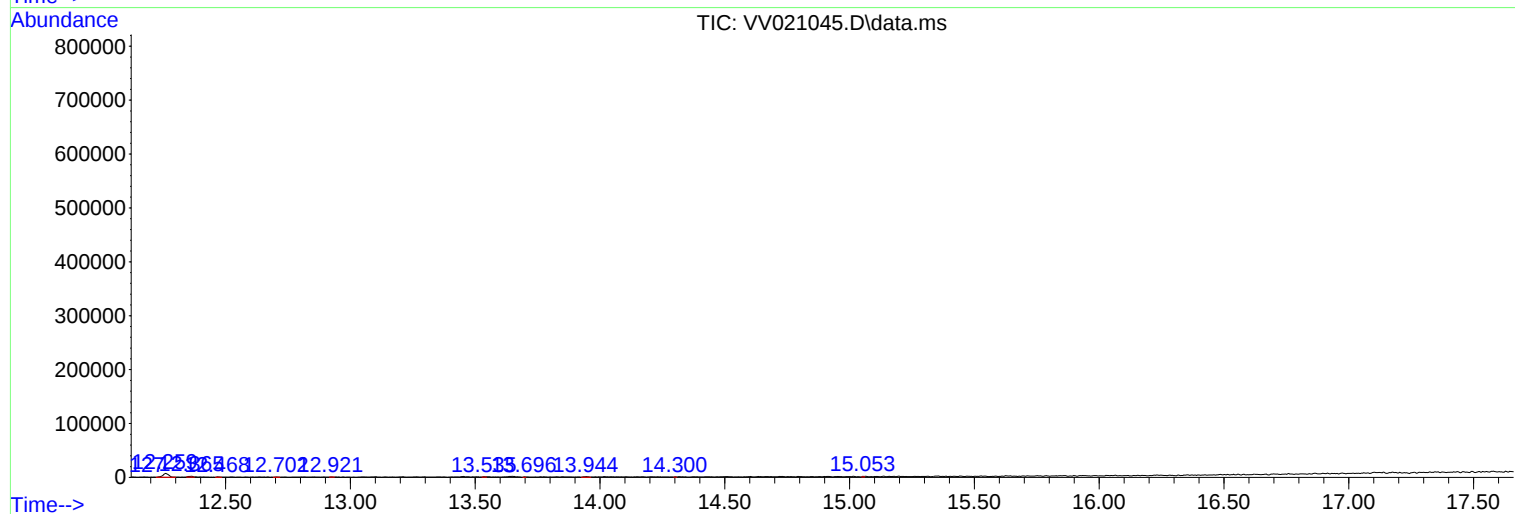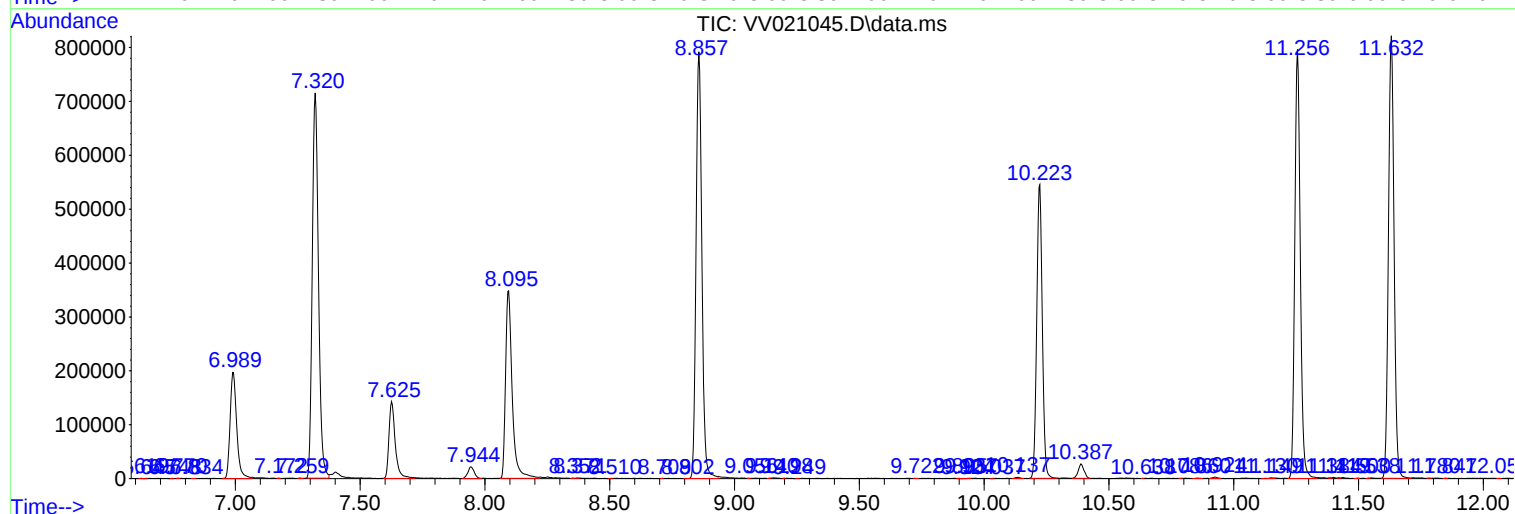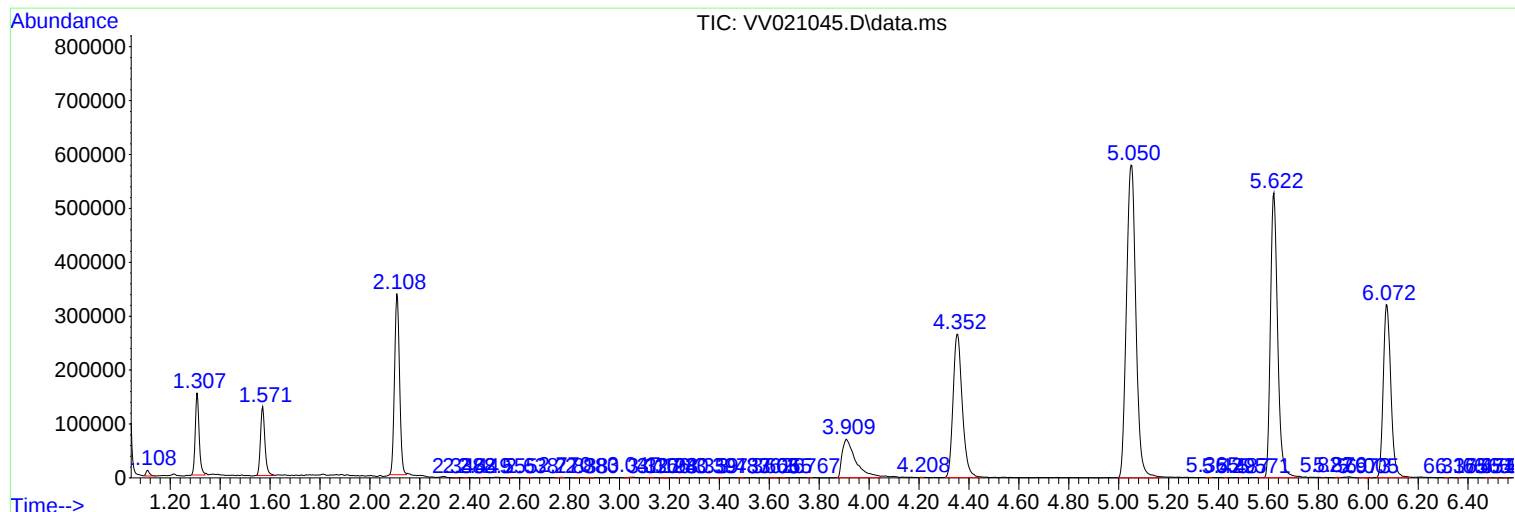

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021045.D
Acq On : 16 Apr 2021 14:15
Operator : SY/MD
Sample : M2067-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG798

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021045.D
Acq On : 16 Apr 2021 14:15
Operator : SY/MD
Sample : M2067-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG798

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
