

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021048.D
 Acq On : 16 Apr 2021 15:39
 Operator : SY/MD
 Sample : VIBLK23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	47	54	70	rBV	370233	409156	25.64%	3.206%
2	1.311	78	84	105	rVB	108038	153149	9.60%	1.200%
3	1.571	159	165	190	rVB	88380	154195	9.66%	1.208%
4	2.098	321	329	348	rVB	346766	488397	30.61%	3.827%
5	2.622	479	492	507	rBV	8924	20360	1.28%	0.160%
6	2.709	514	519	524	rVB4	1137	1234	0.08%	0.010%
7	2.835	555	558	565	rVB2	690	490	0.03%	0.004%
8	2.867	565	568	573	rBV2	370	337	0.02%	0.003%
9	2.889	573	575	578	rBV	571	301	0.02%	0.002%
10	2.928	584	587	590	rVB	593	339	0.02%	0.003%
11	3.034	610	620	630	rBV6	2816	5599	0.35%	0.044%
12	3.182	664	666	673	rVB3	800	726	0.05%	0.006%
13	3.227	678	680	683	rVB2	592	257	0.02%	0.002%
14	3.471	752	756	758	rBV2	410	294	0.02%	0.002%
15	3.529	770	774	776	rBV2	592	494	0.03%	0.004%
16	3.677	818	820	823	rBV2	390	304	0.02%	0.002%
17	3.738	834	839	840	rBV2	521	438	0.03%	0.003%
18	3.793	853	856	860	rBV2	431	273	0.02%	0.002%
19	3.918	883	895	937	rBV2	59180	270739	16.97%	2.122%
20	4.349	1013	1029	1057	rBV2	281013	705914	44.24%	5.532%
21	4.552	1088	1092	1093	rBV2	519	355	0.02%	0.003%
22	4.619	1110	1113	1117	rBV3	605	380	0.02%	0.003%
23	4.658	1119	1125	1129	rVV4	556	699	0.04%	0.005%
24	4.751	1151	1154	1155	rBV	556	299	0.02%	0.002%
25	4.863	1185	1189	1191	rBV	700	517	0.03%	0.004%
26	4.912	1201	1204	1206	rBV	705	477	0.03%	0.004%
27	4.966	1218	1221	1222	rBV	479	291	0.02%	0.002%
28	5.043	1229	1245	1271	rBV2	634724	1595732	100.00%	12.505%
29	5.513	1387	1391	1393	rVV2	520	320	0.02%	0.003%
30	5.616	1411	1423	1448	rBV	475132	976987	61.23%	7.656%
31	5.921	1504	1518	1535	rBV4	45573	100866	6.32%	0.790%
32	6.069	1552	1564	1591	rBV2	340473	702827	44.04%	5.508%
33	6.198	1602	1604	1605	rBV2	768	382	0.02%	0.003%
34	6.336	1644	1647	1650	rBV2	556	390	0.02%	0.003%
35	6.384	1659	1662	1665	rVB2	564	292	0.02%	0.002%
36	6.404	1665	1668	1673	rVB3	1087	715	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021048.D
 Acq On : 16 Apr 2021 15:39
 Operator : SY/MD
 Sample : VIBLK23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.590	1722	1726	1728	rBV3	630	516	0.03%	0.004%
38	6.703	1759	1761	1764	rVB2	609	291	0.02%	0.002%
39	6.738	1767	1772	1773	rBV	412	289	0.02%	0.002%
40	6.780	1781	1785	1790	rBV2	486	503	0.03%	0.004%
41	6.812	1790	1795	1799	rVB2	522	499	0.03%	0.004%
42	6.912	1823	1826	1831	rVB2	443	405	0.03%	0.003%
43	6.934	1831	1833	1834	rBV	600	272	0.02%	0.002%
44	6.989	1838	1850	1881	rBV2	197220	373978	23.44%	2.931%
45	7.207	1915	1918	1920	rBV3	701	354	0.02%	0.003%
46	7.317	1941	1952	1971	rBV	694909	1238931	77.64%	9.709%
47	7.574	2029	2032	2036	rVB3	372	264	0.02%	0.002%
48	7.625	2038	2048	2066	rBV	134114	255268	16.00%	2.000%
49	7.940	2144	2146	2147	rBV	762	389	0.02%	0.003%
50	7.979	2147	2158	2173	rBV2	161882	284771	17.85%	2.232%
51	8.117	2189	2201	2231	rVB	260593	670051	41.99%	5.251%
52	8.352	2272	2274	2278	rBV3	654	423	0.03%	0.003%
53	8.410	2290	2292	2294	rBV2	748	436	0.03%	0.003%
54	8.532	2327	2330	2333	rVB	440	297	0.02%	0.002%
55	8.609	2351	2354	2356	rBV2	540	251	0.02%	0.002%
56	8.670	2366	2373	2381	rBV7	1744	2535	0.16%	0.020%
57	8.857	2419	2431	2458	rBV	668683	1191172	74.65%	9.335%
58	9.143	2517	2520	2521	rBV2	941	533	0.03%	0.004%
59	9.194	2532	2536	2545	rVB4	1017	1064	0.07%	0.008%
60	9.246	2550	2552	2556	rBV2	526	349	0.02%	0.003%
61	9.349	2581	2584	2586	rBV2	417	263	0.02%	0.002%
62	9.381	2591	2594	2596	rBV	650	360	0.02%	0.003%
63	9.426	2604	2608	2609	rBV3	460	308	0.02%	0.002%
64	9.484	2621	2626	2627	rBV	349	263	0.02%	0.002%
65	9.558	2645	2649	2650	rBV2	602	362	0.02%	0.003%
66	9.625	2668	2670	2674	rVB	369	253	0.02%	0.002%
67	9.696	2690	2692	2696	rVB2	663	375	0.02%	0.003%
68	9.760	2708	2712	2713	rBV2	525	303	0.02%	0.002%
69	9.825	2729	2732	2735	rVV	519	320	0.02%	0.003%
70	9.850	2735	2740	2741	rVB2	342	243	0.02%	0.002%
71	9.995	2783	2785	2788	rBV	706	376	0.02%	0.003%
72	10.024	2792	2794	2797	rBV2	513	372	0.02%	0.003%
73	10.124	2818	2825	2826	rBV4	1637	1400	0.09%	0.011%
74	10.230	2842	2858	2878	rBV	547602	891871	55.89%	6.989%
75	10.381	2903	2905	2908	rBV2	848	475	0.03%	0.004%
76	10.426	2916	2919	2923	rVB	568	309	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041621\
 Data File : VW021048.D
 Acq On : 16 Apr 2021 15:39
 Operator : SY/MD
 Sample : VIBLK23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.445	2923	2925	2927	rBV	549	256	0.02%	0.002%
78	10.458	2927	2929	2932	rVB2	406	249	0.02%	0.002%
79	10.481	2932	2936	2939	rBV2	622	486	0.03%	0.004%
80	10.587	2962	2969	2979	rVB4	9994	14675	0.92%	0.115%
81	10.648	2985	2988	2991	rBV2	415	257	0.02%	0.002%
82	10.857	3048	3053	3055	rBV3	722	699	0.04%	0.005%
83	10.924	3067	3074	3083	rBV9	2889	4175	0.26%	0.033%
84	11.149	3141	3144	3149	rVV5	1321	1318	0.08%	0.010%
85	11.191	3153	3157	3159	rBV2	554	332	0.02%	0.003%
86	11.259	3166	3178	3195	rBV	663240	1022825	64.10%	8.015%
87	11.432	3228	3232	3237	rBV5	1253	1549	0.10%	0.012%
88	11.522	3255	3260	3263	rBV2	764	589	0.04%	0.005%
89	11.635	3283	3295	3311	rBV	750036	1192446	74.73%	9.345%
90	12.014	3410	3413	3417	rBV4	640	526	0.03%	0.004%
91	12.069	3427	3430	3433	rBV4	586	424	0.03%	0.003%
92	12.304	3499	3503	3507	rBV2	502	463	0.03%	0.004%
93	12.641	3606	3608	3610	rVB2	640	290	0.02%	0.002%
94	12.667	3613	3616	3619	rBV3	613	381	0.02%	0.003%
95	12.886	3679	3684	3685	rBV	473	292	0.02%	0.002%
96	13.124	3755	3758	3762	rBV3	436	374	0.02%	0.003%
97	13.387	3836	3840	3843	rBV3	795	568	0.04%	0.004%
98	13.448	3856	3859	3862	rBV2	357	277	0.02%	0.002%
99	13.548	3887	3890	3895	rVB2	826	660	0.04%	0.005%
100	13.574	3895	3898	3901	rBV3	770	516	0.03%	0.004%


Sum of corrected areas: 12760846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021048.D
Acq On : 16 Apr 2021 15:39
Operator : SY/MD
Sample : VIBLK23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

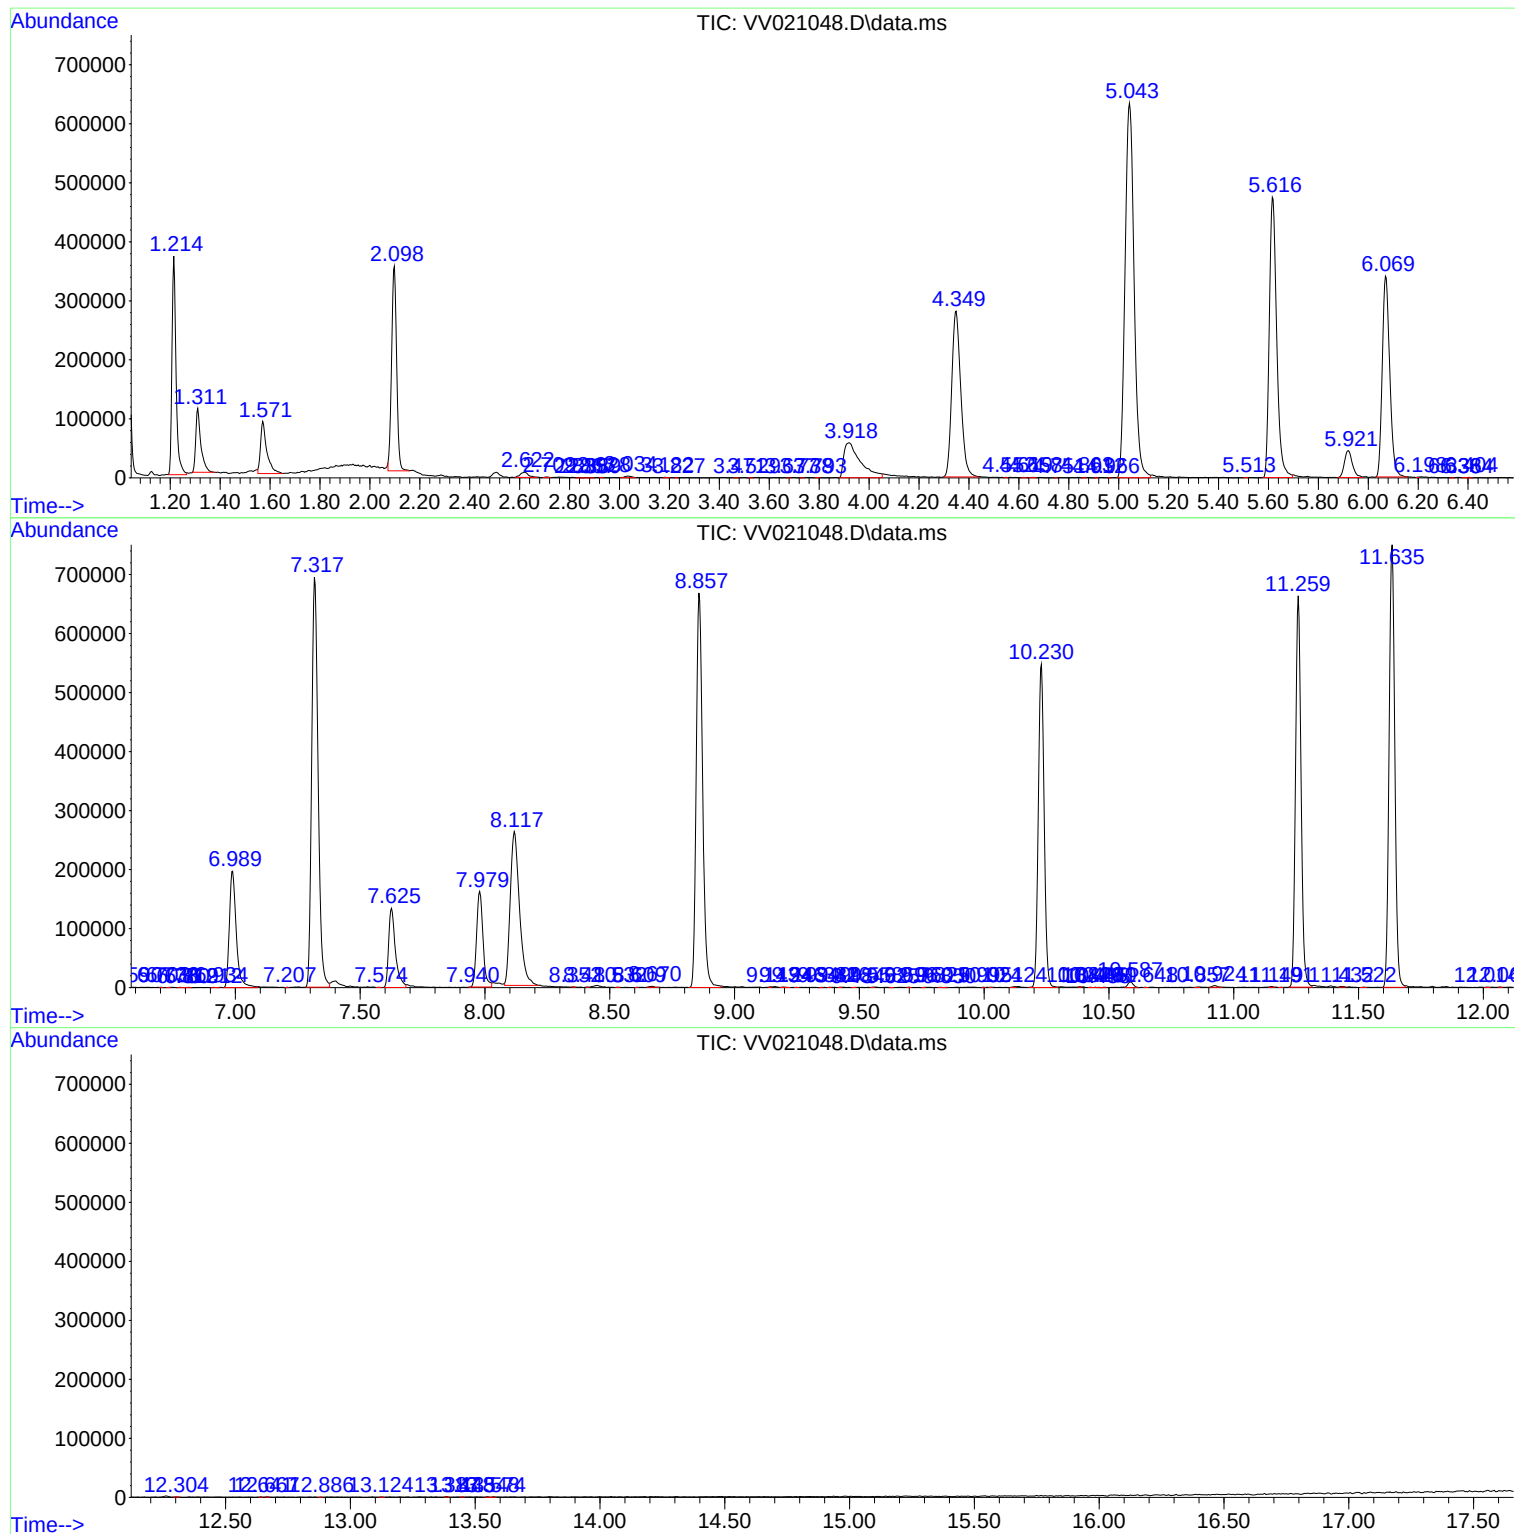

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021048.D
Acq On : 16 Apr 2021 15:39
Operator : SY/MD
Sample : VIBLK23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021048.D
Acq On : 16 Apr 2021 15:39
Operator : SY/MD
Sample : VIBLK23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
