


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021036.D
Acq On : 16 Apr 2021 09:06
Operator : SY/MD
Sample : BFB84
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB184

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Title : VOC Analysis
Last Update : Tue Apr 20 01:39:15 2021

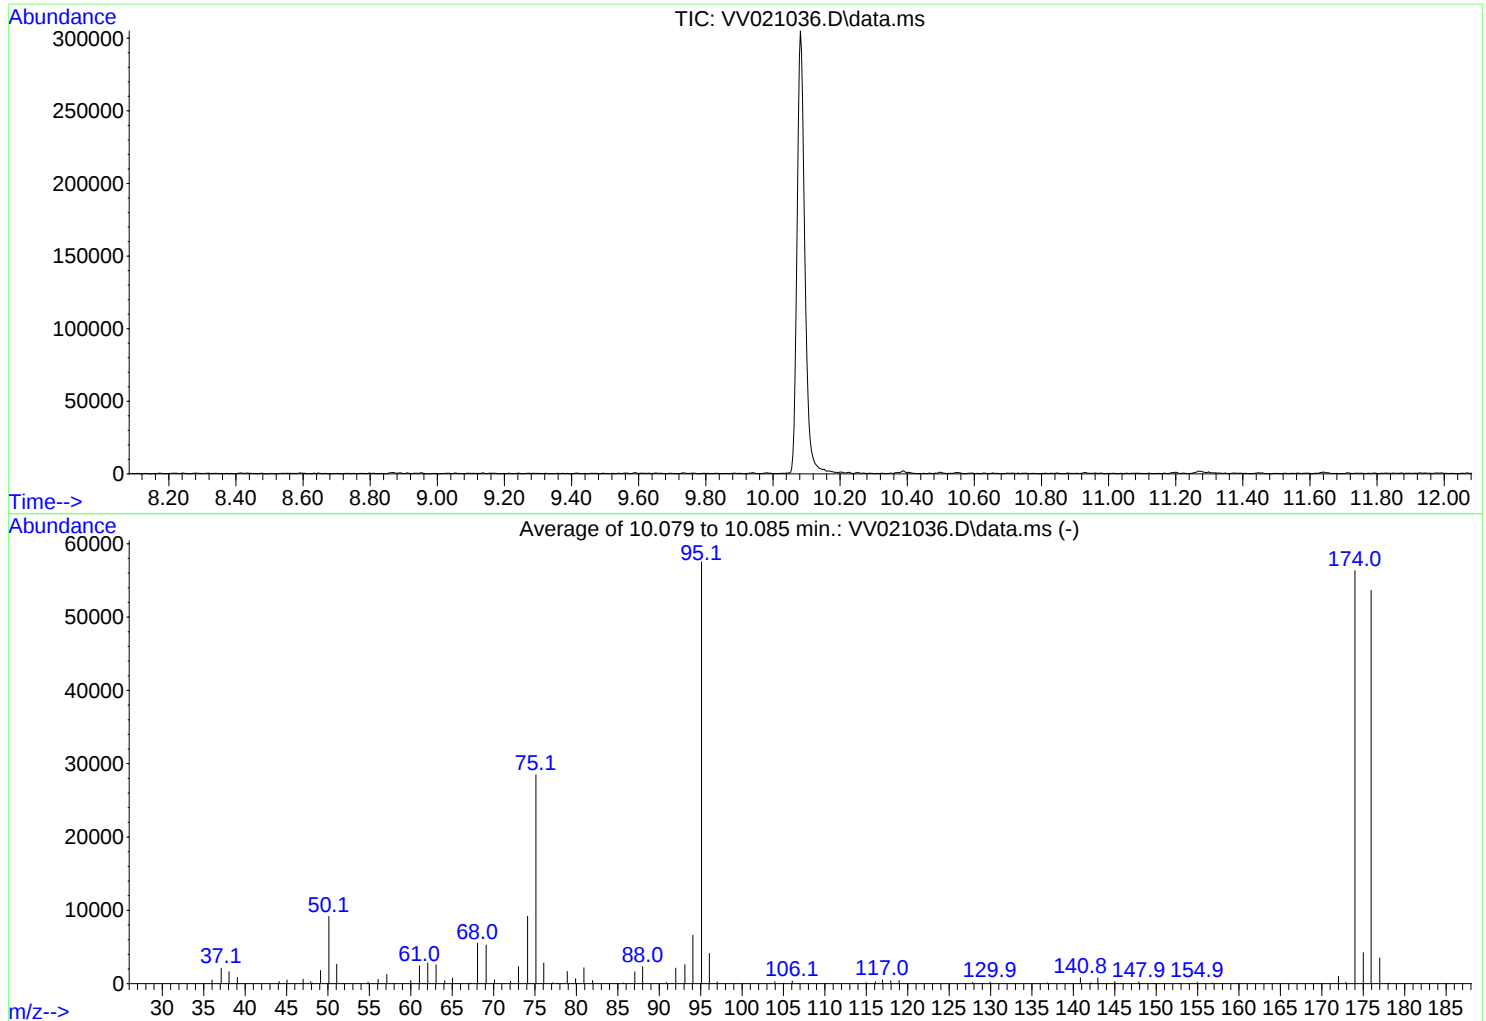

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.9	9166	PASS
75	95	30	80	49.5	28483	PASS
95	95	100	100	100.0	57533	PASS
96	95	5	9	7.2	4120	PASS
173	174	0.00	2	0.4	204	PASS
174	95	50	120	97.9	56341	PASS
175	174	5	9	7.5	4243	PASS
176	174	95	101	95.2	53657	PASS
177	176	5	9	6.5	3507	PASS

Scan 2801 (10.047 min): VV021036.D\data.ms
BFB84

m/z	Abundance
40.00	188.0
44.20	358.0
175.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB184

m/z	Abundance
36.00	459.0
37.10	2063.0
38.00	1693.0
39.00	906.0
44.00	591.0
45.10	506.0
47.00	614.0
47.90	447.0
49.10	1958.0
50.10	9187.0
51.10	2550.0
51.90	112.0
54.90	125.0
56.00	654.0
57.10	1261.0
58.00	117.0
60.00	505.0
61.10	2578.0
62.00	2748.0
63.00	2615.0
64.10	424.0
65.10	720.0
67.30	149.0
68.10	5466.0
69.10	5003.0
70.10	524.0
72.00	354.0
73.00	2262.0
74.10	9131.0
75.10	28280.0
76.00	2455.0
77.20	147.0
78.90	1559.0
79.90	688.0
80.90	2016.0
81.90	455.0
87.00	1689.0
88.00	2127.0
90.90	193.0
92.00	2243.0
93.10	2511.0
94.10	6316.0
95.10	57296.0
96.00	3958.0
97.00	257.0
103.90	232.0
106.10	349.0
115.00	206.0
116.10	205.0
116.90	515.0
118.00	373.0
118.90	411.0
127.80	227.0
128.80	109.0
130.00	251.0
136.80	114.0
140.90	794.0
142.20	138.0
142.90	645.0
145.00	427.0
147.90	262.0
149.70	104.0
152.80	118.0
154.90	161.0
172.00	929.0
172.90	613.0
174.00	53648.0
175.00	4244.0
176.00	50688.0
177.00	3601.0

Instrument :
MSVOA_V
ClientSampleId :
BFB184

m/z	Abundance
36.00	535.0
37.10	2203.0
38.10	1667.0
39.00	857.0
40.10	137.0
44.10	644.0
45.00	498.0
47.00	660.0
47.90	328.0
49.10	1824.0
50.10	9389.0
51.10	2694.0
54.90	221.0
56.10	592.0
57.10	1211.0
60.00	453.0
61.00	2489.0
62.00	2928.0
63.10	2663.0
64.10	386.0
65.10	779.0
67.00	123.0
67.20	125.0
68.00	5696.0
69.10	5576.0
70.10	581.0
72.00	345.0
73.00	2356.0
74.10	9498.0
75.10	29328.0
76.10	2941.0
77.10	133.0
77.70	105.0
78.90	1678.0
79.90	741.0
80.90	2223.0
81.90	448.0
85.70	103.0
87.10	1620.0
88.00	2473.0
90.80	167.0
92.00	2208.0
93.10	2719.0
94.10	6780.0
95.10	59680.0
96.10	4414.0
97.00	248.0
104.00	279.0
106.10	416.0
115.00	163.0
116.10	285.0
116.90	535.0
117.90	403.0
118.90	460.0
127.80	203.0
129.90	216.0
136.80	119.0
140.90	817.0
142.20	146.0
142.90	769.0
145.00	290.0
145.70	106.0
147.90	234.0
152.80	105.0
155.00	176.0
156.80	110.0
172.00	1045.0
174.00	58704.0
175.00	4373.0
176.00	55768.0
177.00	3714.0
178.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB184

m/z	Abundance
36.00	534.0
37.10	1996.0
38.10	1527.0
39.10	808.0
40.00	168.0
44.10	665.0
45.00	490.0
47.00	578.0
48.10	252.0
49.10	1571.0
50.10	8921.0
51.00	2661.0
54.80	250.0
56.10	558.0
57.10	1283.0
60.00	432.0
61.10	2229.0
62.10	2756.0
63.10	2458.0
64.10	389.0
65.00	799.0
68.00	5309.0
69.10	5217.0
70.10	463.0
72.10	280.0
73.00	2303.0
74.10	8967.0
75.10	27840.0
76.10	3082.0
77.10	128.0
77.70	148.0
78.90	1737.0
79.90	622.0
80.90	2245.0
82.00	355.0
85.70	139.0
87.10	1512.0
88.00	2335.0
90.80	152.0
92.00	1881.0
93.10	2598.0
94.00	6729.0
95.10	55624.0
96.10	3989.0
97.00	188.0
104.00	266.0
106.00	381.0
106.80	101.0
116.10	327.0
117.00	463.0
117.90	385.0
119.00	428.0
127.90	163.0
130.00	167.0
136.90	122.0
140.80	818.0
142.10	103.0
143.00	939.0
144.10	115.0
145.10	134.0
145.80	116.0
147.90	240.0
155.00	190.0
156.80	139.0
172.00	1015.0
174.00	56672.0
175.00	4113.0
176.00	54928.0
177.00	3206.0
178.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB184