

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
 Data File : VV035247.D
 Acq On : 16 Apr 2024 17:57
 Operator : SY/MD
 Sample : P2117-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0MH3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	113230	123421	18.22%	2.172%
2	1.359	91	99	101	rBV4	13841	17794	2.63%	0.313%
3	1.532	147	153	173	rVB	97071	118680	17.52%	2.088%
4	2.060	308	317	333	rVB	183861	282206	41.67%	4.966%
5	3.815	852	863	910	rBV2	74762	300713	44.40%	5.292%
6	4.249	982	998	1029	rBV	113735	303561	44.82%	5.342%
7	4.957	1204	1218	1245	rBV2	260806	677240	100.00%	11.918%
8	5.535	1387	1398	1433	rBV	203951	444990	65.71%	7.831%
9	5.851	1486	1496	1509	rBV9	7452	16681	2.46%	0.294%
10	5.989	1521	1539	1563	rBV	155610	332999	49.17%	5.860%
11	6.918	1818	1828	1855	rBV	59656	122505	18.09%	2.156%
12	7.243	1917	1929	1958	rBV	282334	517697	76.44%	9.110%
13	7.561	2019	2028	2052	rBV2	32612	69135	10.21%	1.217%
14	8.027	2164	2173	2216	rBV	281533	623192	92.02%	10.967%
15	8.783	2395	2408	2437	rBV	338774	578525	85.42%	10.180%
16	10.153	2824	2834	2853	rVB	120918	194315	28.69%	3.419%
17	11.185	3145	3155	3181	rBV	306672	500677	73.93%	8.811%
18	11.503	3243	3254	3261	rBV7	5695	11776	1.74%	0.207%
19	11.561	3261	3272	3293	rVB	278610	446580	65.94%	7.859%




Sum of corrected areas: 5682687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035247.D
Acq On : 16 Apr 2024 17:57
Operator : SY/MD
Sample : P2117-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0MH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

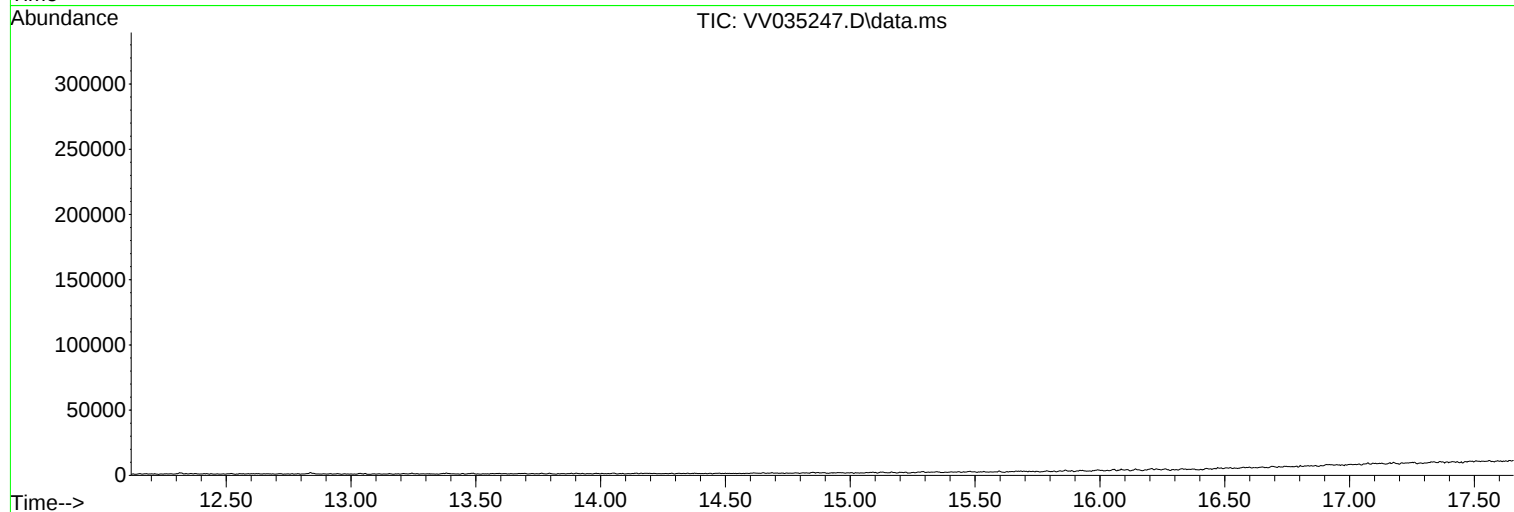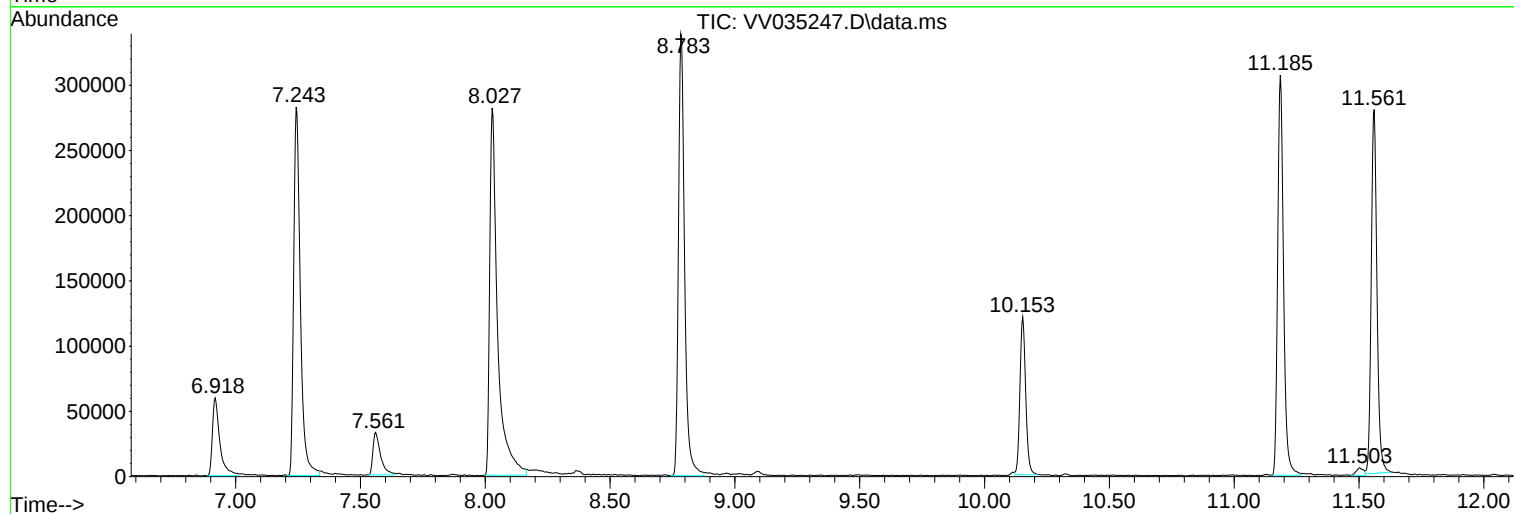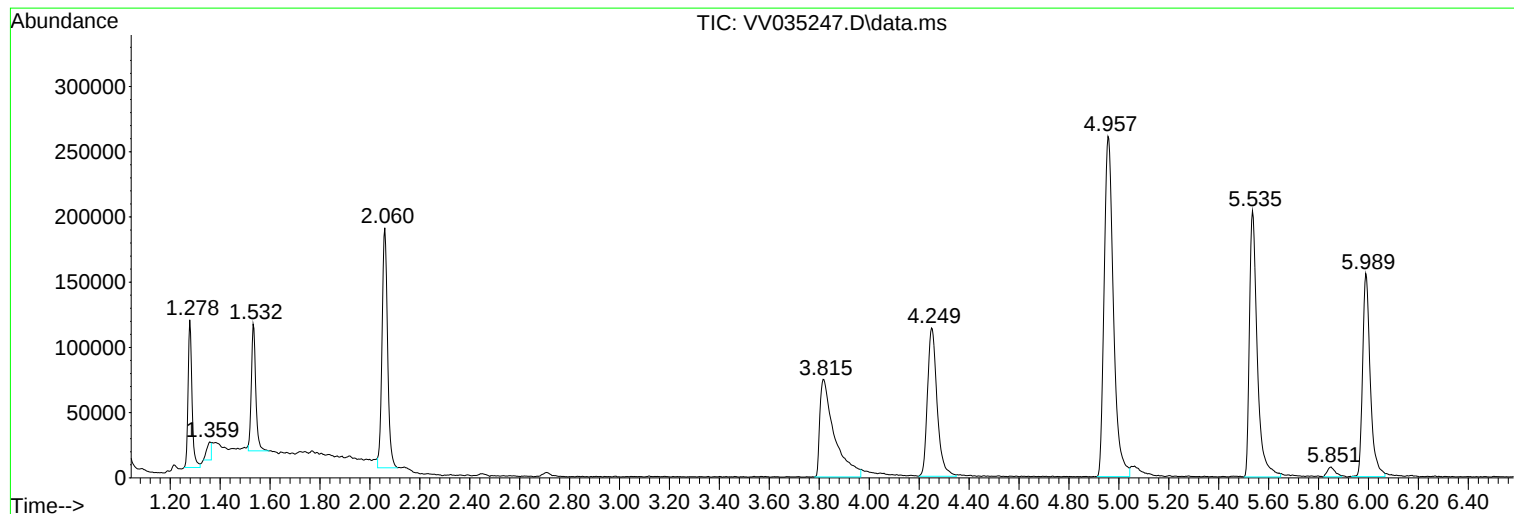

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035247.D
Acq On : 16 Apr 2024 17:57
Operator : SY/MD
Sample : P2117-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0MH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035247.D
Acq On : 16 Apr 2024 17:57
Operator : SY/MD
Sample : P2117-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0MH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc