

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
 Data File : VV035251.D
 Acq On : 16 Apr 2024 19:33
 Operator : SY/MD
 Sample : VIBLK335
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK335

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	124766	133213	17.15%	2.146%
2	1.532	146	153	167	rBV	108497	131087	16.88%	2.112%
3	2.060	307	317	336	rVB	196696	293081	37.74%	4.721%
4	3.815	854	863	904	rBV2	65815	281639	36.27%	4.537%
5	4.249	980	998	1024	rBV	127698	338373	43.57%	5.451%
6	4.957	1203	1218	1251	rBV2	300174	776562	100.00%	12.509%
7	5.535	1386	1398	1431	rBV	207614	453046	58.34%	7.298%
8	5.989	1527	1539	1567	rBV	175324	375719	48.38%	6.052%
9	6.918	1818	1828	1851	rBV	68572	142352	18.33%	2.293%
10	7.243	1919	1929	1950	rBV	320266	579382	74.61%	9.333%
11	7.561	2020	2028	2051	rBV2	40481	82724	10.65%	1.333%
12	8.027	2163	2173	2211	rBV	329498	719249	92.62%	11.586%
13	8.786	2394	2409	2438	rBV	335651	585611	75.41%	9.433%
14	10.153	2823	2834	2850	rBV	132237	217055	27.95%	3.496%
15	11.185	3144	3155	3178	rVV	308548	505735	65.12%	8.147%
16	11.561	3260	3272	3290	rBV	308780	513168	66.08%	8.266%
17	12.587	3584	3591	3604	rBV4	5998	9482	1.22%	0.153%
18	13.207	3769	3784	3794	rBV3	10342	17343	2.23%	0.279%
19	13.445	3848	3858	3870	rBV	20754	34777	4.48%	0.560%
20	13.683	3923	3932	3941	rBV3	11316	18214	2.35%	0.293%




Sum of corrected areas: 6207812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035251.D
Acq On : 16 Apr 2024 19:33
Operator : SY/MD
Sample : VIBLK335
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

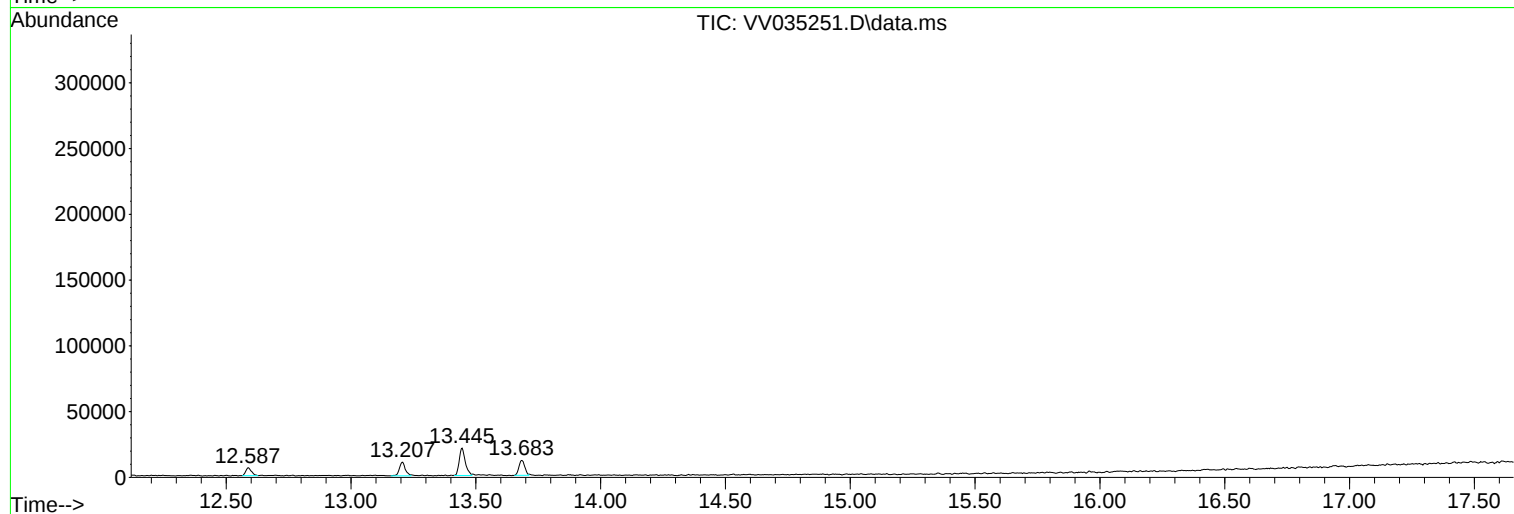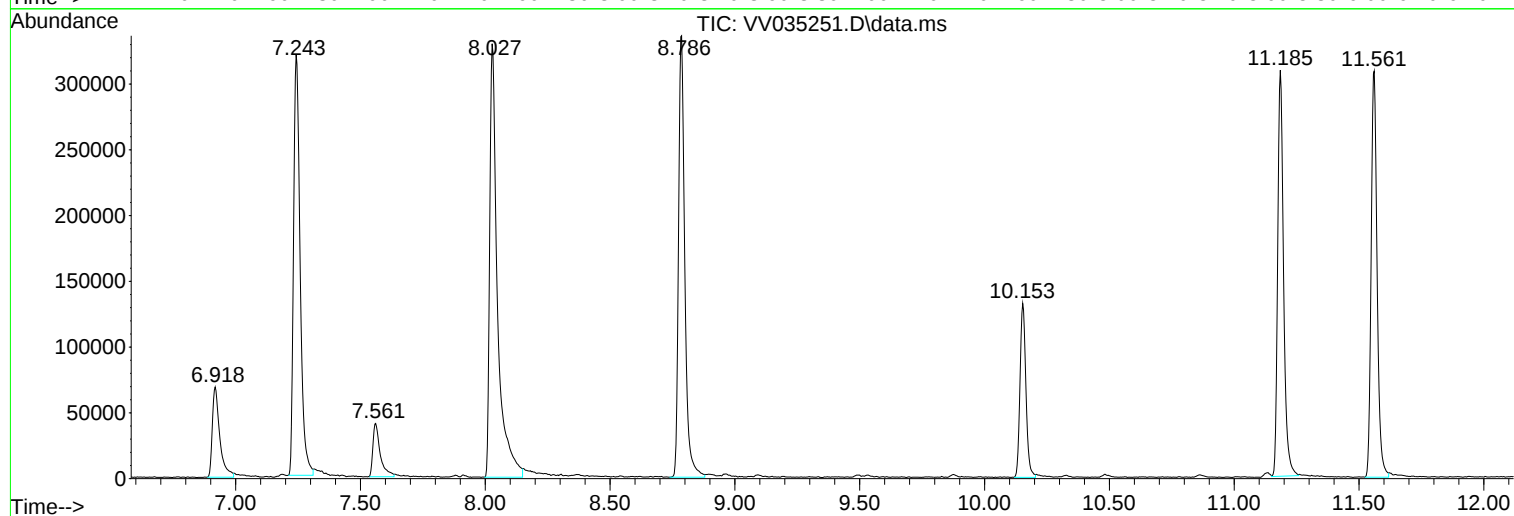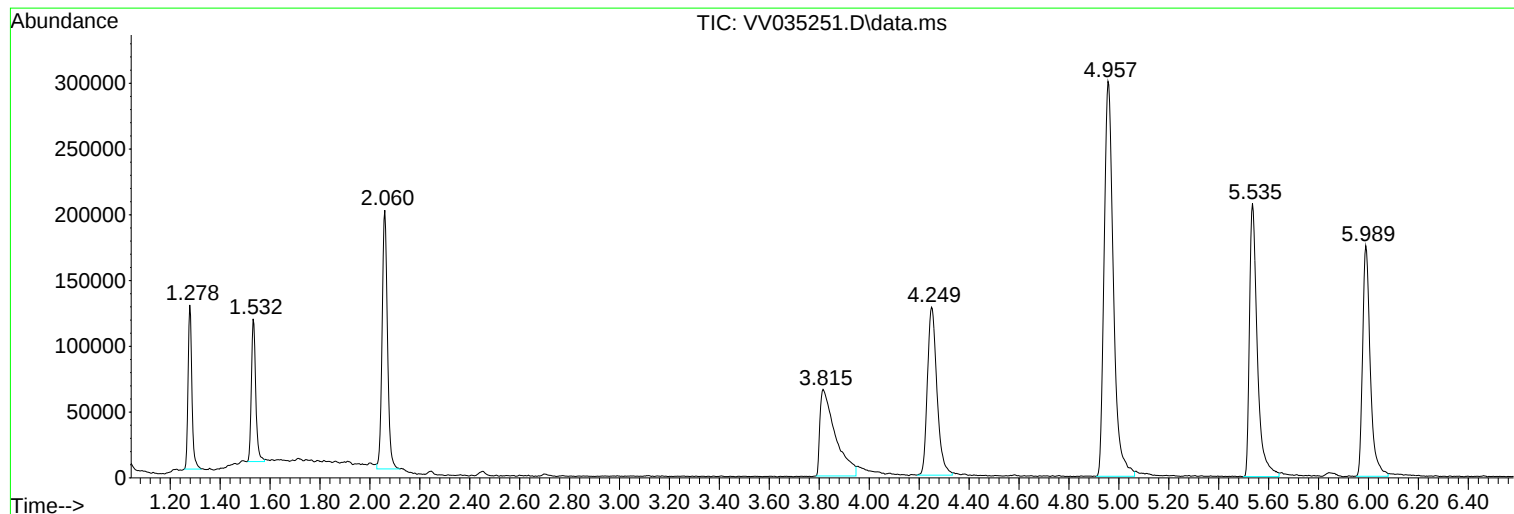

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035251.D
Acq On : 16 Apr 2024 19:33
Operator : SY/MD
Sample : VIBLK335
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035251.D
Acq On : 16 Apr 2024 19:33
Operator : SY/MD
Sample : VIBLK335
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------