


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041624\
Data File : VV035225.D
Acq On : 16 Apr 2024 08:30
Operator : SY/MD
Sample : BFB269
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB269

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 18 00:40:19 2024

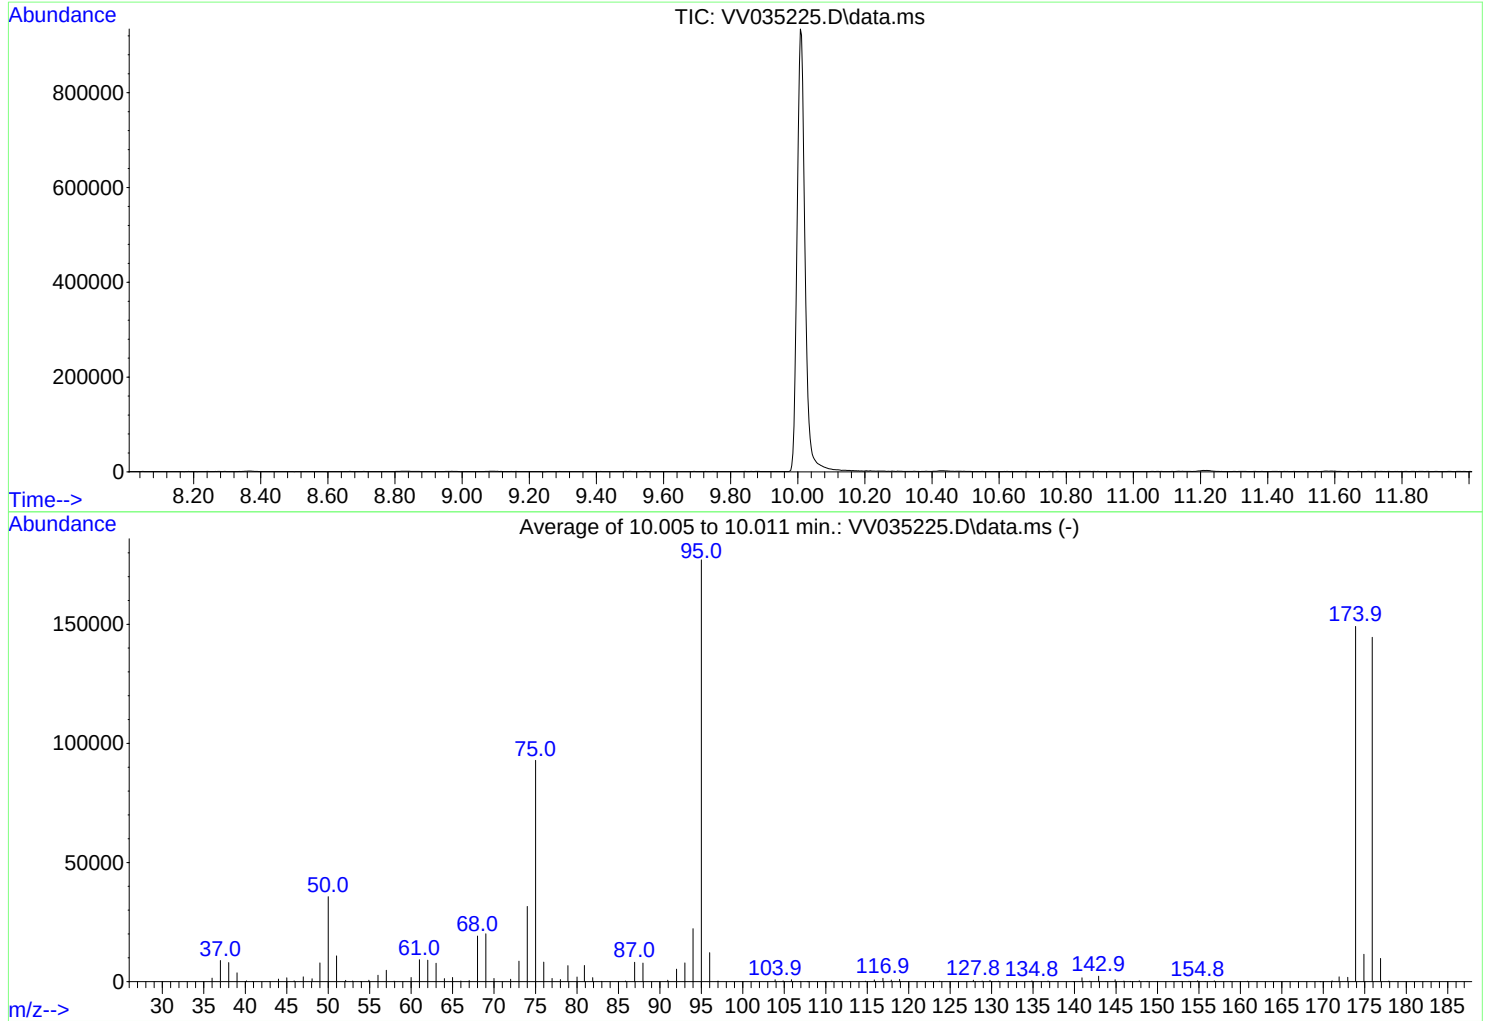

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	35632	PASS
75	95	30	80	52.5	92877	PASS
95	95	100	100	100.0	177045	PASS
96	95	5	9	6.9	12154	PASS
173	174	0.00	2	1.2	1822	PASS
174	95	50	120	84.2	149099	PASS
175	174	5	9	7.7	11486	PASS
176	174	95	105	97.0	144555	PASS
177	176	5	10	6.7	9737	PASS

m/z	Abundance
39.90	261.0
44.00	444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	1508.0
37.00	8862.0
38.00	8077.0
39.00	3634.0
40.20	327.0
43.00	110.0
44.00	1398.0
45.00	1607.0
45.90	394.0
47.00	1855.0
48.00	1205.0
49.00	7657.0
50.00	34408.0
51.00	10474.0
52.10	505.0
52.90	242.0
53.90	104.0
54.90	553.0
56.00	2673.0
57.00	4595.0
58.00	169.0
60.00	1687.0
61.00	8975.0
62.00	8831.0
63.00	7571.0
64.00	1264.0
65.00	1781.0
66.00	252.0
67.00	469.0
68.00	18480.0
69.00	19192.0
70.00	1230.0
72.00	958.0
73.00	8111.0
74.00	30560.0
75.00	88424.0
76.00	7693.0
77.00	1353.0
78.00	739.0
78.90	6324.0
80.00	1830.0
80.90	6716.0
81.90	1547.0
83.00	155.0
85.80	207.0
86.90	7860.0
87.90	7359.0
91.00	617.0
92.00	4996.0
93.00	7529.0
94.00	20880.0
95.00	169152.0
96.00	11782.0
97.00	255.0
103.90	808.0
104.80	332.0
105.90	801.0
106.90	180.0
107.80	105.0
109.90	152.0
110.70	160.0
112.00	132.0
112.90	134.0
114.80	207.0
115.90	666.0
116.90	1341.0
117.90	626.0
118.90	942.0
122.70	112.0
123.80	184.0
127.80	547.0
128.90	262.0
129.80	515.0
130.80	227.0
134.80	322.0
136.80	296.0
139.90	140.0
140.90	1605.0
141.80	157.0
142.90	2159.0
144.90	788.0
145.90	256.0
146.80	140.0
147.80	408.0
148.90	105.0
150.00	180.0
152.80	166.0
153.80	162.0
154.80	352.0
156.90	383.0
158.80	163.0
160.80	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

171.00	307.0
171.90	1876.0
173.00	1744.0
173.90	138304.0
174.90	11182.0
175.90	134208.0
176.90	9048.0
177.90	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	1476.0
37.00	9183.0
38.00	8346.0
39.00	3745.0
40.20	353.0
42.90	105.0
44.00	1504.0
45.00	1675.0
45.90	383.0
47.00	2118.0
48.10	1191.0
49.00	8135.0
50.00	36808.0
51.00	11190.0
52.10	592.0
53.00	275.0
54.90	613.0
56.00	2793.0
57.00	4890.0
57.90	171.0
60.00	1831.0
61.00	9534.0
62.00	9374.0
63.00	7972.0
64.00	1350.0
65.00	1765.0
66.00	267.0
67.00	511.0
68.00	19736.0
69.00	20744.0
70.00	1372.0
72.00	1078.0
73.00	8932.0
74.00	32584.0
75.00	96208.0
76.00	8530.0
77.00	1414.0
78.00	895.0
78.90	6946.0
80.00	2026.0
80.90	6942.0
81.90	1712.0
83.00	130.0
85.80	251.0
86.90	8479.0
88.00	8102.0
91.00	643.0
92.00	5403.0
93.00	8156.0
94.00	22936.0
95.00	182784.0
96.00	12539.0
97.00	317.0
103.90	877.0
104.80	341.0
105.80	838.0
106.90	174.0
109.90	140.0
110.80	179.0
112.00	159.0
112.90	173.0
114.80	234.0
115.80	757.0
116.90	1504.0
117.90	697.0
118.90	1006.0
122.70	101.0
123.70	202.0
127.80	645.0
128.90	253.0
129.80	542.0
130.90	222.0
134.90	322.0
136.80	314.0
139.90	136.0
140.90	1664.0
141.90	185.0
142.90	2336.0
143.80	130.0
144.90	862.0
146.00	289.0
146.80	124.0
147.80	443.0
148.70	129.0
150.00	170.0
152.80	153.0
153.80	195.0
154.90	399.0
155.70	139.0
156.90	385.0
158.80	178.0
160.90	247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

171.00	318.0
171.90	2095.0
172.90	1837.0
173.90	153792.0
174.90	11807.0
175.90	149312.0
176.90	10029.0
177.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	1447.0
37.00	8603.0
38.00	7614.0
39.00	3624.0
40.10	363.0
40.90	130.0
44.00	1573.0
45.00	1566.0
45.90	337.0
47.00	2185.0
48.10	1190.0
49.00	7858.0
50.00	35680.0
51.00	10864.0
52.10	568.0
53.00	287.0
54.90	603.0
56.00	2603.0
57.00	4815.0
57.90	197.0
60.00	1812.0
61.00	9163.0
62.00	8848.0
63.00	7619.0
64.00	1310.0
65.00	1694.0
66.00	268.0
67.00	514.0
68.00	19264.0
69.00	20232.0
70.00	1423.0
72.00	1073.0
73.00	8761.0
74.00	31592.0
75.00	94000.0
76.00	8413.0
77.00	1305.0
78.00	973.0
78.90	6832.0
80.00	2054.0
80.90	6662.0
81.90	1725.0
82.80	136.0
85.90	325.0
87.00	8137.0
88.00	7869.0
90.90	623.0
92.00	5246.0
93.00	7890.0
94.00	22960.0
95.00	179200.0
96.00	12140.0
97.00	338.0
103.90	841.0
104.90	317.0
105.90	774.0
106.90	156.0
109.90	104.0
110.80	204.0
111.90	167.0
112.90	193.0
114.80	217.0
115.80	770.0
116.90	1440.0
117.90	677.0
118.90	969.0
123.70	154.0
127.80	686.0
128.80	239.0
129.80	606.0
130.90	173.0
134.80	310.0
136.80	314.0
140.90	1623.0
141.90	224.0
142.90	2341.0
143.80	165.0
144.90	796.0
145.90	290.0
146.70	117.0
147.80	442.0
148.70	122.0
150.00	136.0
152.90	144.0
153.80	183.0
154.90	422.0
155.80	140.0
156.80	346.0
158.90	176.0
160.90	221.0
169.60	101.0
171.10	343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

171.90	2023.0
172.90	1885.0
173.90	155200.0
174.90	11469.0
175.90	150144.0
176.90	10134.0
177.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269