

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015560.D
 Acq On : 17 Apr 2020 17:12
 Operator : SY/MD
 Sample : L2333-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Quant Time: Apr 18 02:43:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:24 AM

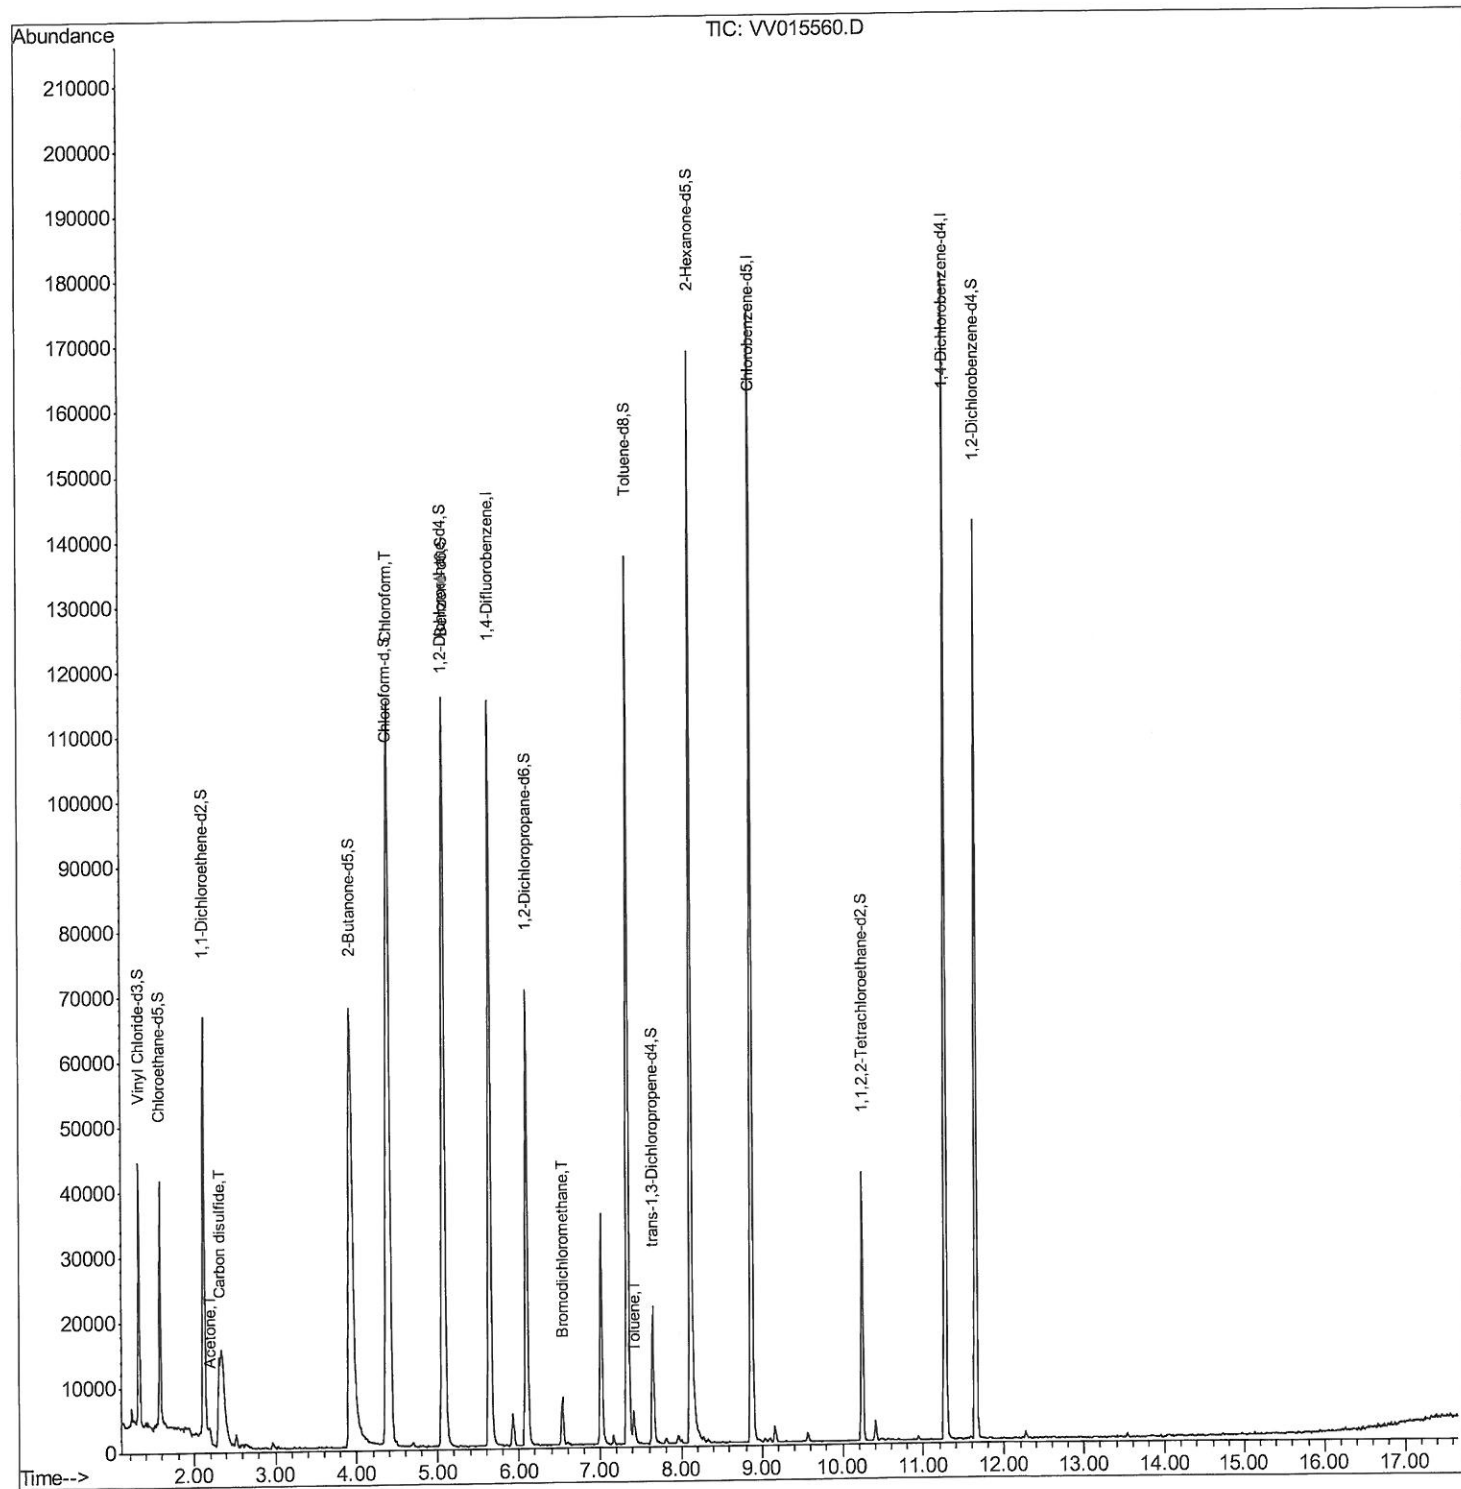

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015560.D
 Acq On : 17 Apr 2020 17:12
 Operator : SY/MD
 Sample : L2333-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0AC1

Quant Time: Apr 18 00:41:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:24 AM

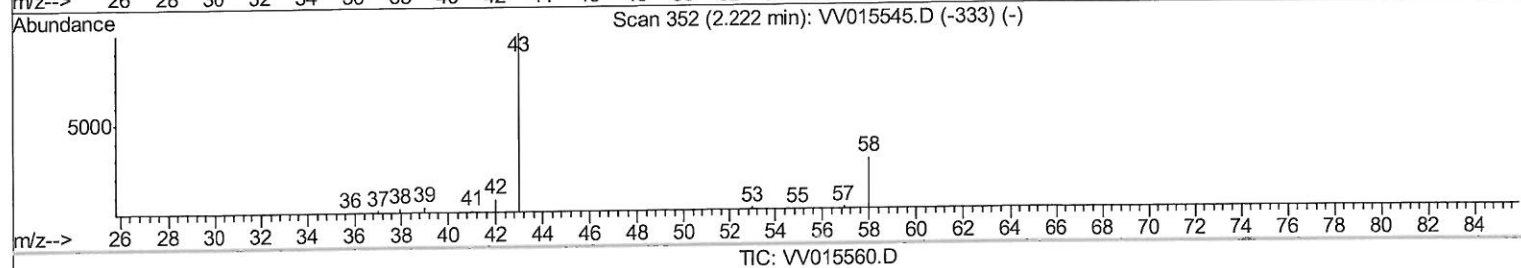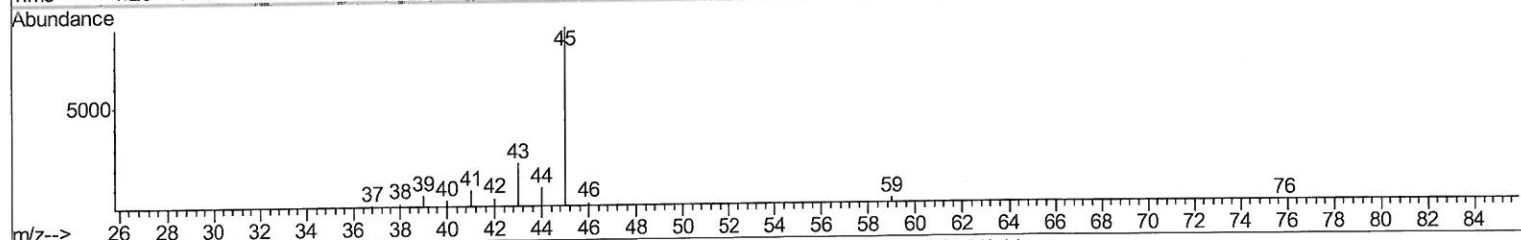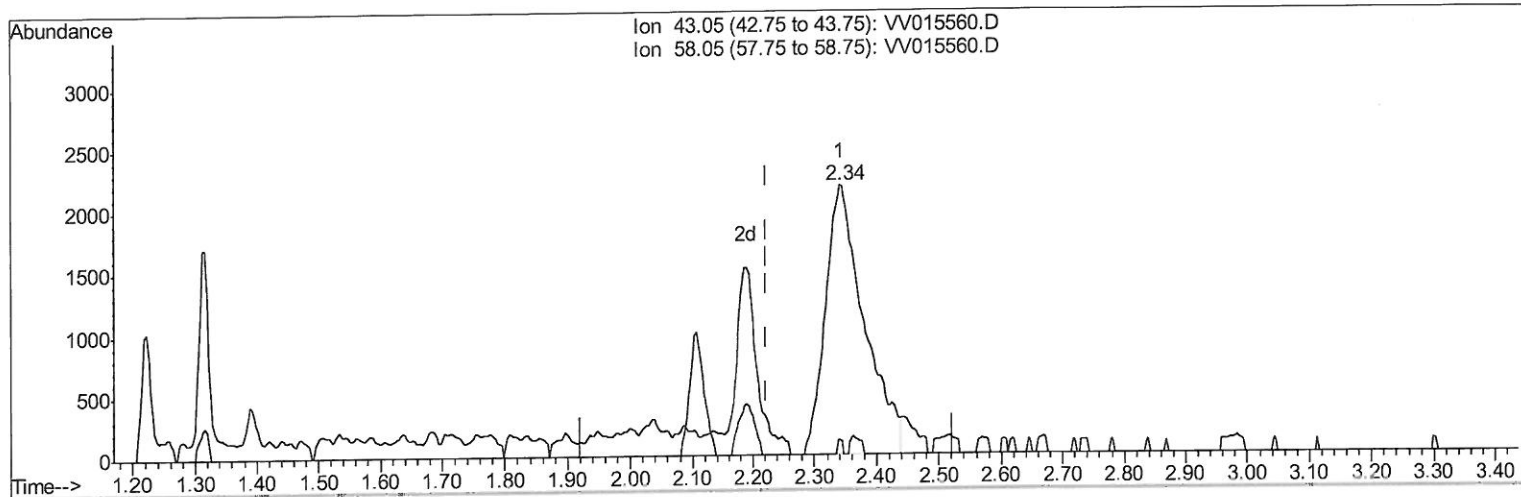

(13) Acetone (T)

2.341min (+0.119) 10.06ug/L

response 9405

Ion	Exp%	Act%
43.05	100	100
58.05	11.10	0.71
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015560.D
 Acq On : 17 Apr 2020 17:12
 Operator : SY/MD
 Sample : L2333-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Quant Time: Apr 18 00:41:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:24 AM

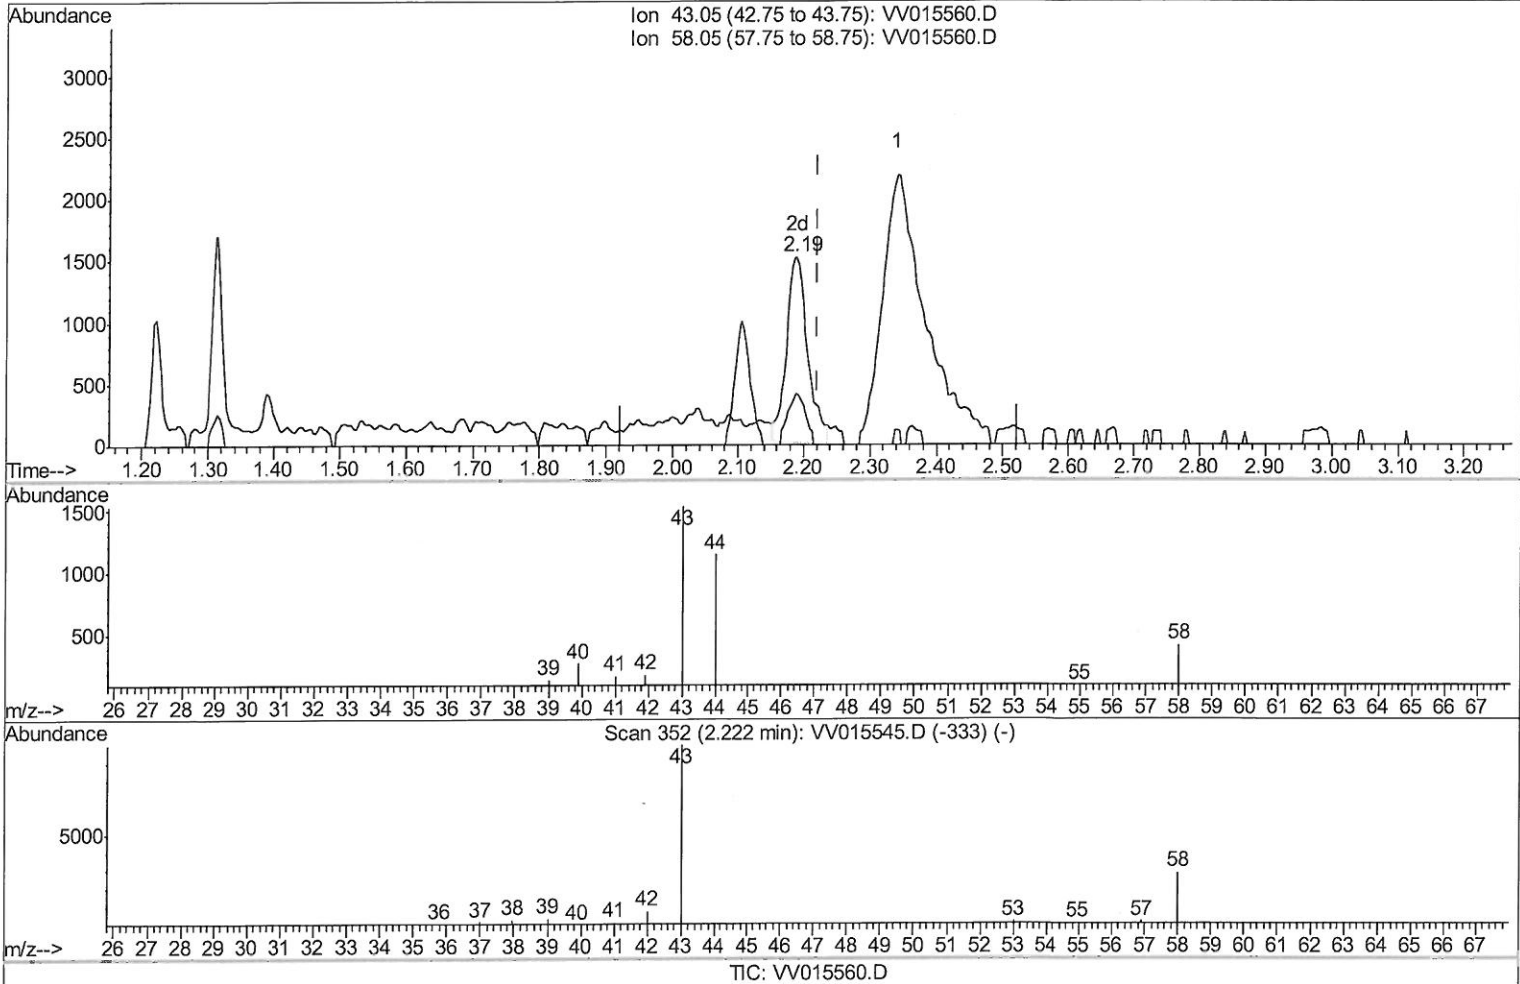

(13) Acetone (T)

2.190min (-0.032) 3.59ug/L m

response 3354

Ion	Exp%	Act%
43.05	100	100
58.05	11.10	2.00
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
4/28/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015560.D
 Acq On : 17 Apr 2020 17:12
 Operator : SY/MD
 Sample : L2333-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample ID :
 C0AC1

Quant Time: Apr 18 02:43:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:24 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	90856	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	86771	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	42072	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	21936	4.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.00%
7) Chloroethane-d5	1.58	69	21971	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.20%
11) 1,1-Dichloroethene-d2	2.12	63	33637	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.91	46	71757	54.21	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.42%
24) Chloroform-d	4.38	84	53927	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
26) 1,2-Dichloroethane-d4	5.06	65	30030	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.07	84	97171	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.09	67	30484	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.34	98	85789	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	7.65	79	11638	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.11	63	54264	43.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.30%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	18491	3.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	32520	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%

Target Compounds

					Ovalue
13) Acetone	2.19	43	3354m	3.586	ug/L
14) Carbon disulfide	2.31	76	9293	0.467	ug/L
25) Chloroform	4.40	83	92819	7.486	ug/L
38) Bromodichloromethane	6.54	83	5171	0.602	ug/L
42) Toluene	7.41	91	3685	0.131	ug/L

2 MD
 4/20/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed