

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015566.D
 Acq On : 17 Apr 2020 19:33
 Operator : SY/MD
 Sample : L2333-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Apr 18 03:49:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:57 AM

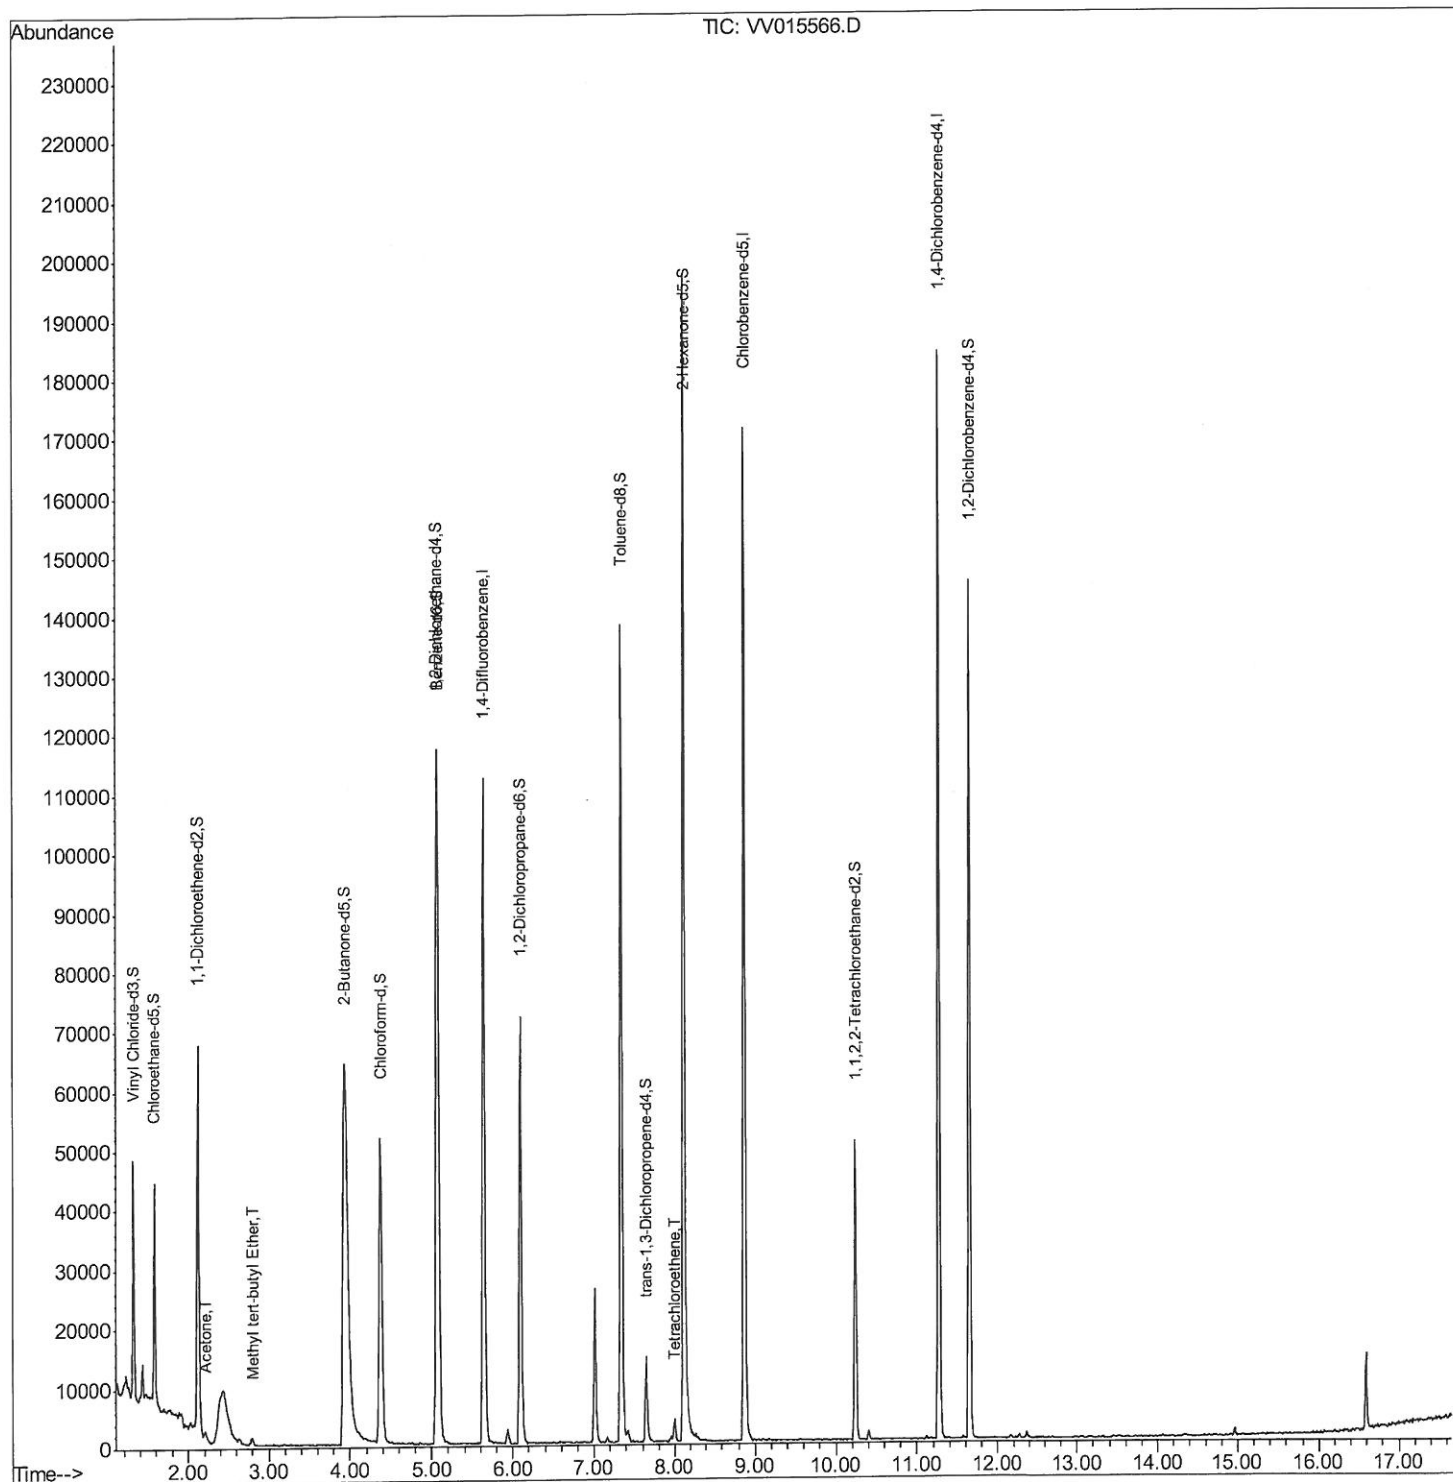

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015566.D
 Acq On : 17 Apr 2020 19:33
 Operator : SY/MD
 Sample : L2333-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Apr 18 00:42:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:57 AM

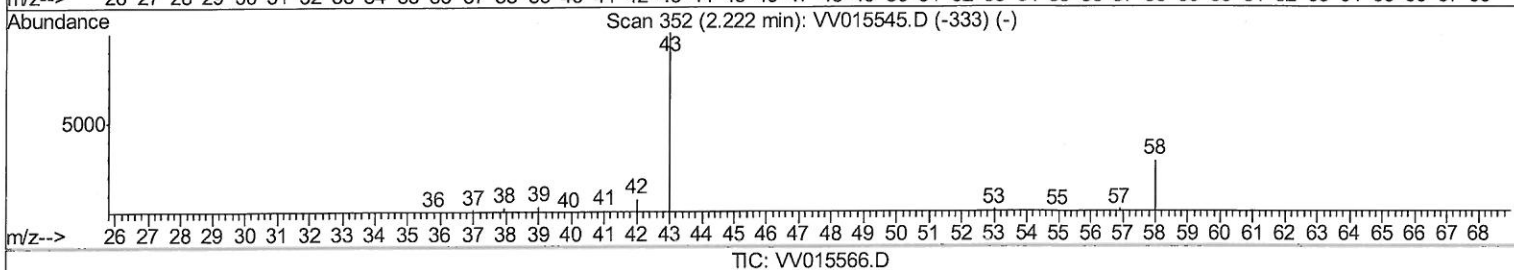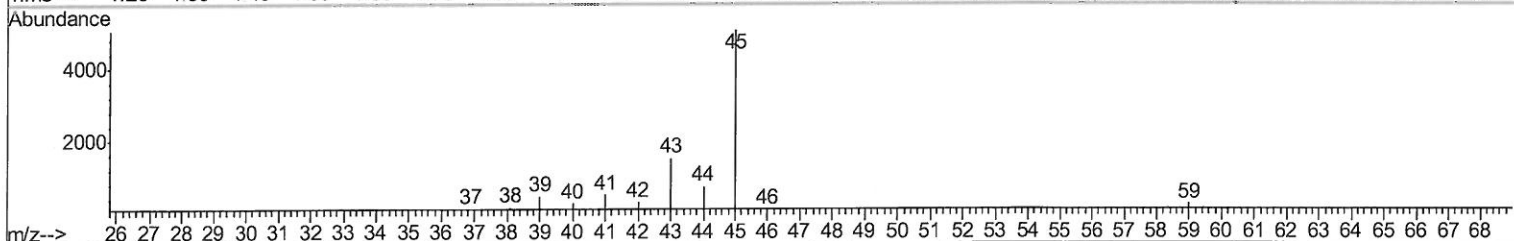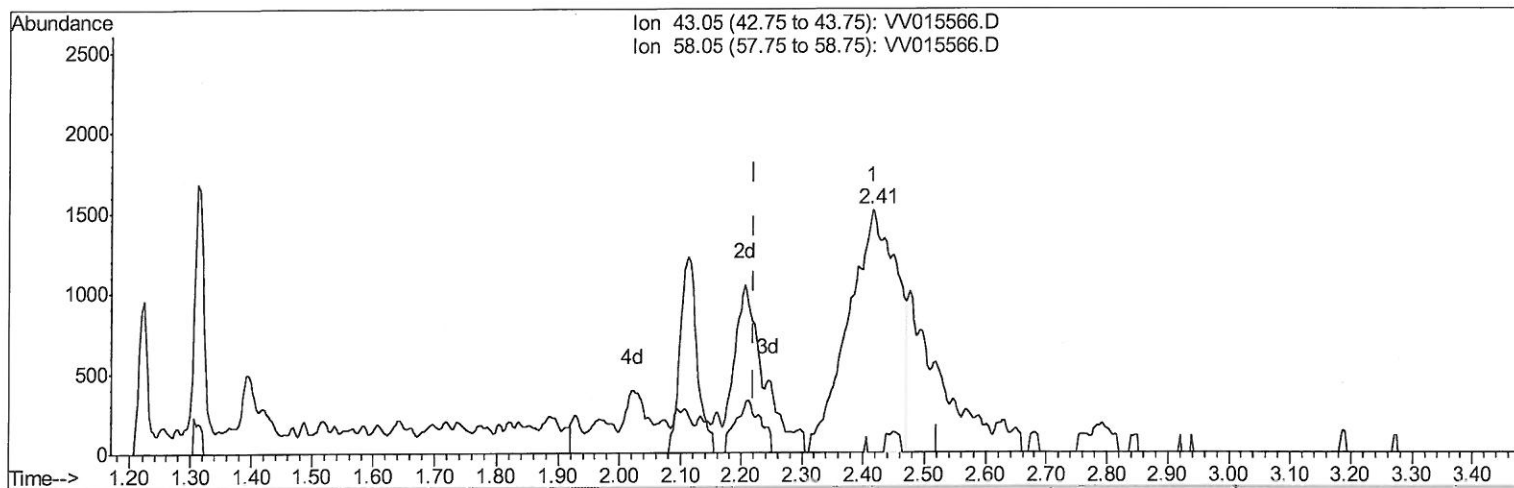

(13) Acetone (T)

2.415min (+0.193) 8.98ug/L

response 8335

Ion	Exp%	Act%
43.05	100	100
58.05	11.10	2.18
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015566.D
 Acq On : 17 Apr 2020 19:33
 Operator : SY/MD
 Sample : L2333-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Apr 18 00:42:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:57 AM

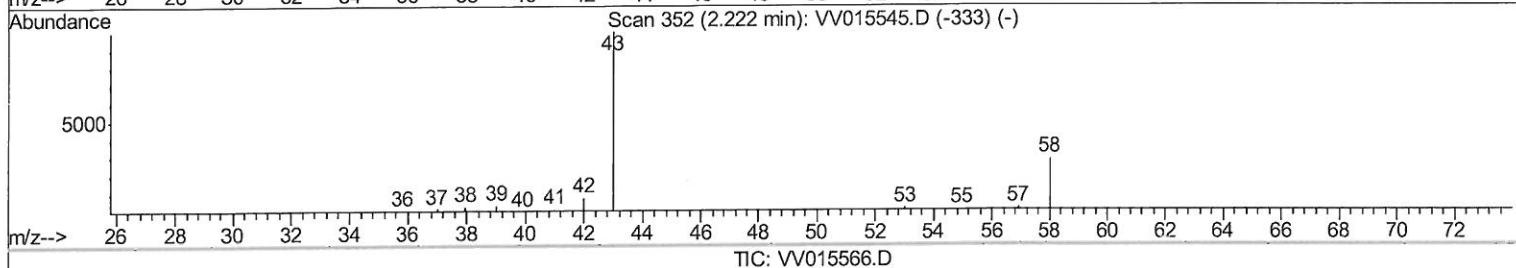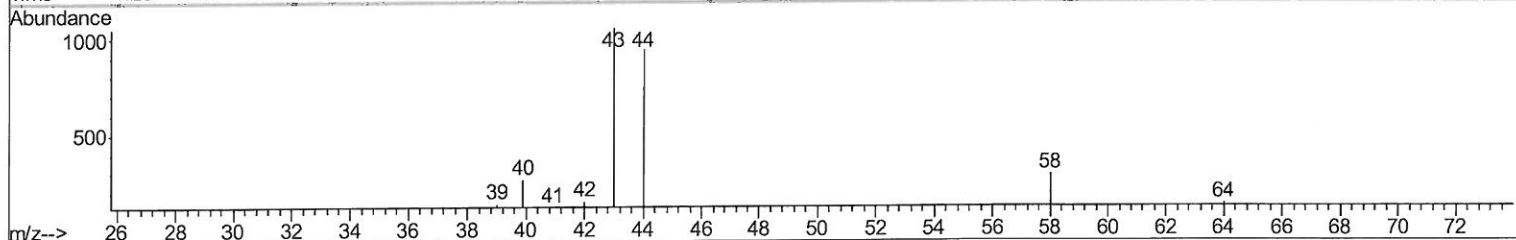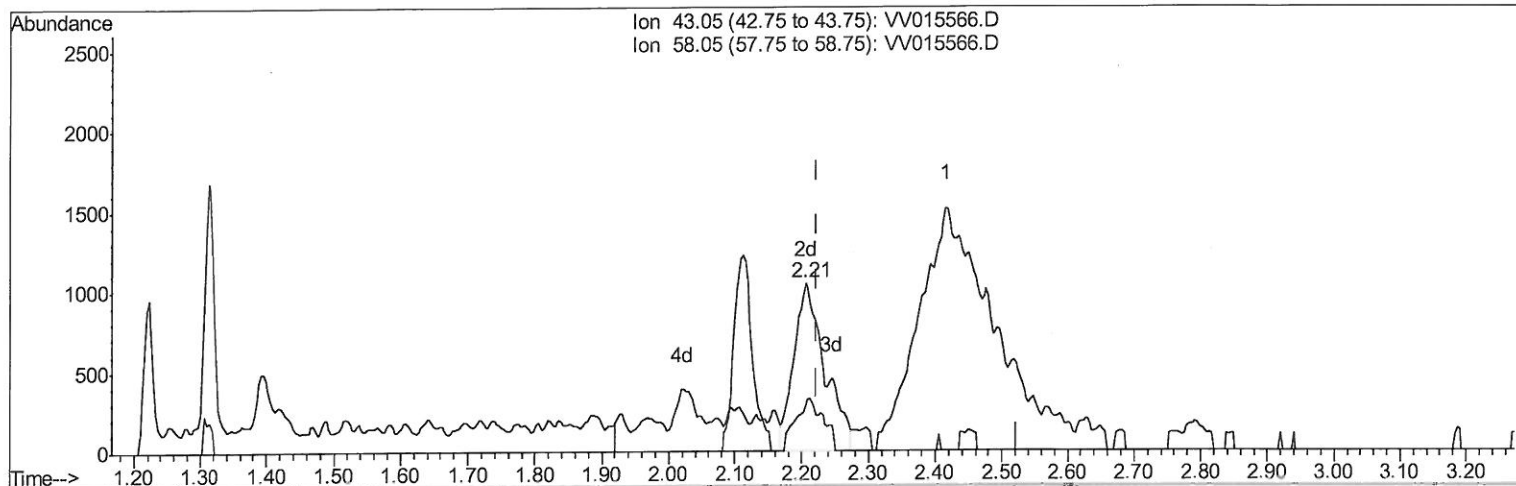

TIC: VV015566.D

(13) Acetone (T)

2.206min (-0.016) 3.64ug/L m

response 3378

Ion	Exp%	Act%
43.05	100	100
58.05	11.10	5.39
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 2 MB
 4/28/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041720\
 Data File : VV015566.D
 Acq On : 17 Apr 2020 19:33
 Operator : SY/MD
 Sample : L2333-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Apr 18 03:49:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 00:37:52 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/20/2020 11:41:57 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	90185	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	85169	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	42511	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	21830	4.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 93.20%	
7) Chloroethane-d5	1.58	69	21809	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 101.20%	
11) 1,1-Dichloroethene-d2	2.12	63	33312	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 67.60%	
20) 2-Butanone-d5	3.93	46	83723	63.72	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	= 127.44%	
24) Chloroform-d	4.38	84	51774	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 100.00%	
26) 1,2-Dichloroethane-d4	5.06	65	30123	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 107.80%	
32) Benzene-d6	5.08	84	96853	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 102.60%	
36) 1,2-Dichloropropane-d6	6.09	67	31650	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 107.60%	
41) Toluene-d8	7.34	98	86992	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 96.40%	
43) trans-1,3-Dichloropropene-	7.65	79	8319	3.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 65.00%	
46) 2-Hexanone-d5	8.11	63	65382	52.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 105.94%	
57) 1,1,2,2-Tetrachloroethane-	10.24	84	22869	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 98.00%	
64) 1,2-Dichlorobenzene-d4	11.65	152	34193	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 100.20%	

Target Compounds					Ovalue	
13) Acetone	2.21	43	3378m	3.639	ug/L	
17) Methyl tert-butyl Ether	2.79	73	946	0.063	ug/L	# 74
47) Tetrachloroethene	7.99	164	791	0.156	ug/L	93

7m0
 4/28/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed