


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041720\
 Data File : VV015544.D
 Acq On : 17 Apr 2020 10:06
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Apr 18 00:37:52 2020

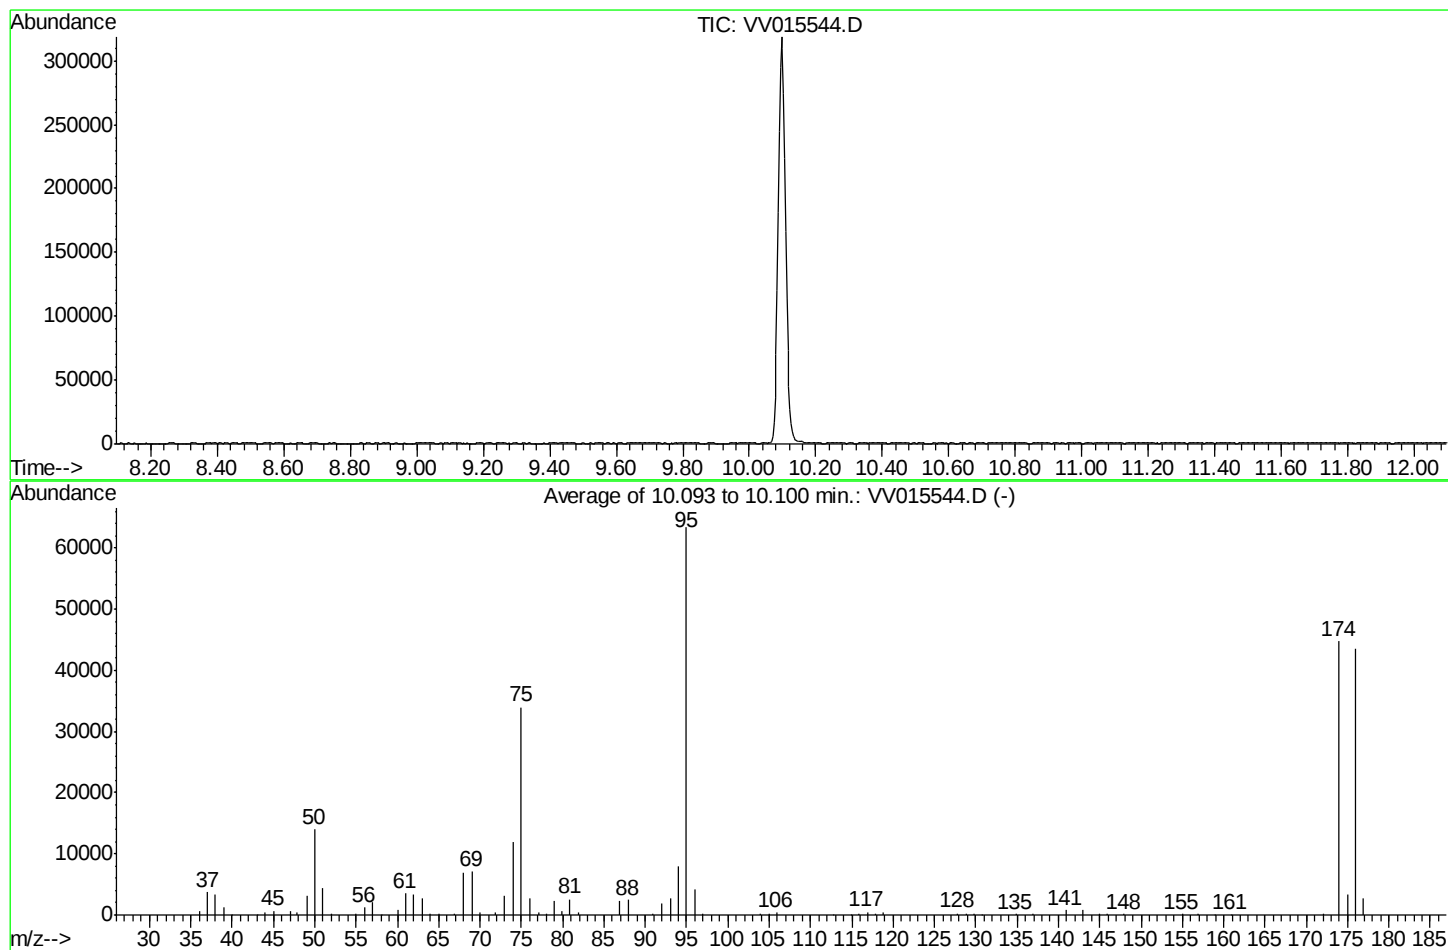

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	14003	PASS
75	95	30	80	53.6	33938	PASS
95	95	100	100	100.0	63370	PASS
96	95	5	9	6.6	4185	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	44717	PASS
175	174	5	9	7.5	3366	PASS
176	174	95	101	97.3	43530	PASS
177	176	5	9	6.3	2731	PASS

m/z	Abundance
36.00	626.0
37.00	3662.0
38.00	3289.0
39.00	1230.0
40.00	244.0
43.00	102.0
44.00	727.0
45.00	616.0
47.00	736.0
47.90	428.0
49.00	3012.0
50.00	13561.0
51.00	4355.0
52.00	284.0
54.90	257.0
56.00	1154.0
57.00	1937.0
60.00	741.0
61.00	3419.0
62.00	3241.0
63.00	2677.0
64.00	271.0
65.00	193.0
66.90	201.0
68.00	6664.0
69.00	6948.0
70.00	567.0
71.90	414.0
73.00	3153.0
74.00	11672.0
75.00	33128.0
76.00	2797.0
77.00	376.0
78.00	319.0
78.90	2345.0
79.90	648.0
80.90	2464.0
81.90	476.0
86.90	2144.0
87.90	2379.0
90.90	260.0
92.00	1898.0
93.00	2705.0
94.00	7641.0
95.00	60784.0
96.00	4050.0
96.90	147.0
103.90	320.0
105.00	139.0
105.90	358.0
112.80	101.0
115.80	270.0
116.90	487.0
117.90	270.0
118.80	347.0
127.80	217.0
128.90	164.0
129.80	209.0
134.90	107.0
136.90	123.0
140.90	826.0
142.90	658.0
144.90	115.0
145.90	117.0
148.00	115.0
155.00	185.0
156.90	119.0
172.10	295.0
174.00	41720.0
175.00	3228.0
176.00	40640.0
176.90	2554.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	697.0
37.00	3890.0
38.00	3455.0
39.00	1369.0
40.00	271.0
44.00	736.0
45.00	674.0
47.00	740.0
47.90	446.0
49.00	3244.0
50.00	14441.0
51.00	4538.0
52.00	255.0
54.90	262.0
56.00	1213.0
57.00	2108.0
58.00	106.0
60.00	836.0
61.00	3595.0
62.00	3532.0
63.00	2914.0
64.00	272.0
65.10	193.0
66.90	196.0
68.00	7238.0
69.00	7239.0
69.90	517.0
71.90	465.0
73.00	3353.0
74.00	12363.0
75.00	35080.0
76.00	2885.0
77.00	339.0
78.00	320.0
78.90	2477.0
79.90	732.0
80.90	2646.0
81.90	511.0
86.90	2293.0
88.00	2570.0
90.90	272.0
92.00	2007.0
93.00	2929.0
94.00	8296.0
95.00	65512.0
96.00	4349.0
97.00	179.0
103.90	322.0
105.00	142.0
105.90	361.0
114.90	101.0
115.80	293.0
116.90	521.0
117.90	278.0
118.80	359.0
127.80	266.0
128.90	171.0
129.90	254.0
130.80	110.0
134.80	131.0
136.90	155.0
140.90	809.0
142.90	801.0
145.00	134.0
145.90	135.0
147.90	150.0
155.00	202.0
156.90	142.0
160.90	112.0
172.00	300.0
174.00	46456.0
175.00	3522.0
176.00	45104.0
177.00	2830.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	715.0
37.00	3704.0
38.00	3248.0
39.00	1349.0
40.00	259.0
44.00	721.0
45.00	627.0
47.00	638.0
47.90	413.0
49.00	3175.0
50.00	14007.0
51.00	4169.0
52.00	213.0
54.90	225.0
56.00	1158.0
57.00	2063.0
58.00	123.0
60.00	803.0
61.00	3479.0
62.00	3450.0
63.00	2736.0
64.00	254.0
65.00	186.0
66.90	175.0
68.00	7126.0
69.00	6993.0
69.90	480.0
71.90	460.0
73.00	3200.0
74.00	11699.0
75.00	33608.0
76.00	2728.0
77.10	310.0
78.00	269.0
78.90	2336.0
79.90	701.0
80.90	2538.0
81.90	507.0
86.90	2354.0
88.00	2460.0
90.90	245.0
92.00	1947.0
93.00	2828.0
94.00	8242.0
95.00	63816.0
96.00	4158.0
97.00	192.0
103.90	295.0
104.90	128.0
105.90	337.0
115.80	291.0
116.90	490.0
117.80	280.0
118.80	334.0
127.80	283.0
128.90	136.0
129.80	265.0
130.70	112.0
134.80	145.0
136.90	171.0
140.90	726.0
142.90	839.0
144.90	126.0
145.90	132.0
147.90	174.0
155.00	182.0
156.90	148.0
158.90	116.0
160.80	129.0
171.90	313.0
174.00	45976.0
175.00	3350.0
176.00	44848.0
177.00	2809.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

Scan 2788 (10.055 min): VV015544.D
BFB37

m/z	Abundance
39.90	236.0
44.00	308.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37