

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
 Data File : VV035255.D
 Acq On : 17 Apr 2024 09:50
 Operator : SY/MD
 Sample : VV0417WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Quant Time: Apr 18 00:40:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 18 00:40:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	181799	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	191265	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	83537	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	77247	4.538	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.532	69	66960	5.063	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.200%
11) 1,1-Dichloroethene-d2	2.056	65	32769	4.538	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.800%
20) 2-Butanone-d5	3.828	46	157513	54.706	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.420%
24) Chloroform-d	4.249	84	135468	5.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	4.944	65	69912	5.519	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	4.960	84	256894	4.728	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
36) 1,2-Dichloropropane-d6	5.989	67	86534	5.121	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.243	98	204429	4.189	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
43) trans-1,3-Dichloroprop...	7.561	79	25357	4.205	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.030	63	108994	43.392	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.780%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	64968	4.991	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	77702	5.233	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.600%
Target Compounds						
16) Methylene chloride	2.449	84	10484	0.603	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035255.D
Acq On : 17 Apr 2024 09:50
Operator : SY/MD
Sample : VV0417WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236


Quant Time: Apr 18 00:40:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 18 00:40:19 2024
Response via : Initial Calibration

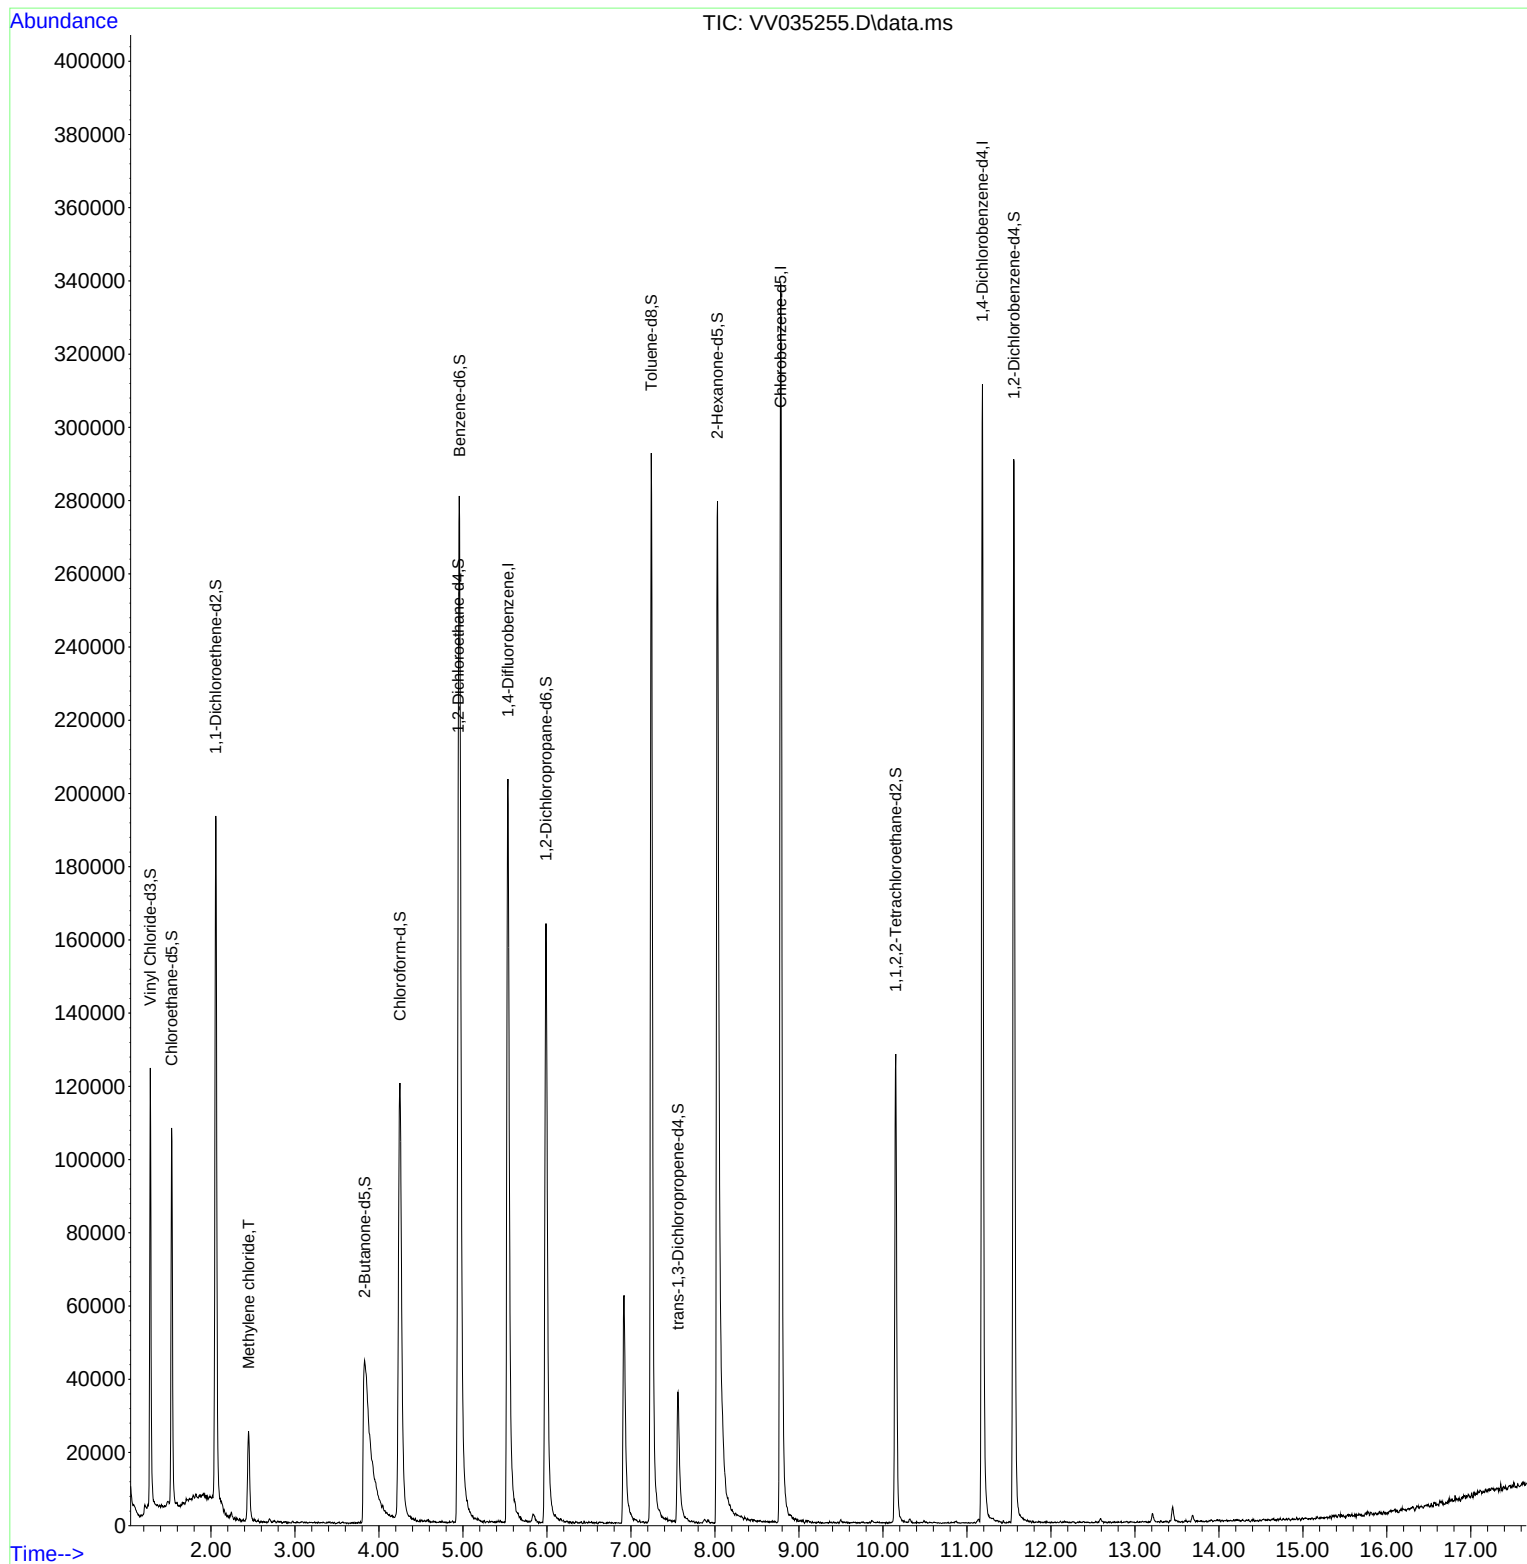

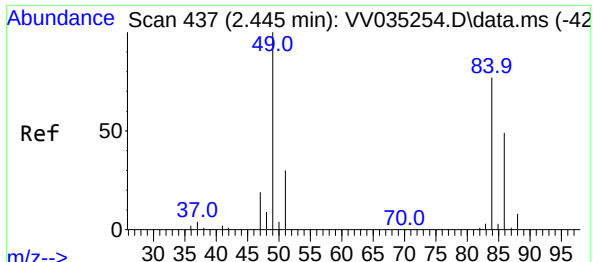

#16
Methylene chloride
Concen: 0.603 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV035255.D
Acq: 17 Apr 2024 09:50

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

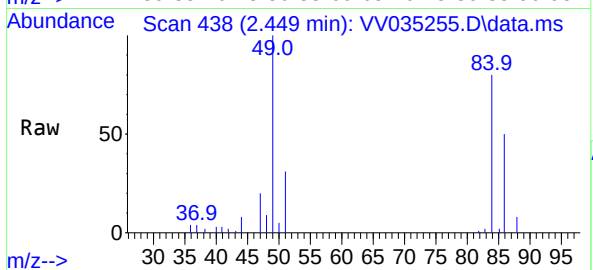

Tgt Ion:	84	Resp:	10484
Ion	Ratio	Lower	Upper
84	100		
86	63.2	45.6	84.6
49	125.5	89.5	166.1

