

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
 Data File : VV035266.D
 Acq On : 17 Apr 2024 14:10
 Operator : SY/MD
 Sample : P2056-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBP0

Quant Time: Apr 18 00:43:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 18 00:40:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	151683	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	172747	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	76597	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	45960	3.236	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.800%
7) Chloroethane-d5	1.532	69	44093	3.996	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.000%
11) 1,1-Dichloroethene-d2	2.060	65	20614	3.421	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.400%
20) 2-Butanone-d5	3.828	46	145982	60.767	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.540%
24) Chloroform-d	4.253	84	115488	5.200	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.000%
26) 1,2-Dichloroethane-d4	4.947	65	62655	5.928	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.600%
32) Benzene-d6	4.963	84	207502	4.228	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	5.992	67	75201	4.927	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.246	98	164434	3.730	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.600%
43) trans-1,3-Dichloroprop...	7.561	79	24430	4.485	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.800%
46) 2-Hexanone-d5	8.027	63	115899	51.087	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.180%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	65195	5.546	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	70905	5.208	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.902	164	621193	54.823	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035266.D
Acq On : 17 Apr 2024 14:10
Operator : SY/MD
Sample : P2056-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP0


Quant Time: Apr 18 00:43:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 18 00:40:19 2024
Response via : Initial Calibration

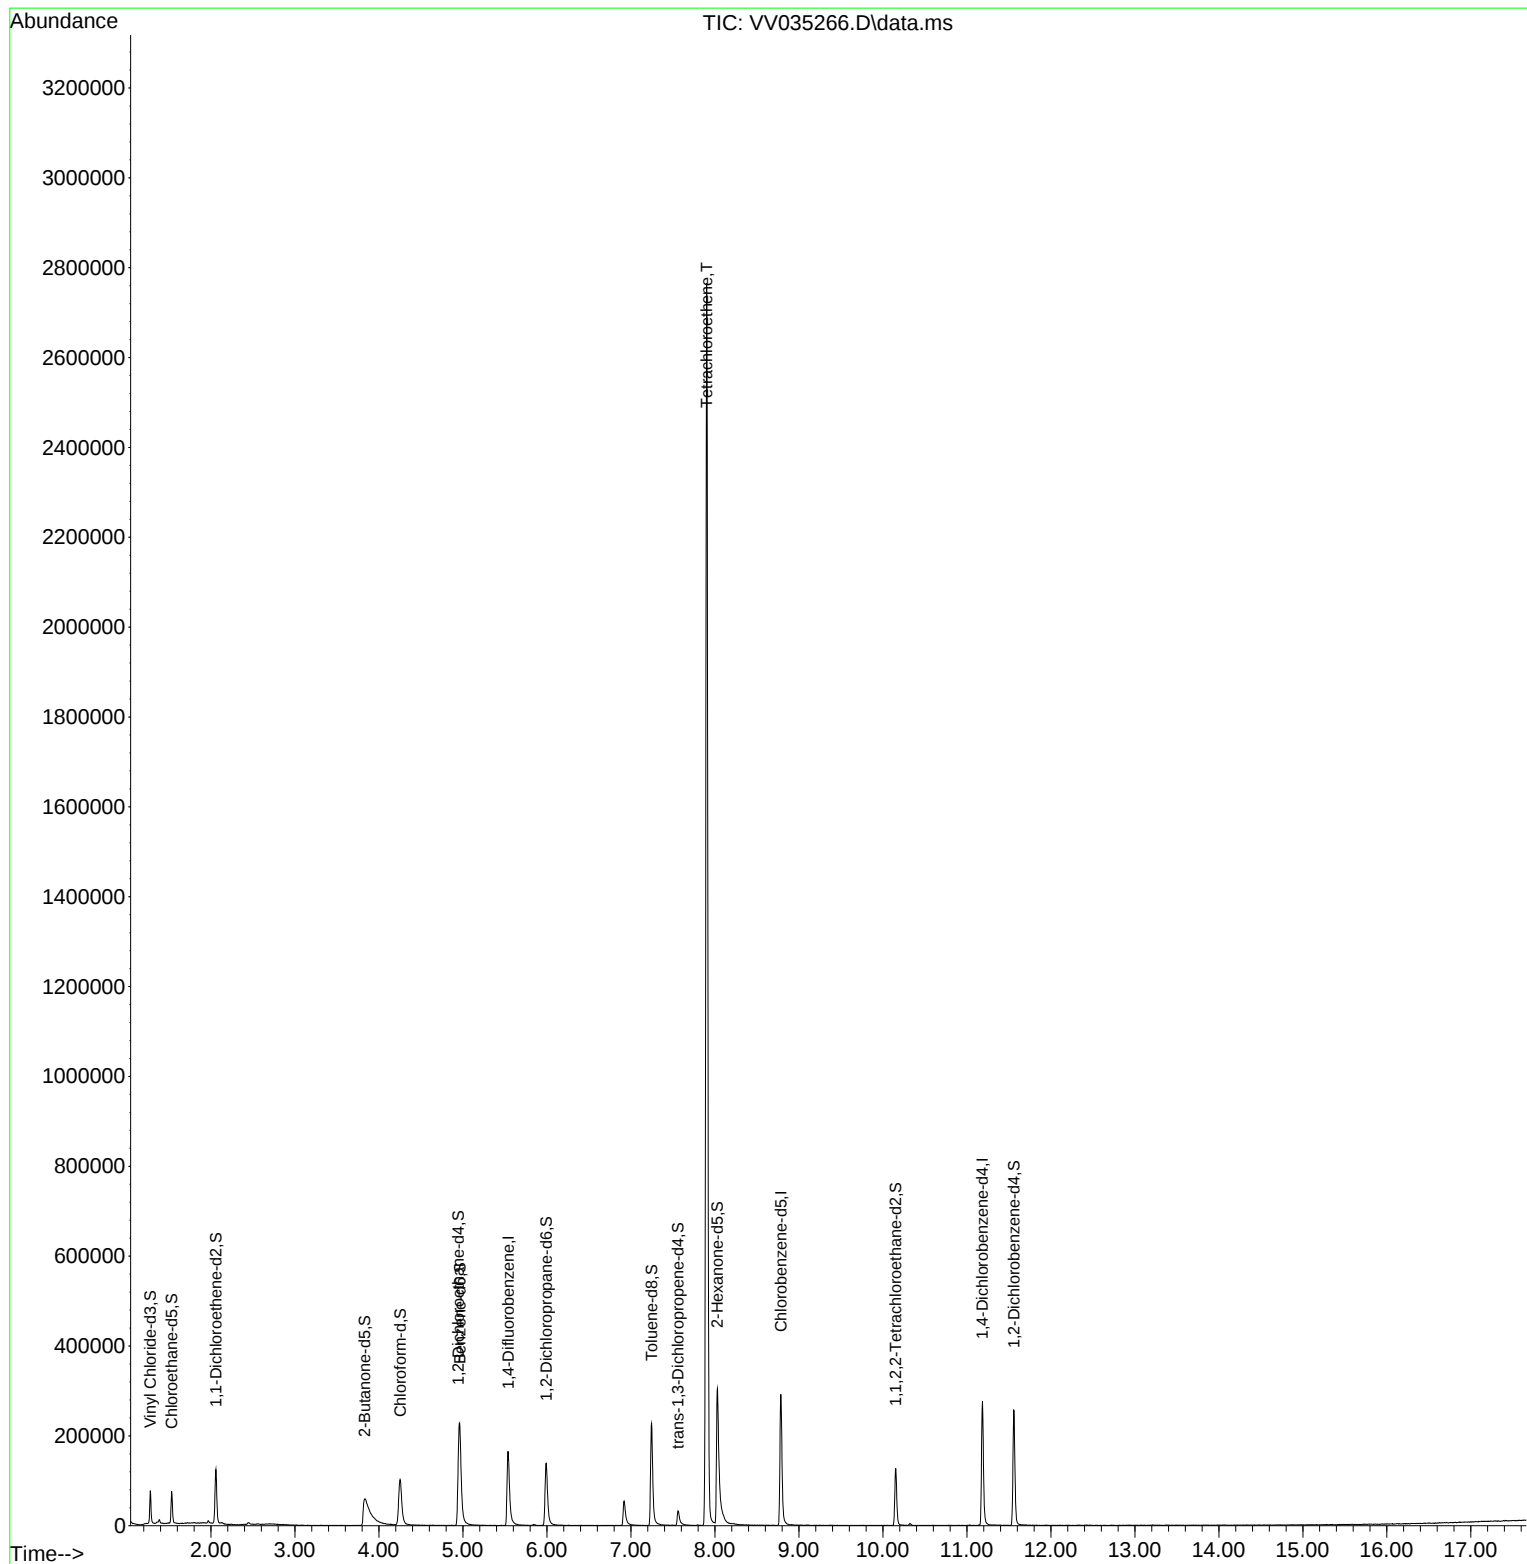

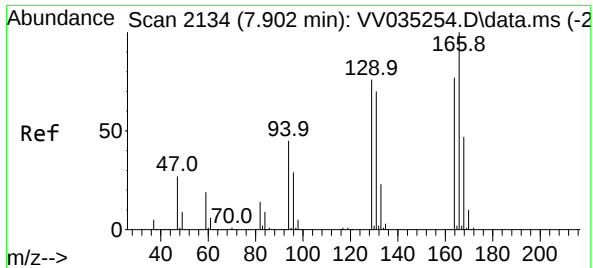

#47
 Tetrachloroethene
 Concen: 54.823 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035266.D
 Acq: 17 Apr 2024 14:10

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP0

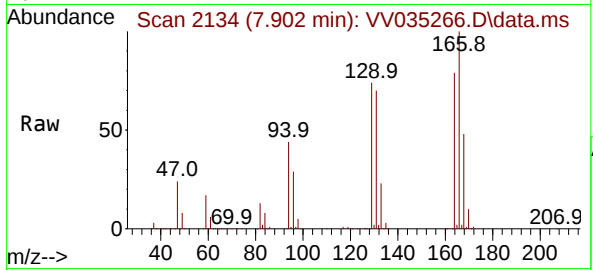

Tgt Ion:	164	Resp:	621193
Ion	Ratio	Lower	Upper
164	100		
129	93.4	65.3	121.3
131	89.1	60.9	113.1
166	126.6	87.4	162.4

