

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
 Data File : VV035259.D
 Acq On : 17 Apr 2024 11:29
 Operator : SY/MD
 Sample : P2100-02DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	107933	117429	17.28%	1.880%
2	1.532	146	153	165	rVB	93345	109500	16.11%	1.753%
3	2.056	306	316	328	rBV	176296	254770	37.48%	4.078%
4	2.445	426	437	454	rBV	38653	66649	9.81%	1.067%
5	3.828	853	867	921	rBV4	64536	339758	49.99%	5.439%
6	4.249	982	998	1026	rBV	115458	301641	44.38%	4.829%
7	4.957	1203	1218	1247	rBV2	263100	679679	100.00%	10.880%
8	5.535	1384	1398	1431	rBV	210501	462745	68.08%	7.407%
9	5.834	1479	1491	1524	rBV	217339	463324	68.17%	7.417%
10	5.989	1524	1539	1571	rVV2	154816	334467	49.21%	5.354%
11	6.918	1818	1828	1851	rBV2	61461	128956	18.97%	2.064%
12	7.243	1916	1929	1962	rBV	281169	514458	75.69%	8.235%
13	7.561	2019	2028	2051	rBV2	34499	74340	10.94%	1.190%
14	7.908	2128	2136	2154	rVB3	10981	19459	2.86%	0.311%
15	8.030	2165	2174	2222	rBV	262658	650811	95.75%	10.418%
16	8.783	2397	2408	2437	rBV	338555	590057	86.81%	9.445%
17	10.153	2823	2834	2859	rBV	121438	199124	29.30%	3.187%
18	11.185	3143	3155	3182	rBV	308445	501811	73.83%	8.033%
19	11.558	3258	3271	3299	rBV	264635	438050	64.45%	7.012%




Sum of corrected areas: 6247028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035259.D
Acq On : 17 Apr 2024 11:29
Operator : SY/MD
Sample : P2100-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

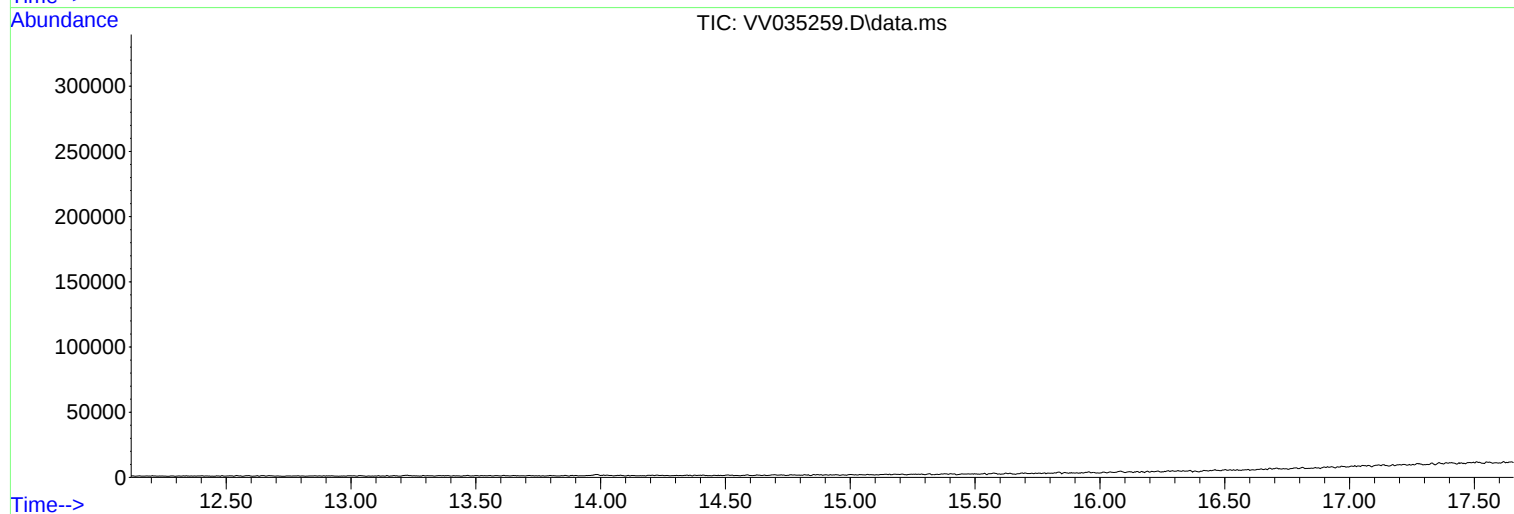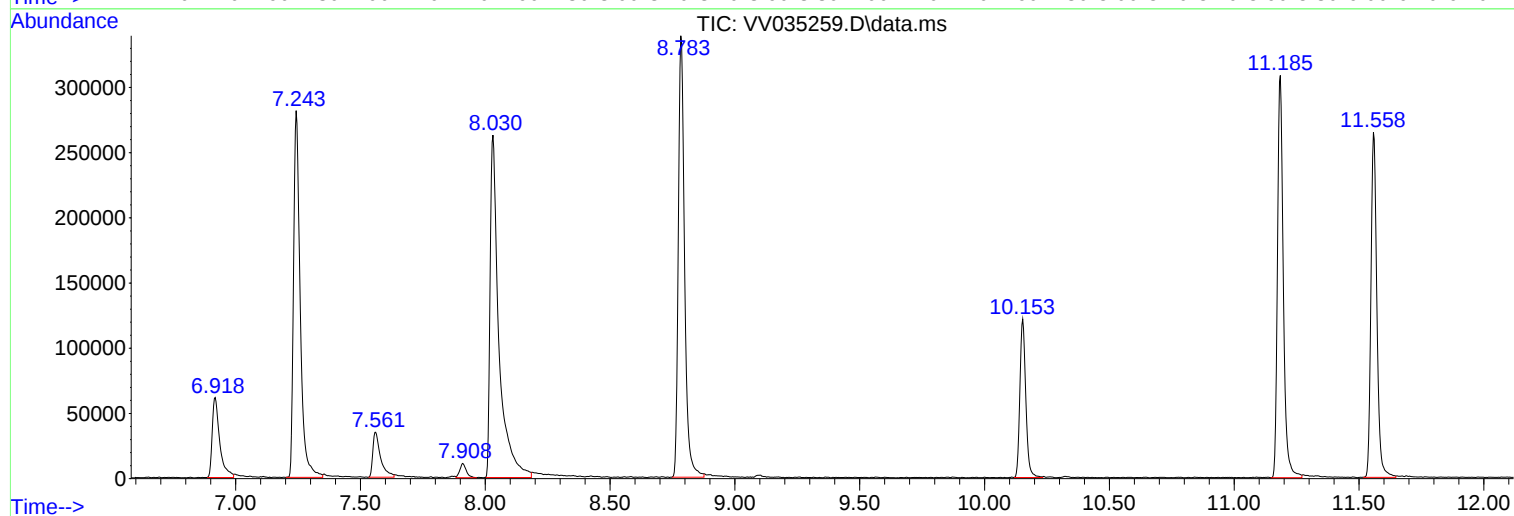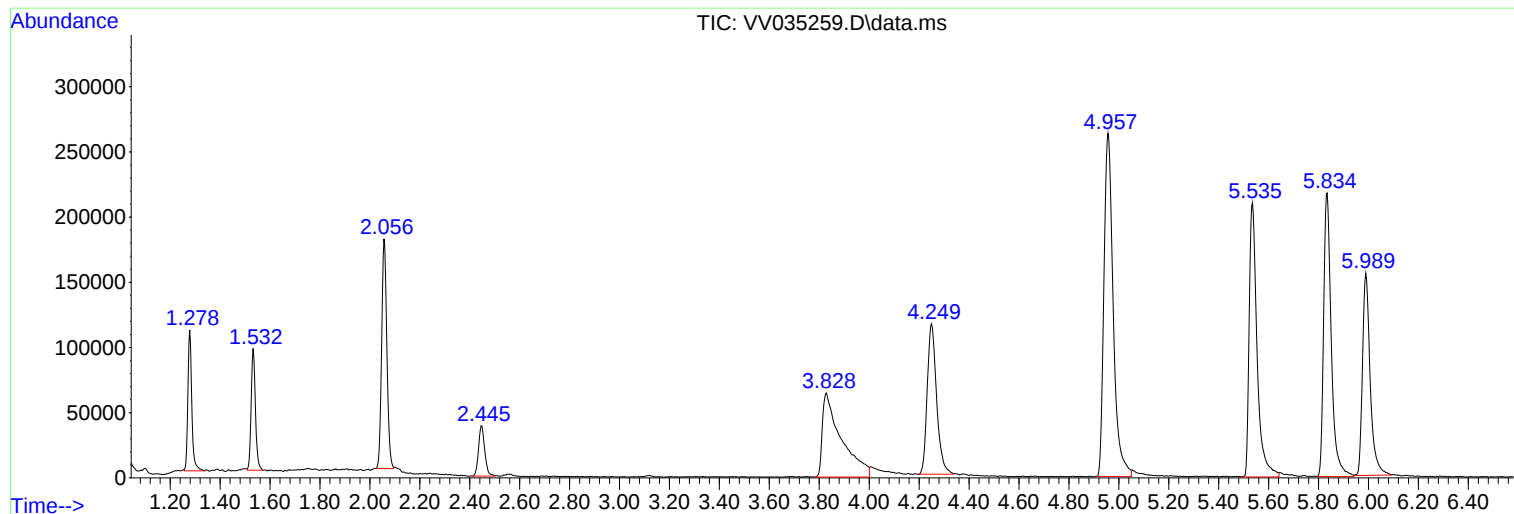

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035259.D
Acq On : 17 Apr 2024 11:29
Operator : SY/MD
Sample : P2100-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035259.D
Acq On : 17 Apr 2024 11:29
Operator : SY/MD
Sample : P2100-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
