


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041724\
Data File : VV035253.D
Acq On : 17 Apr 2024 08:25
Operator : SY/MD
Sample : BFB270
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB270

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 18 00:40:19 2024

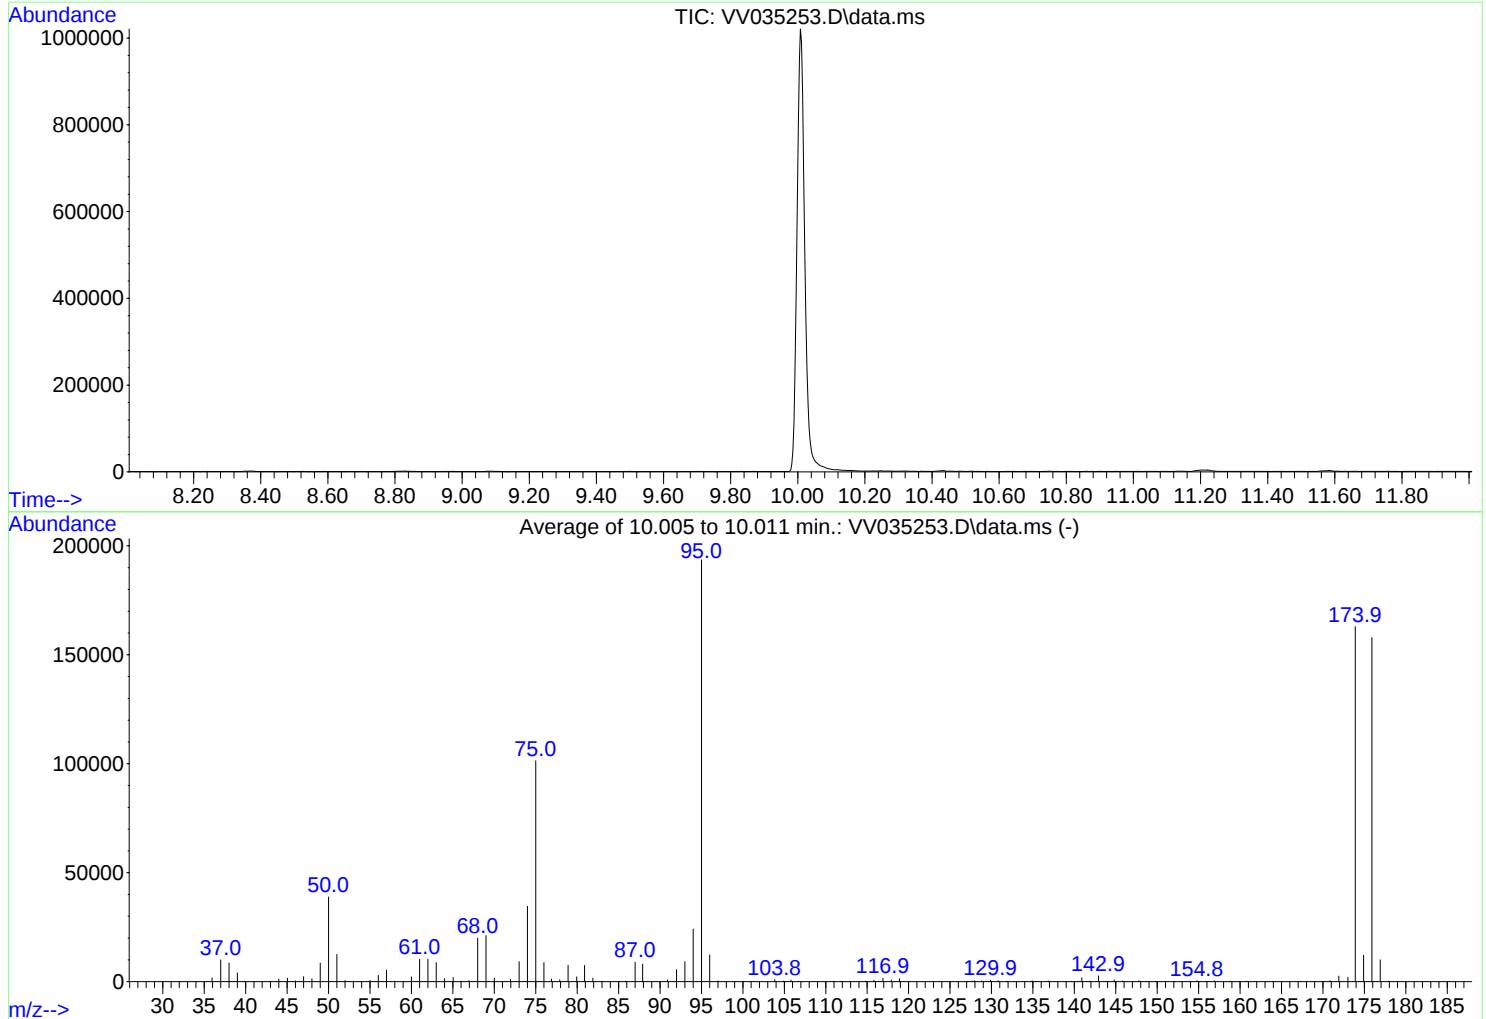

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	38843	PASS
75	95	30	80	52.4	101341	PASS
95	95	100	100	100.0	193579	PASS
96	95	5	9	6.3	12264	PASS
173	174	0.00	2	1.2	2015	PASS
174	95	50	120	84.2	162944	PASS
175	174	5	9	7.5	12154	PASS
176	174	95	105	96.9	157867	PASS
177	176	5	10	6.3	10012	PASS

Scan 2776 (9.966 min): VV035253.D\data.ms
BFB270

m/z	Abundance
35.80	109.0
40.00	210.0
44.10	496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
36.00	1790.0
37.00	9906.0
38.00	8592.0
39.00	4000.0
39.90	425.0
42.90	137.0
44.00	1623.0
45.00	1588.0
46.00	358.0
47.00	2308.0
48.00	1296.0
49.00	8256.0
50.00	37984.0
51.00	11857.0
52.00	630.0
53.00	277.0
53.90	176.0
55.00	532.0
56.00	2672.0
57.00	5069.0
58.00	207.0
59.00	101.0
60.00	2210.0
61.00	10024.0
62.00	10127.0
63.00	8524.0
64.00	1394.0
65.10	1933.0
66.00	212.0
67.00	519.0
68.00	19624.0
69.00	20584.0
70.00	1578.0
72.00	981.0
73.00	9005.0
74.00	33216.0
75.00	98176.0
76.00	8496.0
76.90	1121.0
77.90	897.0
78.90	7333.0
79.90	2153.0
80.90	7373.0
81.90	1551.0
83.00	216.0
85.90	292.0
87.00	8401.0
87.90	7966.0
90.90	764.0
92.00	5213.0
93.00	8620.0
94.00	22936.0
95.00	186816.0
96.00	12265.0
97.00	367.0
103.90	863.0
104.90	338.0
105.80	745.0
106.80	152.0
110.00	109.0
110.90	191.0
111.90	140.0
112.90	183.0
114.80	197.0
115.80	567.0
116.90	1487.0
117.90	726.0
118.90	1246.0
125.90	105.0
127.70	619.0
128.80	334.0
129.90	557.0
130.80	412.0
134.90	271.0
136.80	302.0
139.60	118.0
140.10	118.0
140.90	1676.0
141.90	218.0
142.90	2647.0
143.80	204.0
144.80	804.0
145.80	331.0
147.10	127.0
147.80	427.0
148.70	192.0
149.80	206.0
152.00	103.0
152.90	134.0
154.00	166.0
154.80	424.0
155.80	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

156.90	291.0
158.80	218.0
160.80	210.0
170.90	423.0
171.90	2443.0
173.00	1945.0
173.90	155136.0
174.90	11527.0
175.90	148800.0
176.90	9820.0
178.00	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
36.00	1898.0
37.00	10412.0
38.00	8828.0
39.00	4239.0
39.90	433.0
42.00	106.0
42.90	121.0
44.00	1701.0
45.10	1603.0
46.00	360.0
47.00	2385.0
48.00	1451.0
49.00	8858.0
50.00	40128.0
51.00	13007.0
52.00	564.0
53.00	323.0
53.90	173.0
55.00	564.0
56.00	2933.0
57.00	5469.0
57.90	316.0
60.00	2263.0
61.00	10508.0
62.00	10617.0
63.00	9134.0
64.00	1418.0
65.00	1982.0
66.00	236.0
66.90	582.0
68.00	20576.0
69.00	21888.0
70.00	1691.0
72.00	1030.0
73.00	9452.0
74.00	35872.0
75.00	104792.0
76.00	9082.0
76.90	1199.0
77.90	883.0
78.90	7742.0
79.90	2280.0
80.90	7577.0
81.90	1606.0
83.00	200.0
85.80	292.0
87.00	9185.0
87.90	8425.0
90.90	796.0
92.00	5691.0
93.00	9532.0
94.00	25040.0
95.00	200064.0
96.00	12525.0
97.00	391.0
103.80	979.0
104.90	311.0
105.80	775.0
106.70	163.0
109.90	120.0
110.90	206.0
111.90	186.0
112.90	181.0
114.80	195.0
115.80	665.0
116.90	1570.0
117.90	732.0
118.90	1397.0
125.90	134.0
127.90	658.0
128.80	379.0
129.90	679.0
130.80	422.0
131.80	104.0
134.90	352.0
136.90	354.0
139.70	125.0
140.00	137.0
140.90	1781.0
141.90	215.0
142.90	2821.0
143.80	182.0
144.80	875.0
145.80	367.0
147.00	146.0
147.80	447.0
148.70	171.0
149.80	170.0
152.90	142.0
153.90	176.0
154.80	470.0
155.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

156.90	403.0
158.80	253.0
160.80	220.0
170.80	446.0
171.90	2705.0
173.00	2102.0
173.90	168256.0
174.90	12654.0
175.90	163776.0
176.90	10338.0
178.00	278.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
36.00	1825.0
37.00	9746.0
38.00	8351.0
39.00	3935.0
39.90	449.0
42.00	157.0
42.90	118.0
44.00	1682.0
45.00	1563.0
46.00	328.0
47.00	2256.0
48.00	1341.0
49.00	8509.0
50.00	38416.0
51.00	12659.0
52.00	465.0
53.00	345.0
53.90	171.0
55.00	548.0
56.00	3006.0
57.00	5277.0
57.90	366.0
60.00	2064.0
61.00	10119.0
62.00	10276.0
63.00	8584.0
64.00	1319.0
65.00	1915.0
66.00	208.0
66.90	577.0
68.00	19736.0
69.00	21032.0
70.00	1614.0
71.90	1046.0
73.00	9010.0
74.00	34592.0
75.00	101056.0
76.00	8583.0
76.90	1137.0
77.90	924.0
78.90	7390.0
80.00	2142.0
80.90	7218.0
81.90	1606.0
83.00	159.0
85.90	264.0
87.00	8981.0
87.90	7920.0
90.90	796.0
92.00	5744.0
93.00	9455.0
94.00	24216.0
95.00	193856.0
96.00	12002.0
97.00	369.0
103.80	932.0
104.90	258.0
105.80	776.0
106.70	189.0
109.90	126.0
110.90	192.0
111.80	191.0
112.90	189.0
114.80	183.0
115.80	731.0
116.90	1484.0
117.90	691.0
118.90	1346.0
122.80	123.0
126.00	125.0
127.00	112.0
128.00	664.0
128.80	376.0
129.90	799.0
130.80	428.0
134.90	384.0
136.90	349.0
140.00	117.0
140.90	1735.0
141.80	215.0
142.90	2543.0
143.80	130.0
144.80	828.0
145.80	349.0
147.00	138.0
147.80	432.0
148.70	136.0
149.80	125.0
153.00	126.0
153.90	162.0
154.80	468.0
155.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

156.90	443.0
158.80	279.0
160.80	203.0
170.80	396.0
171.90	2592.0
173.00	1997.0
173.90	165440.0
174.90	12280.0
175.90	161024.0
176.90	9879.0
177.90	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270