

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041819\
 Data File : VV010406.D
 Acq On : 20 Apr 2019 01:53
 Operator : SY/MD
 Sample : K2456-23
 Misc : 5.09G/10mL/MSVOA V/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAHP1

Quant Time: Apr 20 04:39:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041819S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 20 04:30:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.68	114	1563	25.00	ug/L	0.02
28) Chlorobenzene-d5	8.89	117	162	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.32	152	250	25.00	ug/L	0.02

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	1100	55.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	221.68%#
7) Chloroethane-d5	1.59	69	706	42.35	ug/L	0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	169.40%#
10) 1,1-Dichloroethene-d2	2.14	63	1472	30.74	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	122.96%#
20) 2-Butanone-d5	0.00	46	0	0.00	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.00%#
24) Chloroform-d	4.38	84	268	6.52	ug/L	-0.02
Spiked Amount	25.000	Range	40 - 150	Recovery	=	26.08%#
26) 1,2-Dichloroethane-d4	5.09	65	243	10.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	40.08%#
29) Benzene-d6	5.10	84	2770	334.04	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	1336.16%#
33) 1,2-Dichloropropane-d6	6.12	67	813	335.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	1340.00%#
37) Toluene-d8	7.37	98	1165	146.14	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	=	584.56%#
38) trans-1,3-Dichloropropene-	7.69	79	51	42.73	ug/L	0.04
Spiked Amount	25.000	Range	30 - 135	Recovery	=	170.92%#
39) 2-Hexanone-d5	8.14	63	40	74.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	148.04%#
48) 1,1,2,2-Tetrachloroethane-	10.28	84	385	158.62	ug/L	0.02
Spiked Amount	25.000	Range	45 - 120	Recovery	=	634.48%#
61) 1,2-Dichlorobenzene-d4	11.68	152	212	21.57	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.28%

Target Compounds

					Ovalue
3) Chloromethane	1.25	50	146	7.086	ug/L # 41
5) Vinyl chloride	1.13	62	43	1.998	ug/L # 41
6) Bromomethane	1.54	94	153	11.113	ug/L 100
8) Chloroethane	1.59	64	130	9.476	ug/L # 44
13) Acetone	2.20	43	75	11.498	ug/L # 45
15) Methyl Acetate	2.48	43	42	3.945	ug/L # 47
16) Methylene chloride	2.55	84	51	2.043	ug/L 83
17) Methyl tert-butyl Ether	2.95	73	44	0.900	ug/L # 1
21) 2-Butanone	4.13	43	19	2.687	ug/L # 49
22) cis-1,2-Dichloroethene	4.13	96	51	2.324	ug/L # 1
36) Methylcyclohexane	6.12	83	167	49.035	ug/L # 21
40) 1,2-Dichloropropane	6.11	63	51	25.153	ug/L # 86
43) 4-Methyl-2-pentanone	7.08	43	44	27.776	ug/L # 1
49) 2-Hexanone	8.10	43	57	51.406	ug/L # 37
69) Naphthalene	13.57	128	1345	71.867	ug/L # 73


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041819\
Data File : VV010406.D
Acq On : 20 Apr 2019 01:53
Operator : SY/MD
Sample : K2456-23
Misc : 5.09G/10mL/MSVOA V/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAHP1

Quant Time: Apr 20 04:39:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041819S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 20 04:30:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						

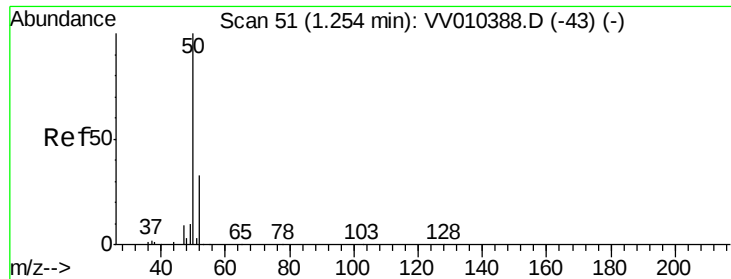

#3

Chloromethane

Concen: 7.086 ug/L

RT: 1.25 min Scan# 50

Delta R.T. -0.00 min

Lab File: VV010406.D

Acq: 20 Apr 2019 01:53

Instrument :

MSVOA_V

ClientSampleId :


GAHP1

Tot Ion: 50 Resp: 146

Ion Ratio Lower Upper

50 100

52 0.0 23.2 43.2#

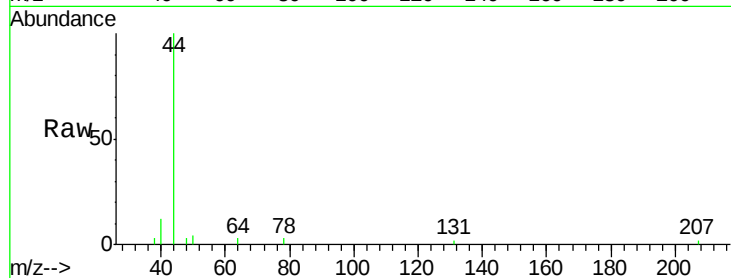

Abundance Ion 50.00 (49.70 to 50.70): VV0

Ion 52.00 (51.70 to 52.70): VV0

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25

1.25



1.25

1.25

1.25

1.25

1.25

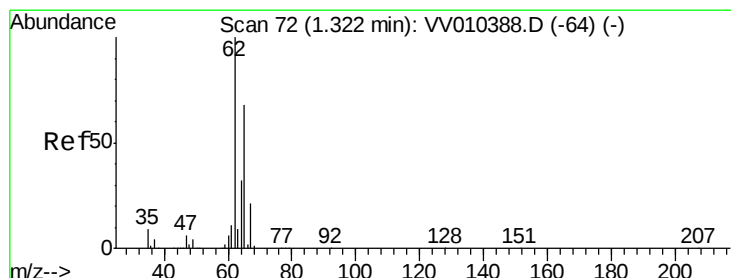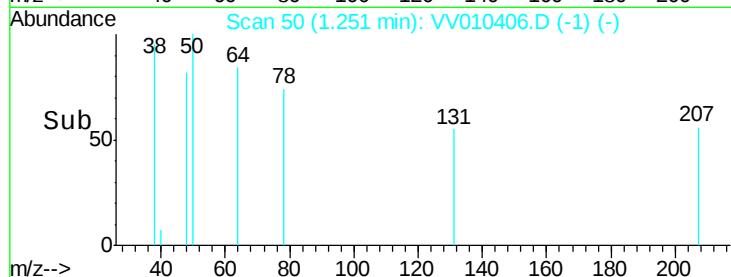

#5

Vinyl chloride

Concen: 1.998 ug/L

RT: 1.13 min Scan# 12

Delta R.T. -0.19 min

Lab File: VV010406.D


Acq: 20 Apr 2019 01:53

Tgt Ion: 62 Resp: 43

Ion Ratio Lower Upper

62 100

64 0.0 23.9 44.3#

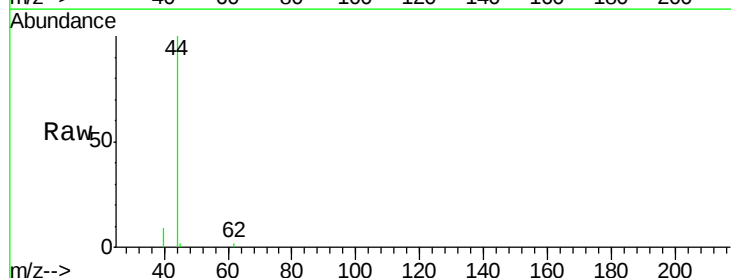

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 64.00 (63.70 to 64.70): VV0

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13

1.13


1.13

1.13


1.13

1.13

1.13

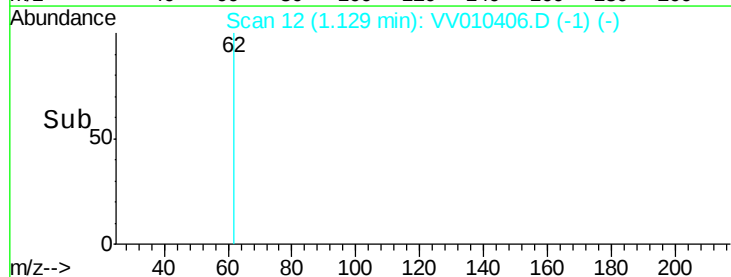

Time-->

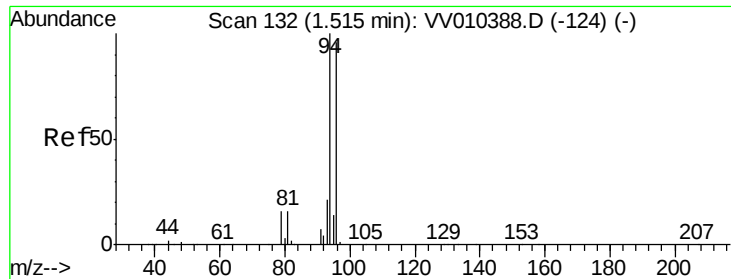

#6

Bromomethane

Concen: 11.113 ug/L

RT: 1.54 min Scan# 140

Delta R.T. 0.03 min

Lab File: VV010406.D

Acq: 20 Apr 2019 01:53





Instrument :
MSVOA_V
ClientSampled :
GAHP1

Tot Ion: 94 Resp: 153

Ion Ratio Lower Upper

94 100

96 93.5 9.3 177.1

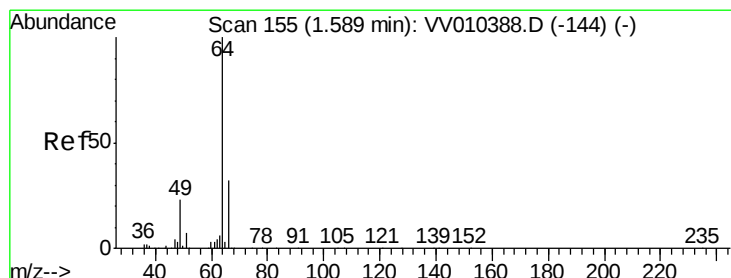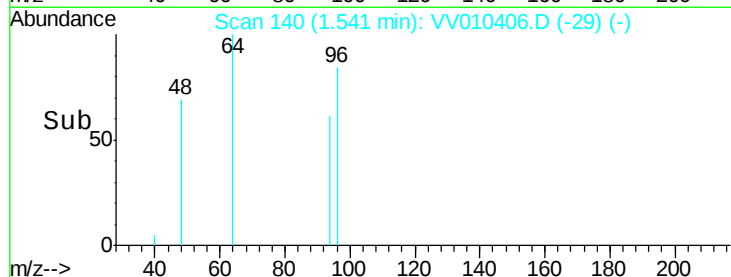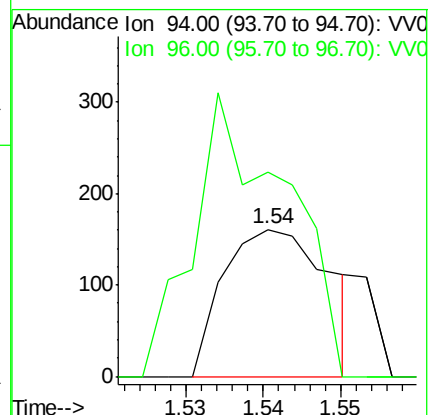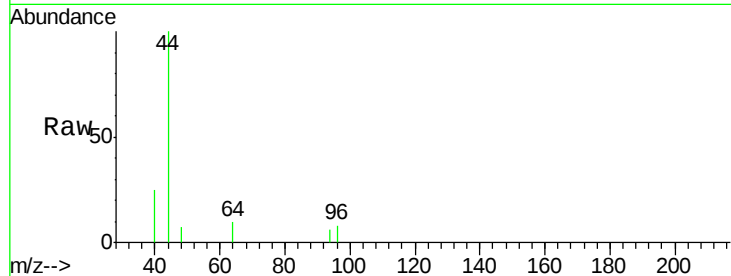

#8

Chloroethane

Concen: 9.476 ug/L

RT: 1.59 min Scan# 156

Delta R.T. 0.00 min

Lab File: VV010406.D




Acq: 20 Apr 2019 01:53


Tgt Ion: 64 Resp: 130

Ion Ratio Lower Upper

64 100

66 0.0 21.4 39.8#

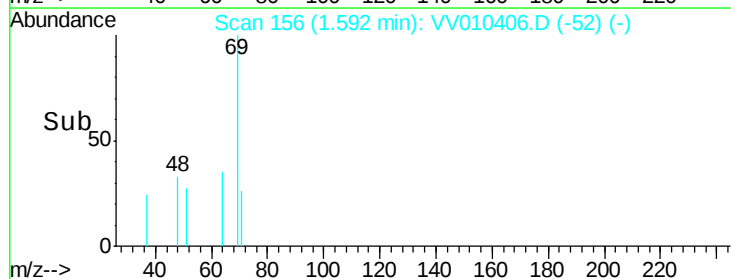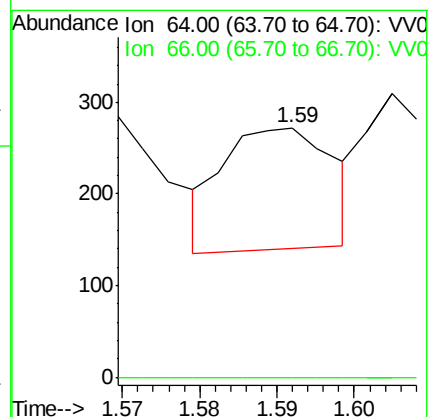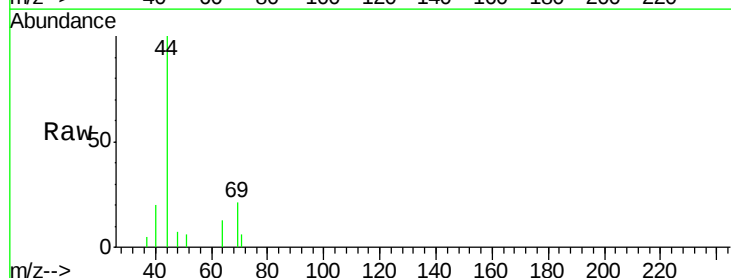

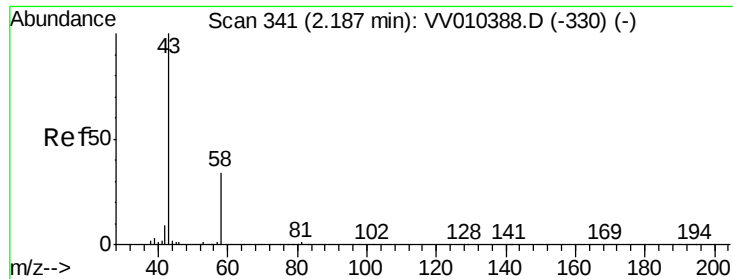

#13

Acetone

Concen: 11.498 ug/L

RT: 2.20 min Scan# 344

Delta R.T. 0.01 min

Lab File: VV010406.D

Acq: 20 Apr 2019 01:53

Instrument :

MSVOA_V

ClientSampled :


GAHP1

Tot Ion: 43 Resp: 75

Ion Ratio Lower Upper

43 100

58 0.0 0.0 60.0

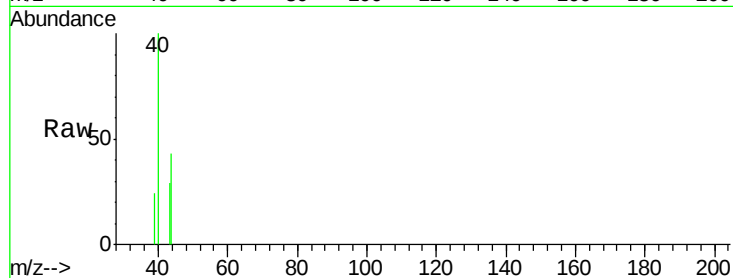

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

150

100

50

0

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21



2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

2.19 2.19 2.19 2.20 2.21

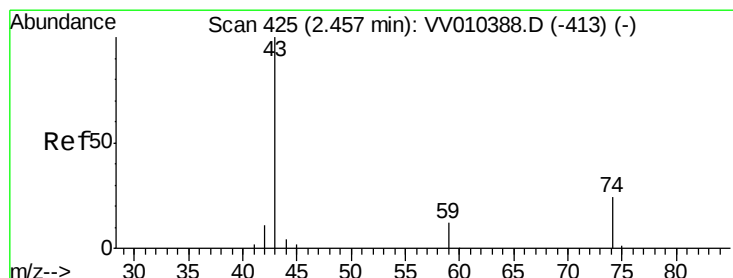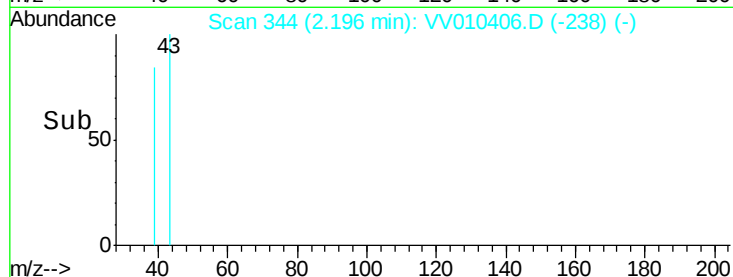

#15

Methyl Acetate

Concen: 3.945 ug/L

RT: 2.48 min Scan# 431

Delta R.T. 0.02 min

Lab File: VV010406.D


Acq: 20 Apr 2019 01:53

Tgt Ion: 43 Resp: 42

Ion Ratio Lower Upper

43 100

74 0.0 22.1 33.1#

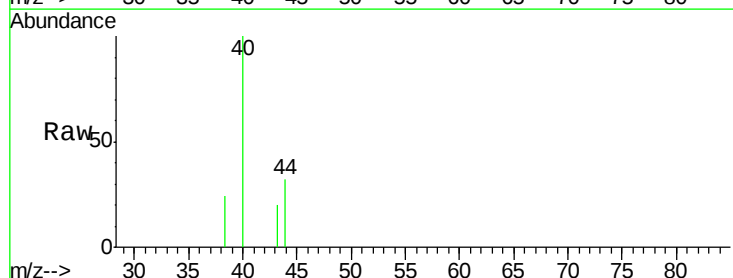

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 74.00 (73.70 to 74.70): VV0

100

50

0

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48


2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

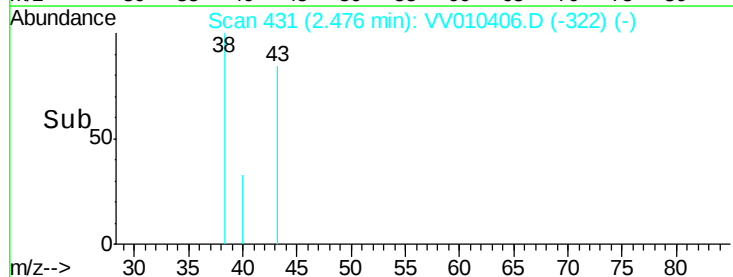

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 74.00 (73.70 to 74.70): VV0

100

50

0

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48


2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48

2.47 2.48 2.48 2.48 2.48





2.47 2.48 2.48 2.48 2.48

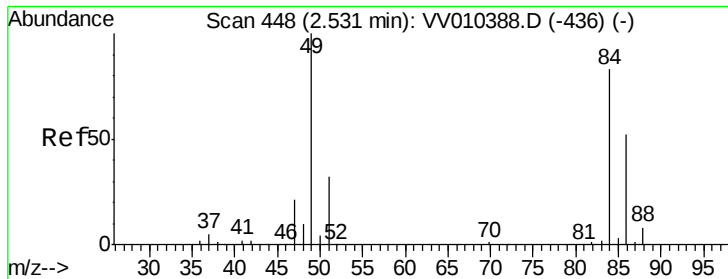

#16
Methylene chloride
Concen: 2.043 ug/L
RT: 2.55 min Scan# 453
Delta R.T. 0.02 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53




Instrument :
MSVOA_V
ClientSampled :
GAHP1


Tot Ion: 84 Resp: 51
Ion Ratio Lower Upper
84 100
49 104.9 83.8 155.6
86 47.9 46.1 85.5

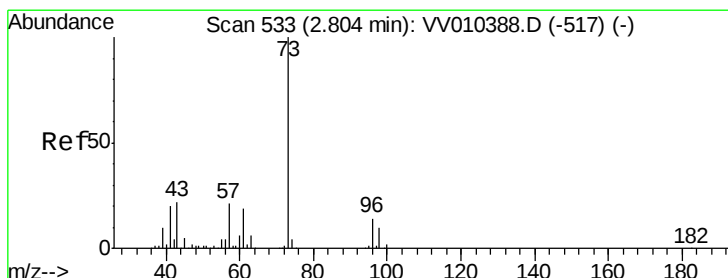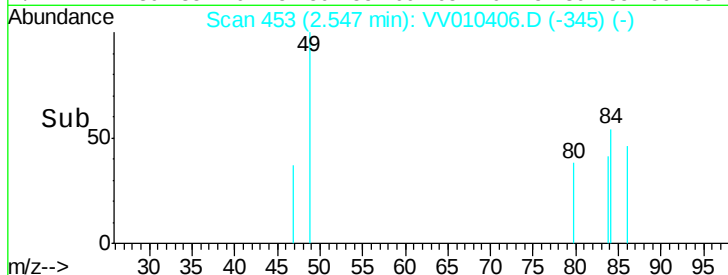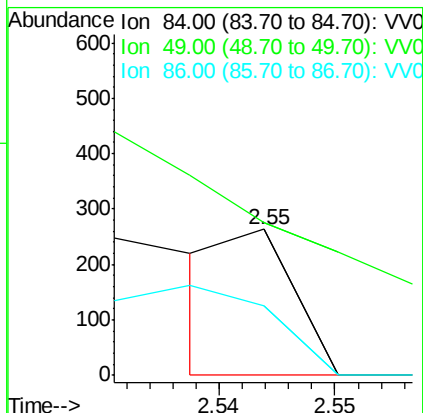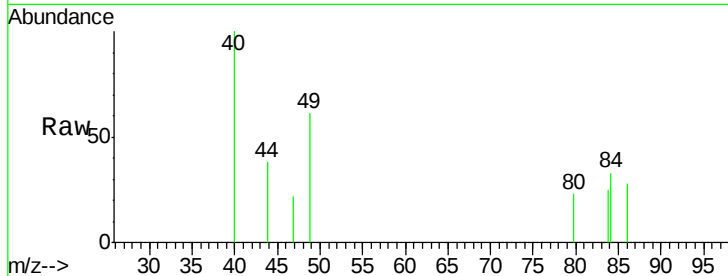

#17
Methyl tert-butyl Ether
Concen: 0.900 ug/L
RT: 2.95 min Scan# 577
Delta R.T. 0.14 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53

Tgt Ion: 73 Resp: 44
Ion Ratio Lower Upper
73 100
43 154.5 16.6 24.8#
57 0.0 17.0 25.6#

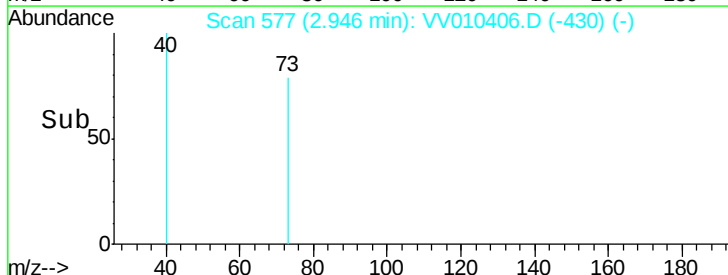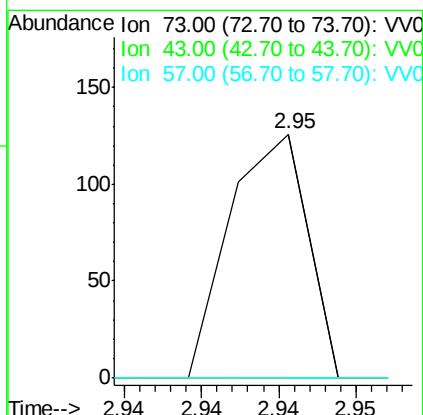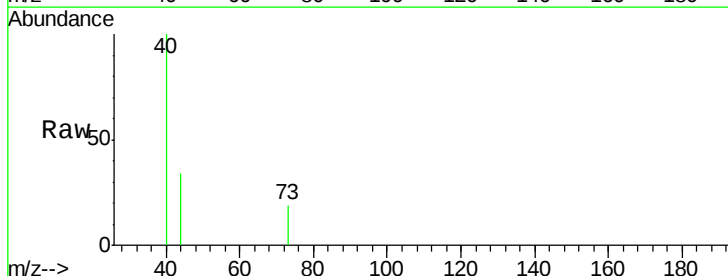

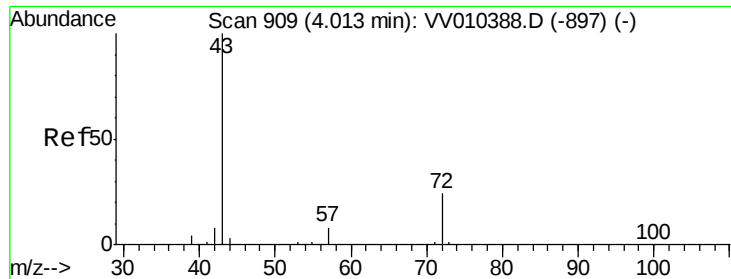

#21

2-Butanone

Concen: 2.687 ug/L

RT: 4.13 min Scan# 946

Delta R.T. 0.12 min

Lab File: VV010406.D

Acq: 20 Apr 2019 01:53

Instrument :

MSVOA_V

ClientSampled :





GAHP1

Tot Ion: 43 Resp: 19

Ion Ratio Lower Upper

43 100

72 0.0 13.1 39.1#

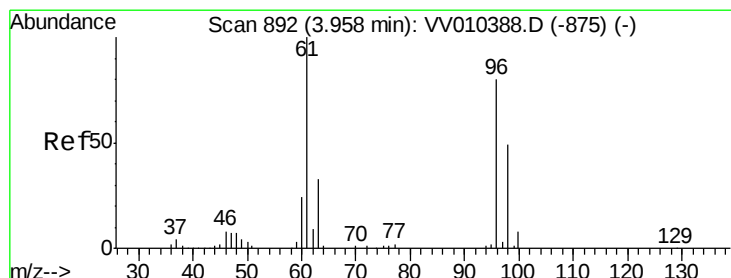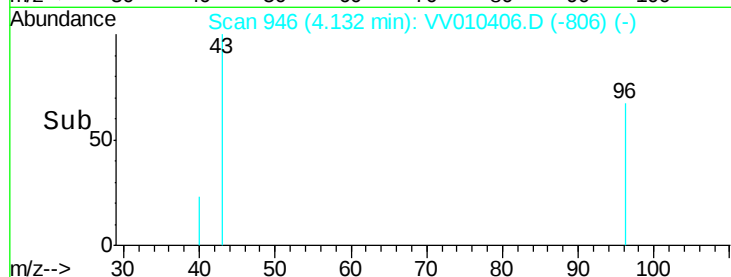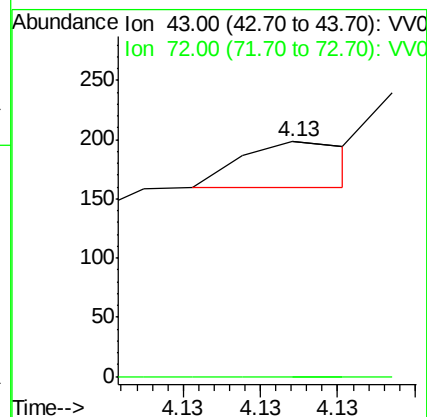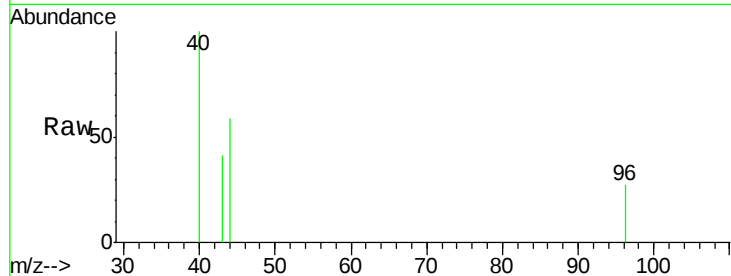

#22

cis-1,2-Dichloroethene

Concen: 2.324 ug/L

RT: 4.13 min Scan# 946

Delta R.T. 0.17 min

Lab File: VV010406.D

Acq: 20 Apr 2019 01:53




Tgt Ion: 96 Resp: 51


Ion Ratio Lower Upper

96 100

61 0.0 83.7 155.4#

98 0.0 43.7 81.1#

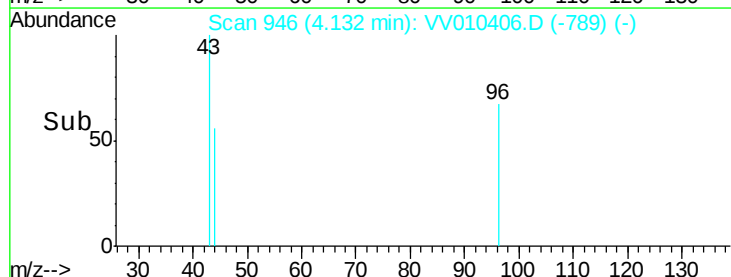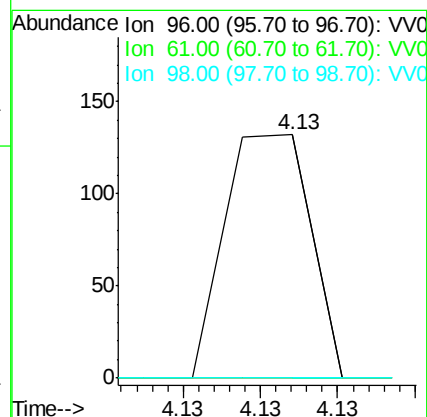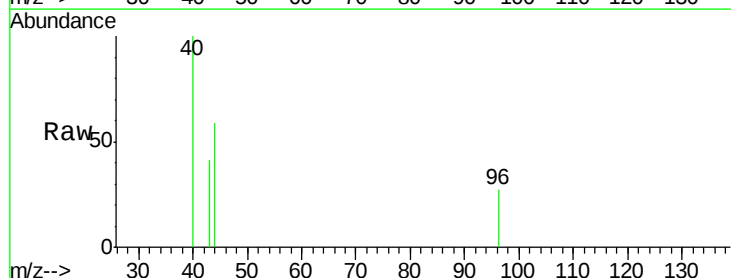




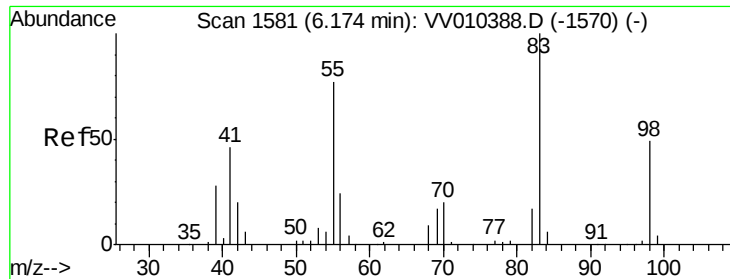


#36
Methvlcvclohexane
Concen: 49.035 ug/L
RT: 6.12 min Scan# 1565
Delta R.T. -0.05 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53

Instrument :
MSVOA_V
ClientSampled :
GAHP1

Tot Ion: 83 Resp: 167




Ion	Ratio	Lower	Upper
83	100		
55	0.0	55.9	83.9#
98	0.0	37.3	55.9#

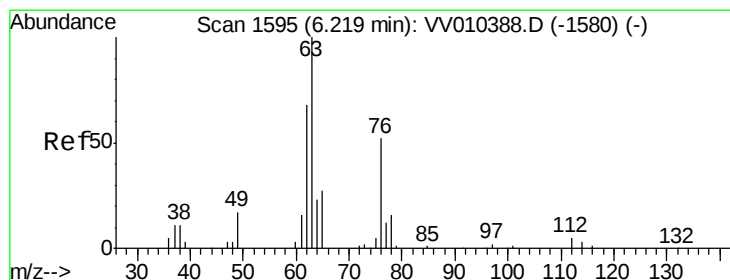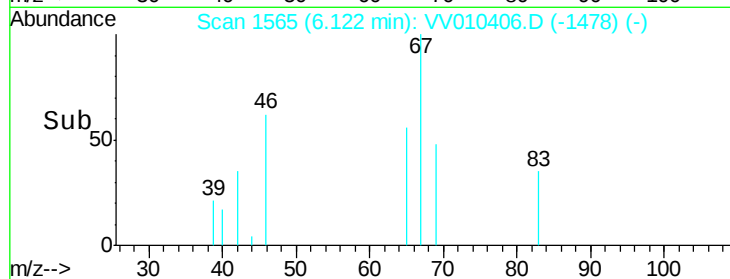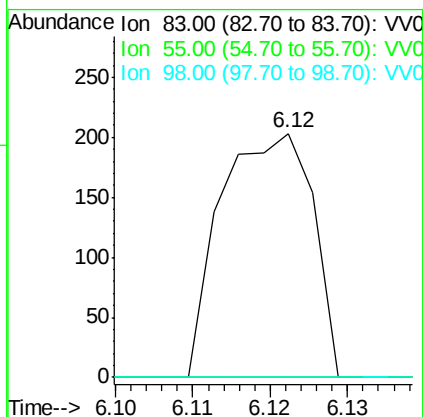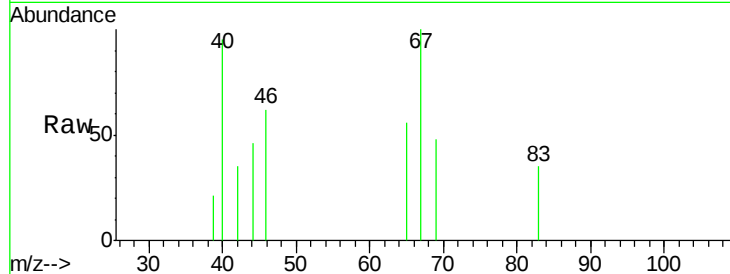


#40
1,2-Dichloropropane
Concen: 25.153 ug/L
RT: 6.11 min Scan# 1562
Delta R.T. -0.11 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53

Tgt Ion: 63 Resp: 51

Ion	Ratio	Lower	Upper
63	100		
112	0.0	3.6	5.4#


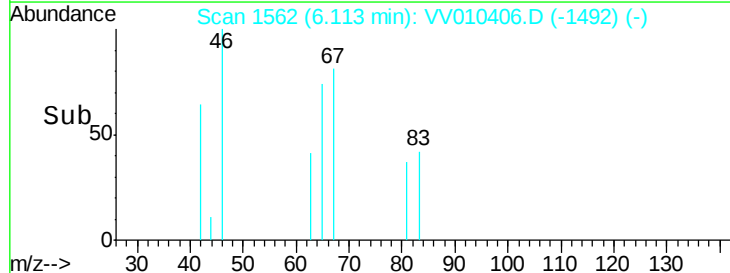
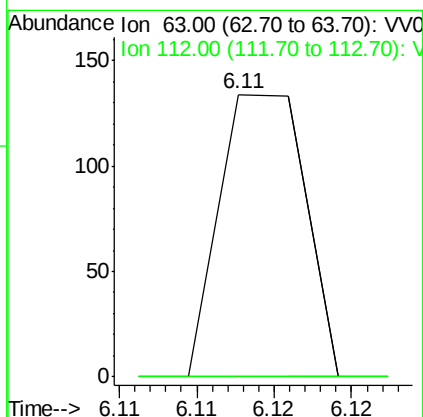
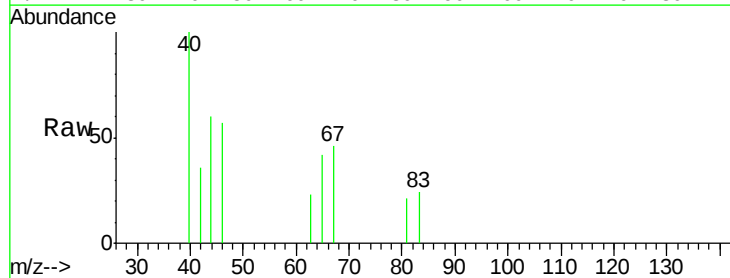


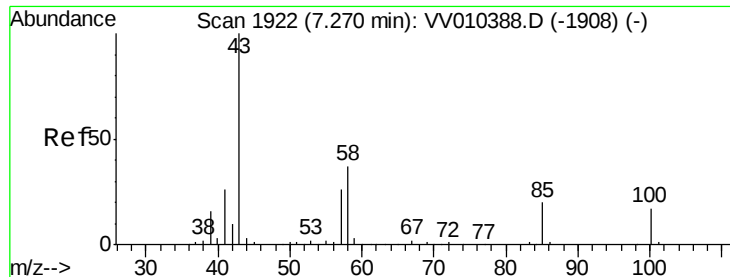

#43
4-Methyl-2-pentanone
Concen: 27.776 ug/L
RT: 7.08 min Scan# 1864
Delta R.T. -0.19 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53




Instrument :
MSVOA_V
ClientSampleId :
GAHP1


Tot Ion: 43 Resp: 44
Ion Ratio Lower Upper
43 100
58 0.0 30.0 45.0#
100 1881.8 12.6 19.0#

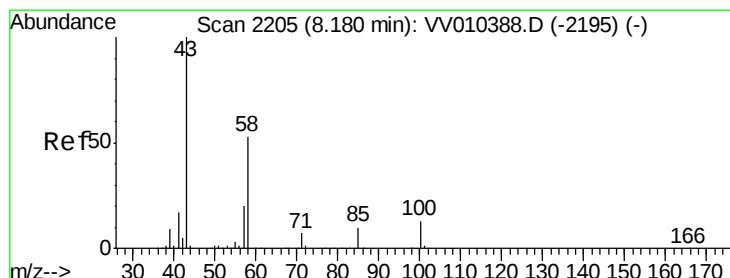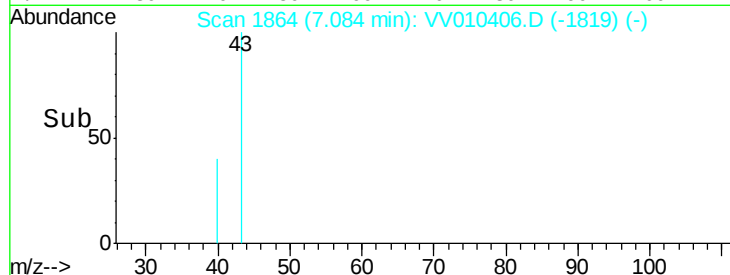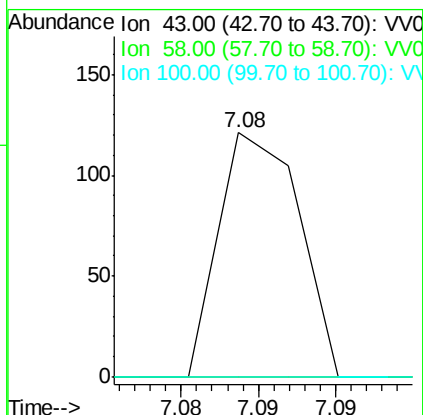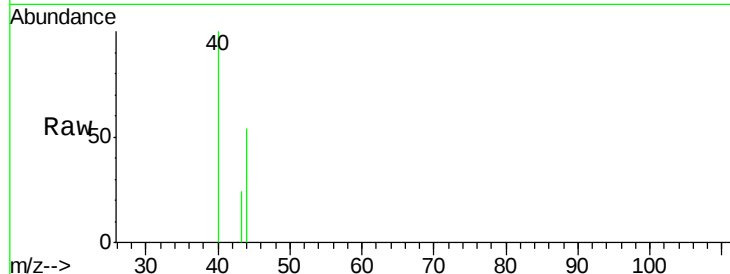

#49
2-Hexanone
Concen: 51.406 ug/L
RT: 8.10 min Scan# 2180
Delta R.T. -0.08 min
Lab File: VV010406.D
Acq: 20 Apr 2019 01:53

Tgt Ion: 43 Resp: 57
Ion Ratio Lower Upper
43 100
58 0.0 44.9 67.3#
57 0.0 15.8 23.6#
100 0.0 10.1 15.1#

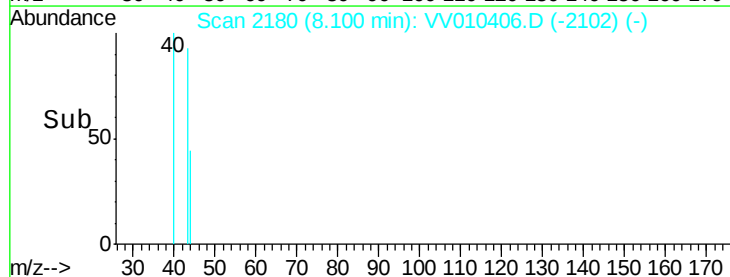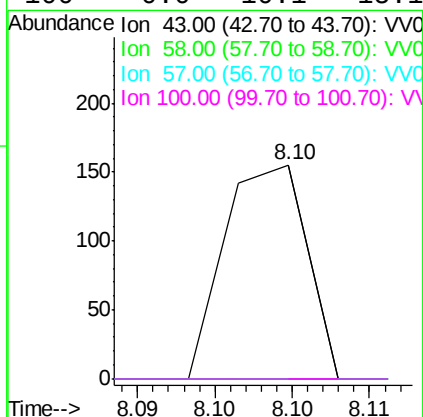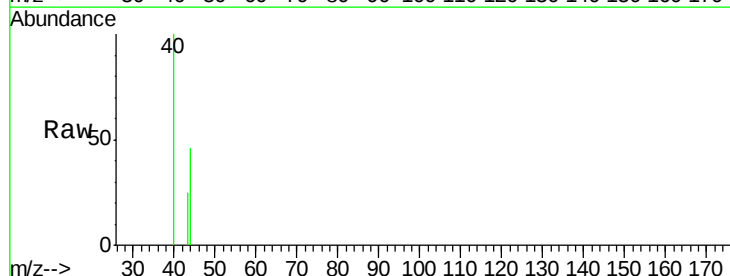

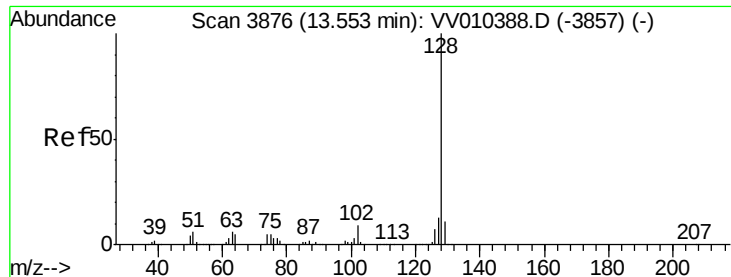

#69

Naphthalene

Concen: 71.867 ug/L

RT: 13.57 min Scan# 3880

Delta R.T. 0.01 min

Lab File: VV010406.D


Acq: 20 Apr 2019 01:53

Instrument :

MSVOA_V

ClientSampleId :

GAHP1

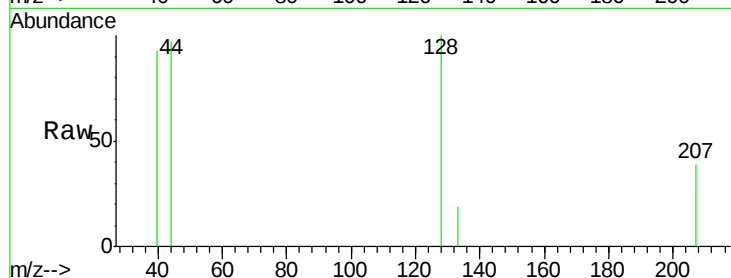


Tot Ion:128 Resp: 1345

Ion Ratio Lower Upper

128 100

129 0.0 8.7 13.1#

127 3.4 10.7 16.1#

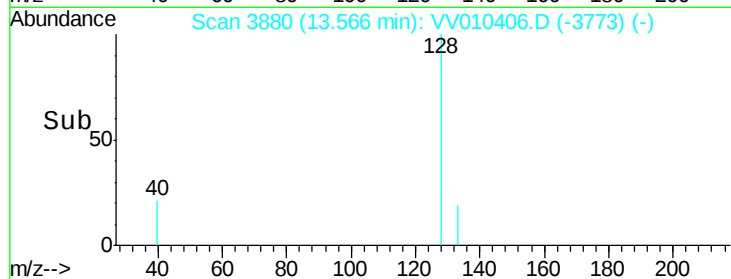

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

