

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030620.D
 Acq On : 18 Apr 2023 16:17
 Operator : SY/MD
 Sample : 02360-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP2

Quant Time: Apr 19 01:46:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	232907	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	224785	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	115978	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	66219	38.784	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.560%
7) Chloroethane-d5	1.536	69	57008	39.844	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.680%
11) 1,1-Dichloroethene-d2	2.066	65	34464	42.564	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.120%
21) 2-Butanone-d5	3.796	46	84250	89.838	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.840%
24) Chloroform-d	4.259	84	135144	43.677	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.360%
26) 1,2-Dichloroethane-d4	4.950	65	89645	45.063	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.120%
32) Benzene-d6	4.970	84	243644	45.845	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.680%
36) 1,2-Dichloropropane-d6	5.995	67	79365	48.076	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.160%
41) Toluene-d8	7.252	98	213901	42.867	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.740%
43) trans-1,3-Dichloroprop...	7.558	79	37244	44.762	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.520%
47) 2-Hexanone-d5	8.034	63	52292	80.408	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.410%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	108226	45.180	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.360%
66) 1,2-Dichlorobenzene-d4	11.571	152	86323	46.827	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.660%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.841	95	158095	89.042	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030620.D
Acq On : 18 Apr 2023 16:17
Operator : SY/MD
Sample : 02360-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP2


Quant Time: Apr 19 01:46:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

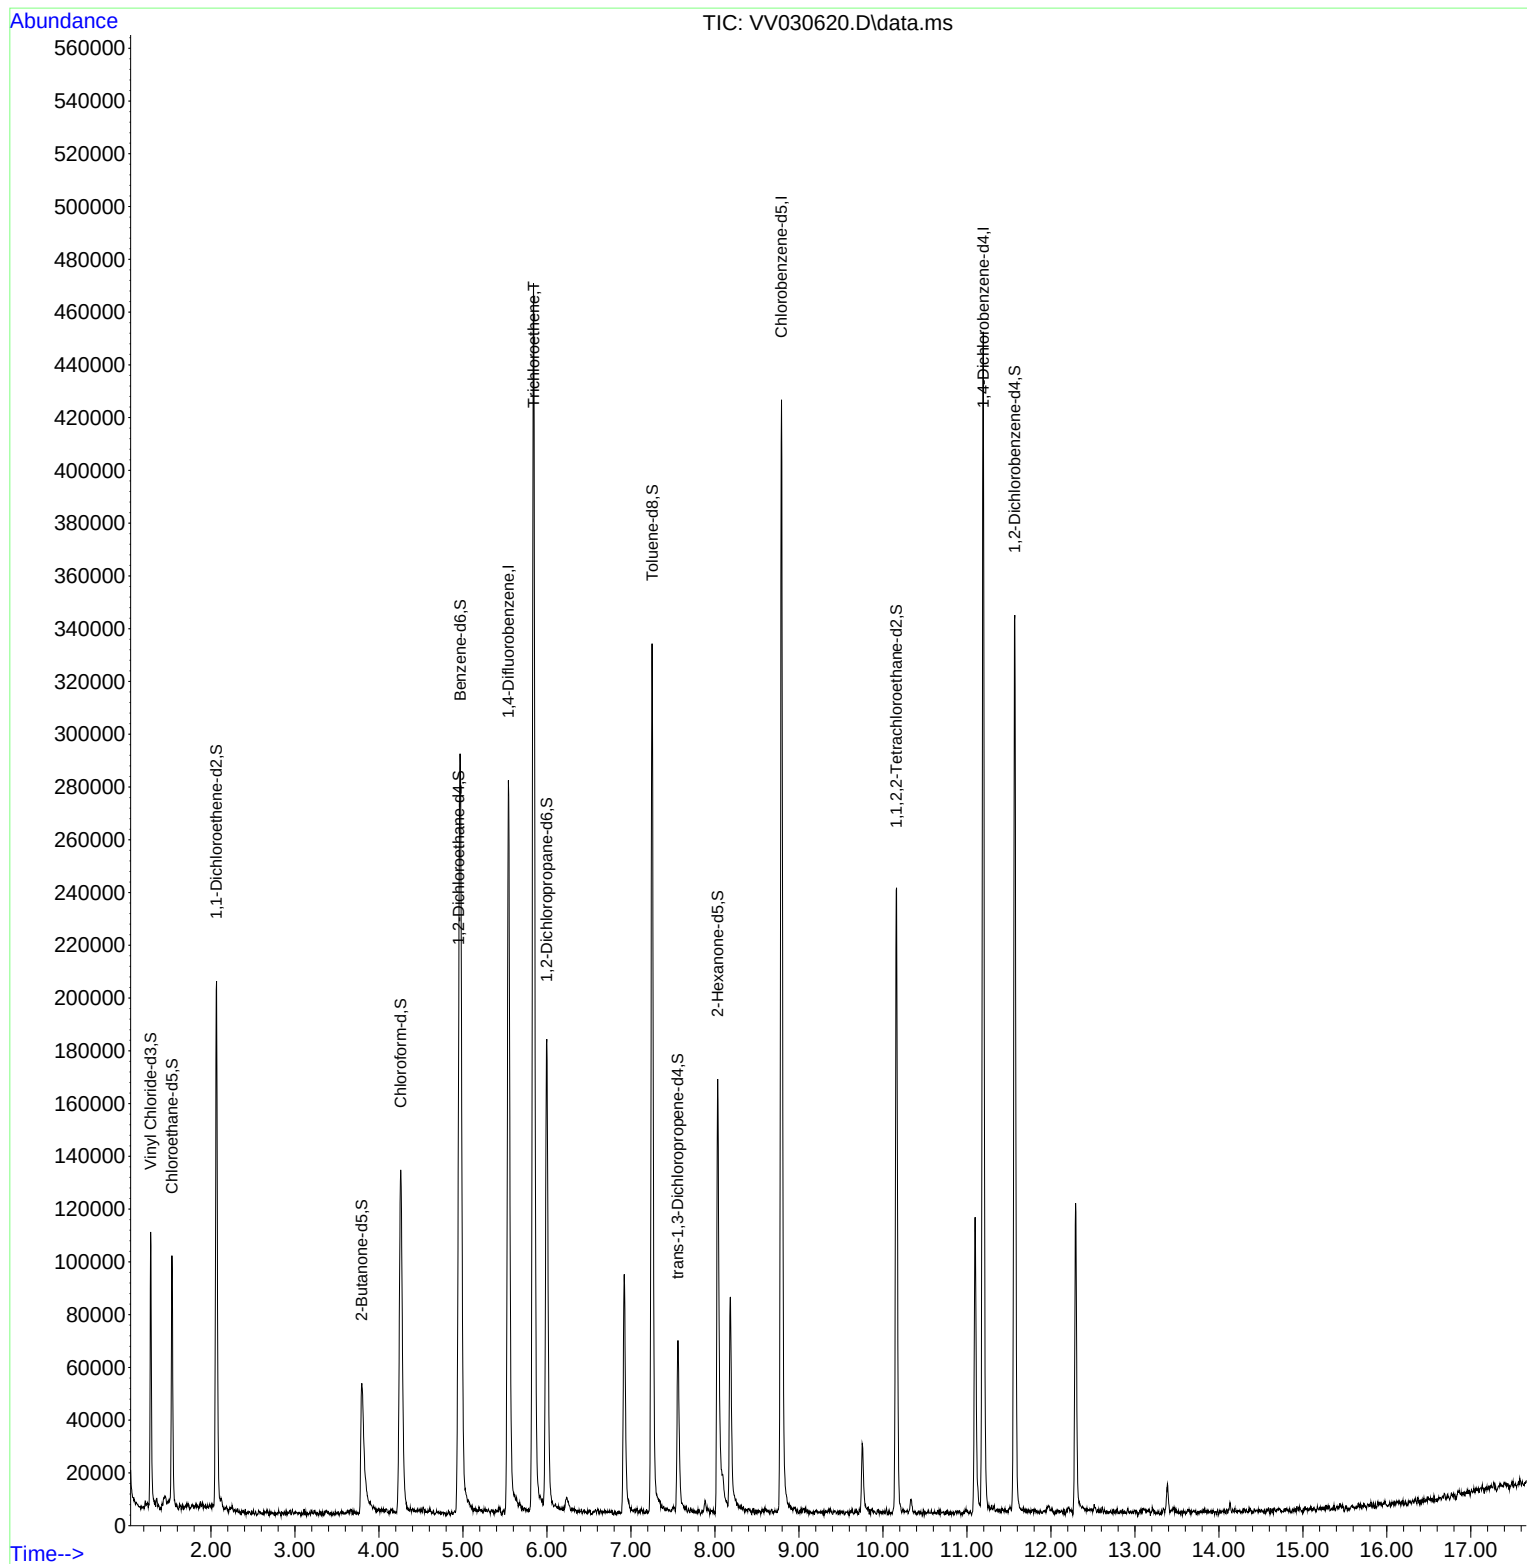

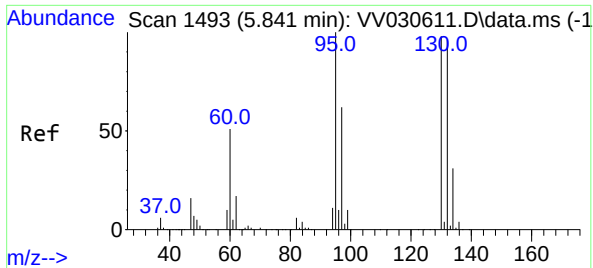

#34
 Trichloroethene
 Concen: 89.042 ug/L
 RT: 5.841 min Scan# 1493
 Delta R.T. 0.000 min
 Lab File: VV030620.D
 Acq: 18 Apr 2023 16:17

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP2

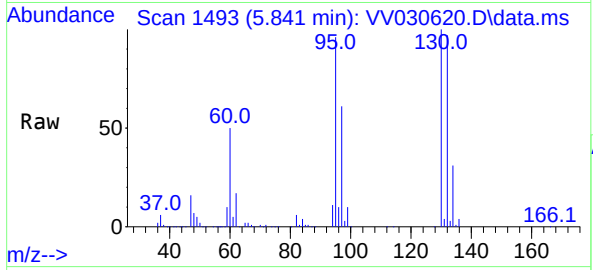

Tgt Ion: 95 Resp: 158095

Ion	Ratio	Lower	Upper
95	100		
97	64.0	45.8	85.2
132	101.2	70.6	131.2
130	104.3	70.9	131.7

