

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030626.D
 Acq On : 18 Apr 2023 18:40
 Operator : SY/MD
 Sample : 02360-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3DL

Quant Time: Apr 19 01:47:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	226275	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	223710	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	104646	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	62214	37.506	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.020%
7) Chloroethane-d5	1.535	69	55075	39.621	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.240%
11) 1,1-Dichloroethene-d2	2.066	65	32653	41.509	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.020%
21) 2-Butanone-d5	3.799	46	85935	94.321	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.320%
24) Chloroform-d	4.259	84	129185	42.974	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.940%
26) 1,2-Dichloroethane-d4	4.950	65	88598	45.842	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.680%
32) Benzene-d6	4.969	84	233228	44.096	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.200%
36) 1,2-Dichloropropane-d6	5.998	67	75219	45.783	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.560%
41) Toluene-d8	7.252	98	204177	41.115	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.240%
43) trans-1,3-Dichloroprop...	7.561	79	34440	41.590	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.180%
47) 2-Hexanone-d5	8.034	63	54808	84.682	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.680%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	103225	43.299	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	78628	47.272	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.540%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.841	95	153457	86.845	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030626.D
Acq On : 18 Apr 2023 18:40
Operator : SY/MD
Sample : 02360-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3DL

Quant Time: Apr 19 01:47:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

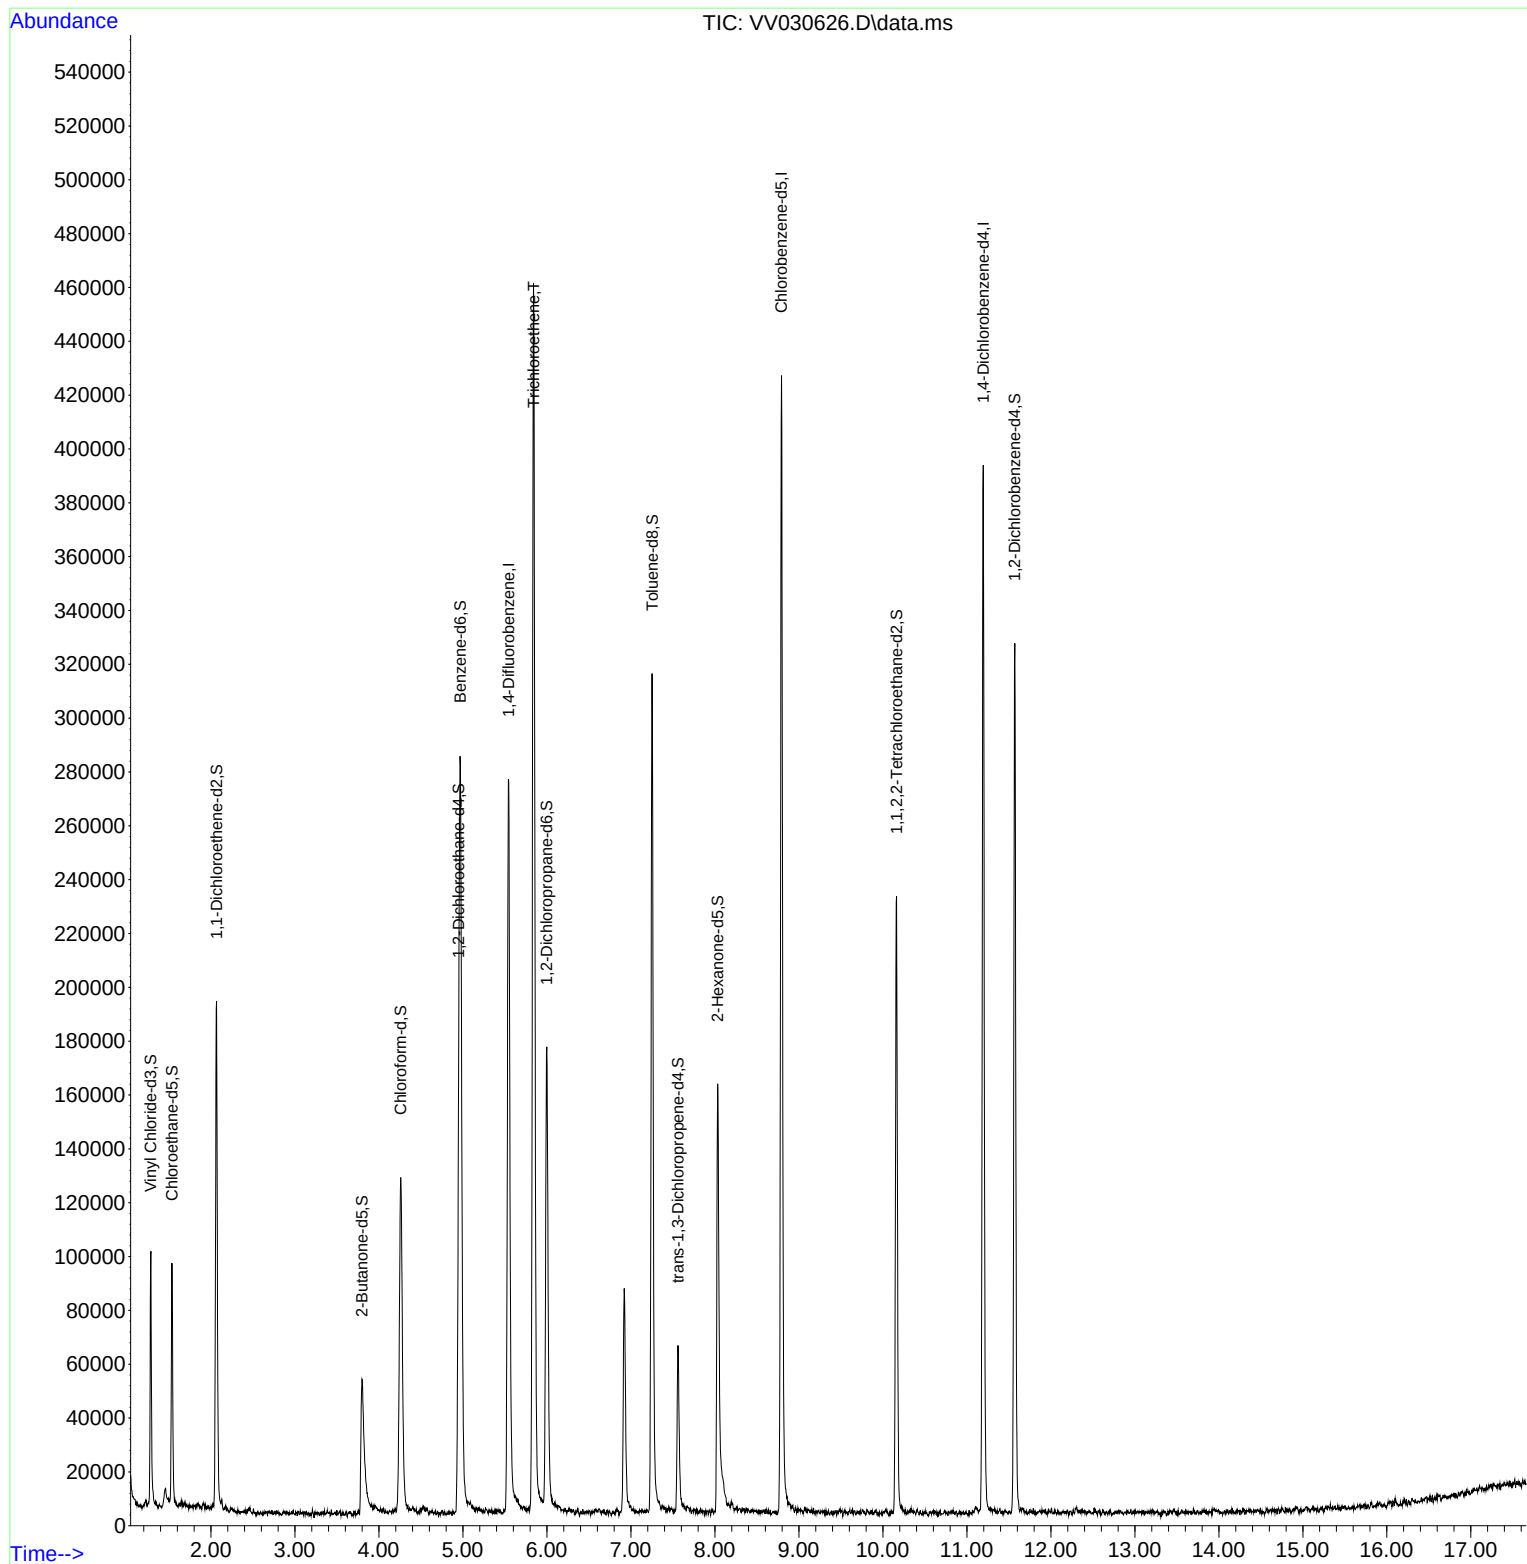

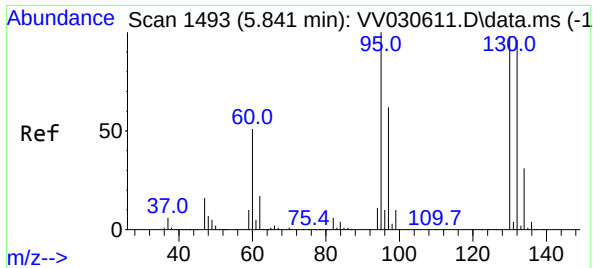

#34
 Trichloroethene
 Concen: 86.845 ug/L
 RT: 5.841 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VV030626.D
 Acq: 18 Apr 2023 18:40

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3DL

Tgt Ion: 95 Resp: 153457

Ion	Ratio	Lower	Upper
95	100		
97	64.6	45.8	85.2
132	95.3	70.6	131.2
130	102.9	70.9	131.7

