

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030645.D
 Acq On : 19 Apr 2023 02:39
 Operator : SY/MD
 Sample : 02398-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP1

Quant Time: Apr 19 04:31:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	225170	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	219870	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	101347	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	61499	37.257	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.520%
7) Chloroethane-d5	1.536	69	52375	37.864	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.720%
11) 1,1-Dichloroethene-d2	2.066	65	31649	40.430	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.860%
21) 2-Butanone-d5	3.799	46	86183	95.057	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.060%
24) Chloroform-d	4.259	84	129870	43.414	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.820%
26) 1,2-Dichloroethane-d4	4.950	65	88280	45.902	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.800%
32) Benzene-d6	4.970	84	228855	44.025	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.040%
36) 1,2-Dichloropropane-d6	5.998	67	74508	46.142	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.280%
41) Toluene-d8	7.252	98	196133	40.185	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.380%
43) trans-1,3-Dichloroprop...	7.561	79	35193	43.242	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.480%
47) 2-Hexanone-d5	8.034	63	54106	85.058	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.060%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	105666	45.097	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.200%
66) 1,2-Dichlorobenzene-d4	11.571	152	82044	50.931	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.860%
Target Compounds						
44) trans-1,3-Dichloropropene	7.564	75	1950	0.736	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030645.D
Acq On : 19 Apr 2023 02:39
Operator : SY/MD
Sample : 02398-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP1


Quant Time: Apr 19 04:31:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

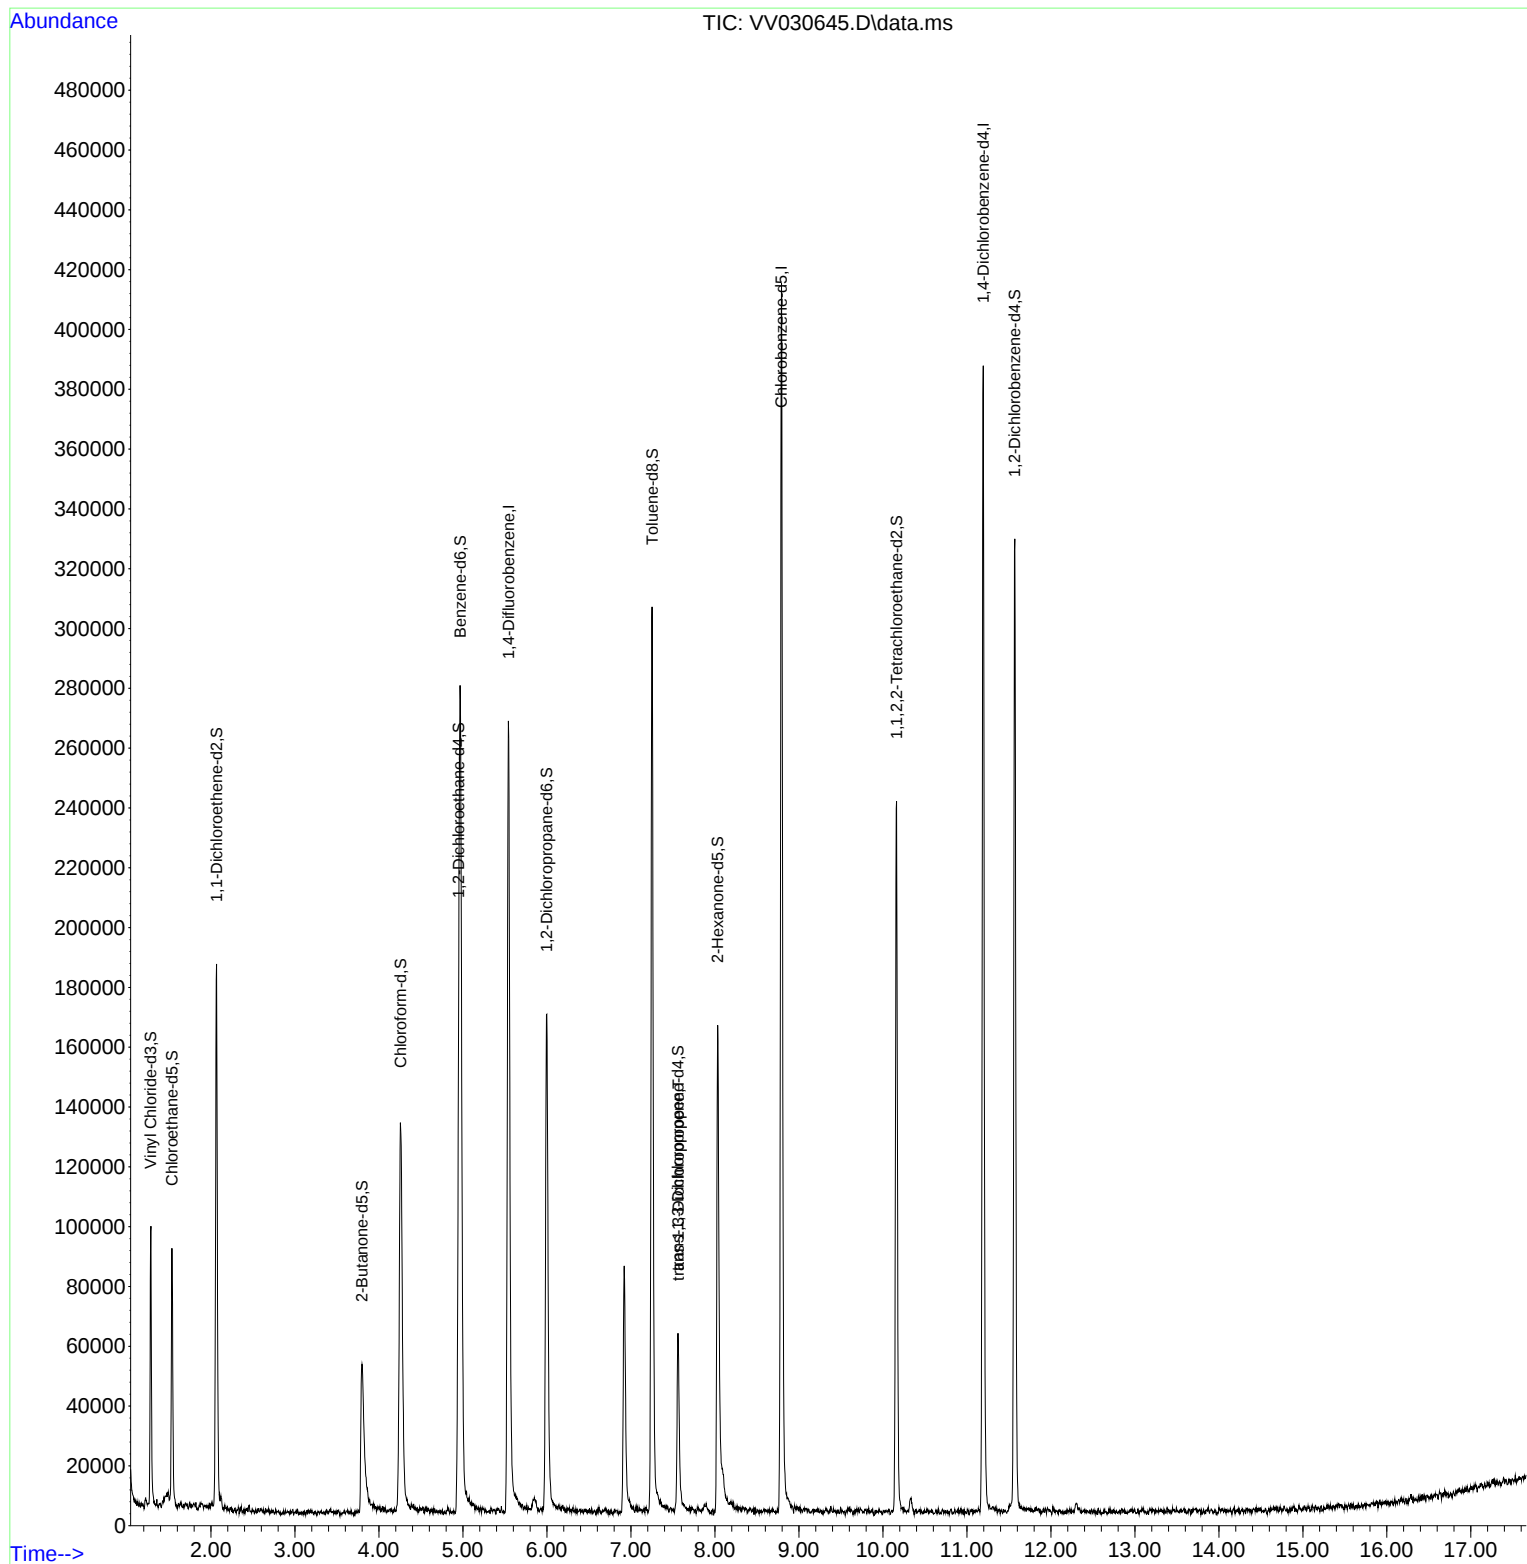

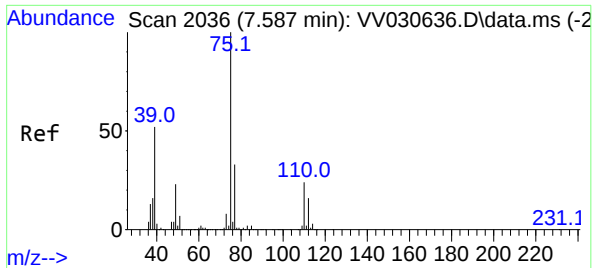

#44
 trans-1,3-Dichloropropene
 Concen: 0.736 ug/L
 RT: 7.564 min Scan# 2036
 Delta R.T. -0.022 min
 Lab File: VV030645.D
 Acq: 19 Apr 2023 02:39

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP1

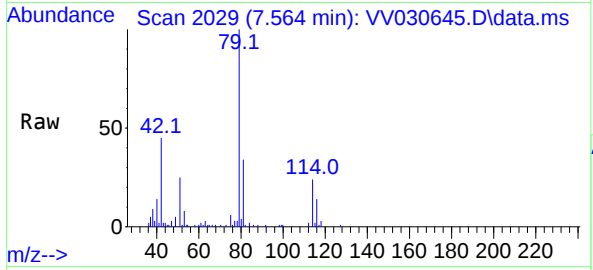

Tgt Ion: 75 Resp: 1950
 Ion Ratio Lower Upper
 75 100
 77 46.5 22.1 41.1#

