

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030629.D
 Acq On : 18 Apr 2023 19:52
 Operator : SY/MD
 Sample : 02360-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP4DL




Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:48:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

04/19/2023
 Supervised By :Mahesh
 Dadoda

04/20/2023

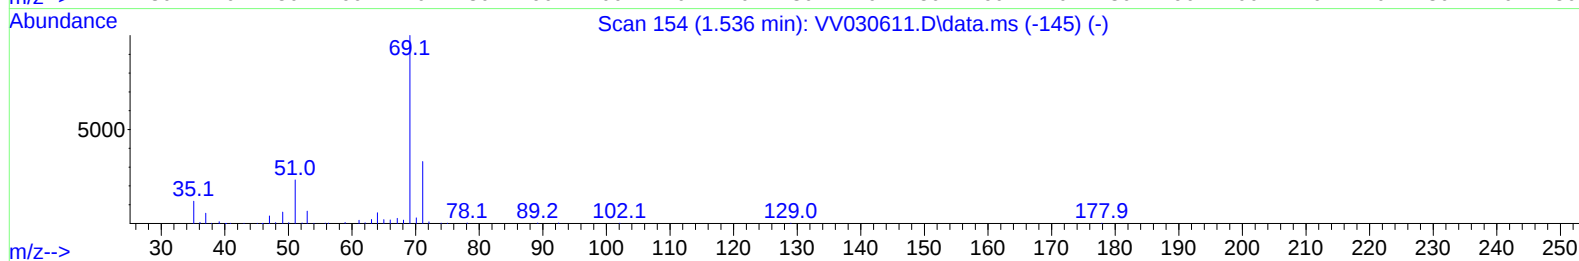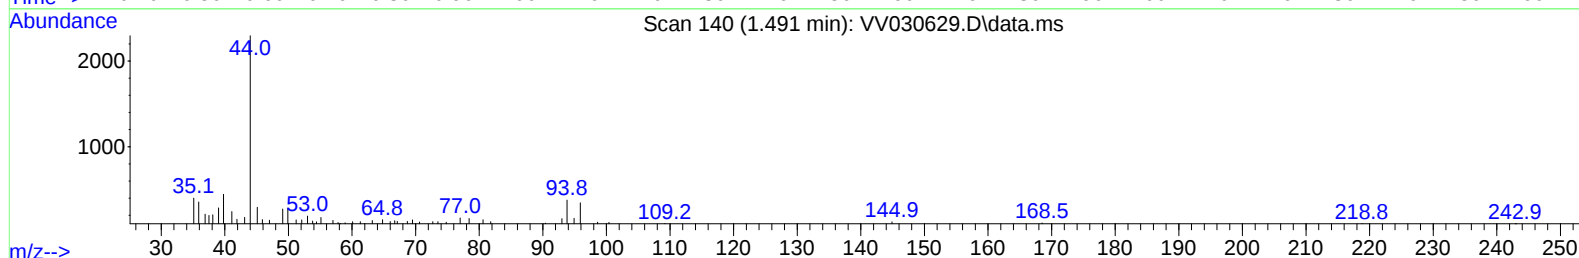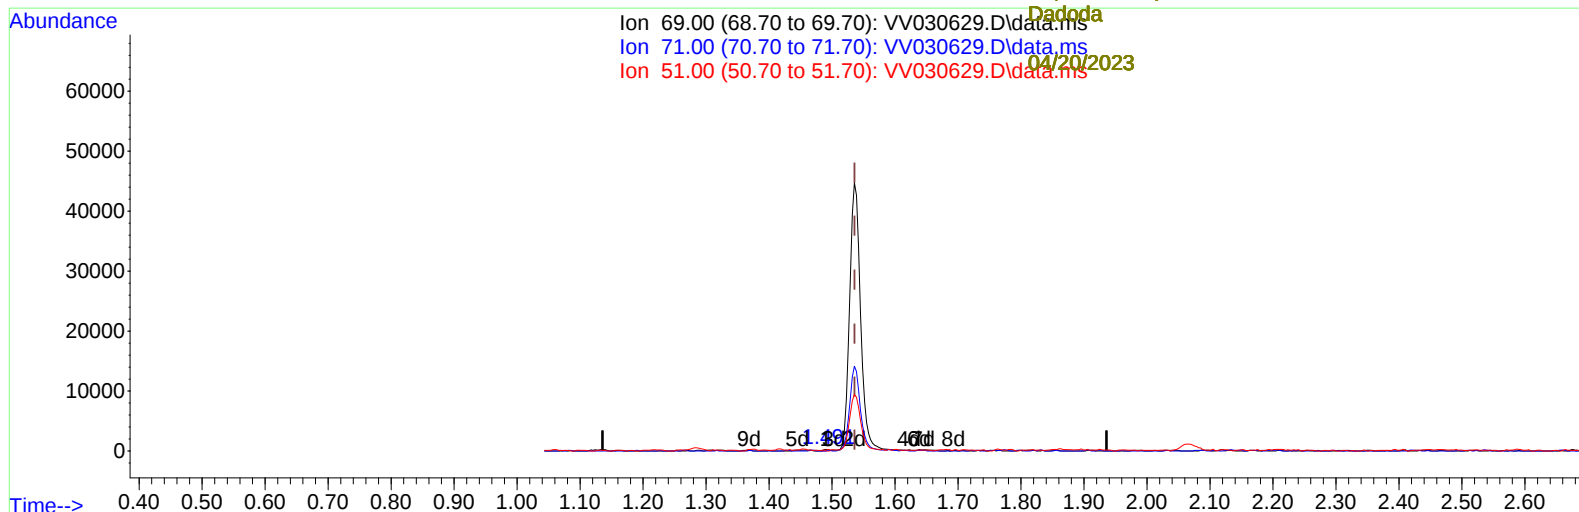

TIC: VV030629.D\data.ms

(7) Chloroethane-d5 (S)

1.491min (-0.045) 0.12 ug/L

response 170

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	28.82
51.00	30.70	28.82
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030629.D
 Acq On : 18 Apr 2023 19:52
 Operator : SY/MD
 Sample : 02360-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:48:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

04/19/2023
 Supervised By :Mahesh
 Dadoda

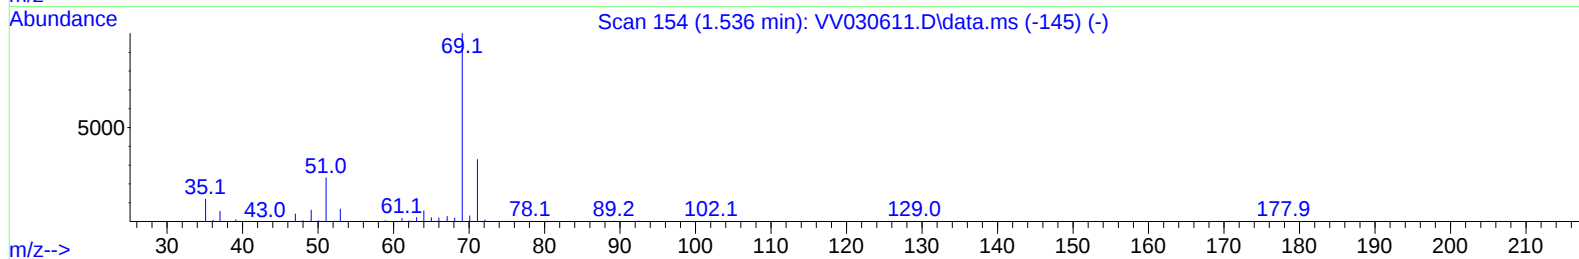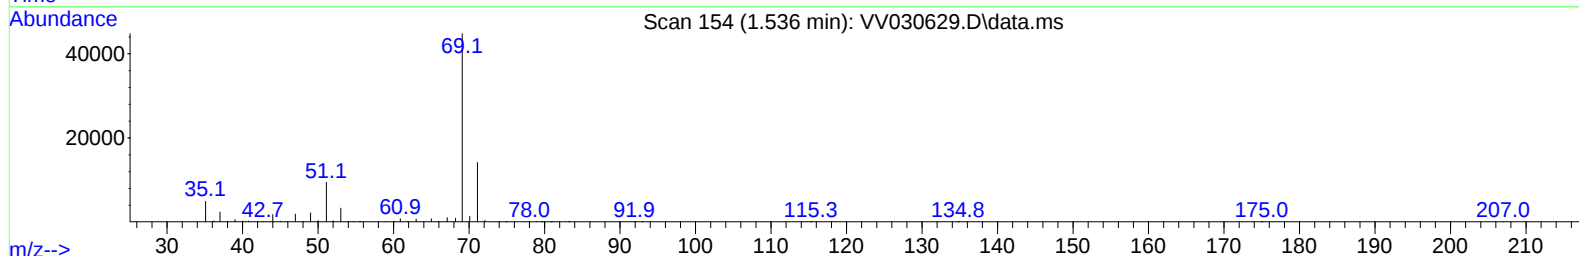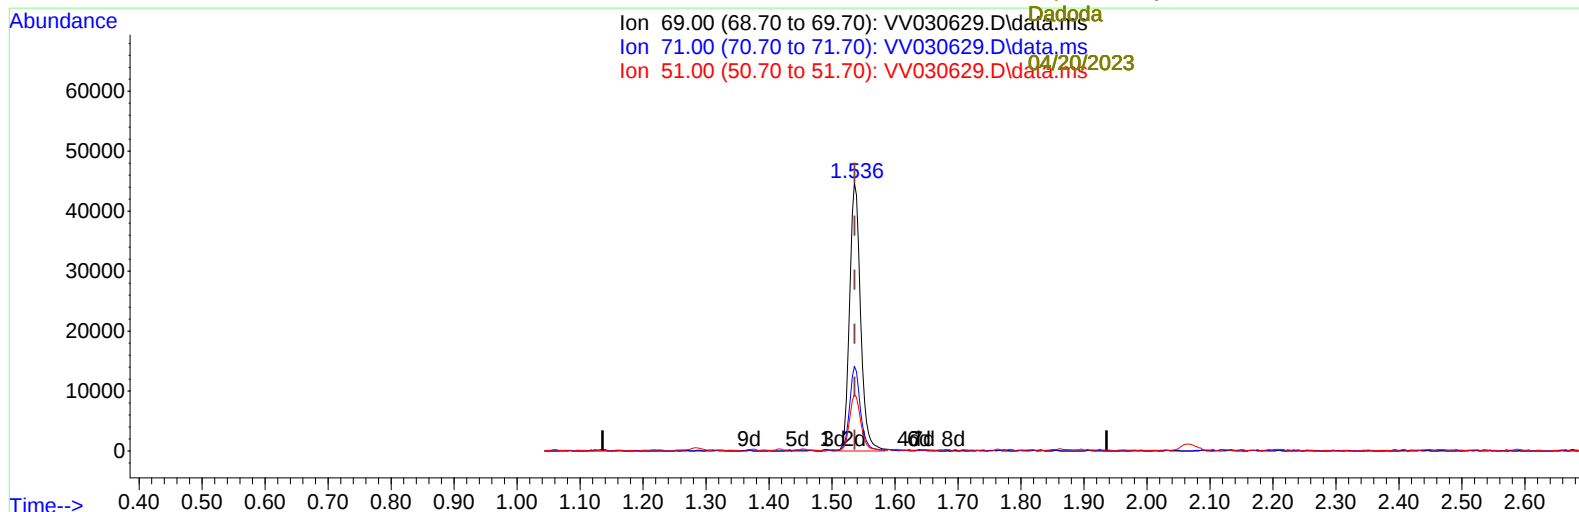

TIC: VV030629.D\data.ms

(7) Chloroethane-d5 (S)

1.536min (-0.000) 39.28 ug/L m

response 54116

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	0.09#
51.00	30.70	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030629.D
 Acq On : 18 Apr 2023 19:52
 Operator : SY/MD
 Sample : 02360-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:48:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

04/19/2023
 Supervised By :Mahesh
 Dadoda

04/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		224256	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		219643	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		101954	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		62090	37.768	ug/L	0.00
Spiked Amount	50.000			Recovery	=	75.540%	
7) Chloroethane-d5	1.536	69		54116m	39.282	ug/L	0.00
Spiked Amount	50.000			Recovery	=	78.560%	
11) 1,1-Dichloroethene-d2	2.066	65		31910	40.930	ug/L	0.00
Spiked Amount	50.000			Recovery	=	81.860%	
21) 2-Butanone-d5	3.799	46		85898	95.129	ug/L	0.00
Spiked Amount	100.000			Recovery	=	95.130%	
24) Chloroform-d	4.262	84		129539	43.480	ug/L	0.00
Spiked Amount	50.000			Recovery	=	86.960%	
26) 1,2-Dichloroethane-d4	4.950	65		89059	46.496	ug/L	0.00
Spiked Amount	50.000			Recovery	=	93.000%	
32) Benzene-d6	4.973	84		232180	44.710	ug/L	0.00
Spiked Amount	50.000			Recovery	=	89.420%	
36) 1,2-Dichloropropane-d6	5.998	67		73351	45.473	ug/L	0.00
Spiked Amount	50.000			Recovery	=	90.940%	
41) Toluene-d8	7.252	98		202944	41.624	ug/L	0.00
Spiked Amount	50.000			Recovery	=	83.240%	
43) trans-1,3-Dichloroprop...	7.561	79		33771	41.538	ug/L	0.00
Spiked Amount	50.000			Recovery	=	83.080%	
47) 2-Hexanone-d5	8.034	63		54231	85.342	ug/L	0.00
Spiked Amount	100.000			Recovery	=	85.340%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		102174	43.652	ug/L	0.00
Spiked Amount	50.000			Recovery	=	87.300%	
66) 1,2-Dichlorobenzene-d4	11.570	152		79034	48.771	ug/L	0.00
Spiked Amount	50.000			Recovery	=	97.540%	
Target Compounds							
						Qvalue	
34) Trichloroethene	5.841	95		174165	100.389	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030629.D
Acq On : 18 Apr 2023 19:52
Operator : SY/MD
Sample : 02360-12DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:48:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

Reviewed By :John
Carlone

04/19/2023
Supervised By :Mahesh
Dadoda

04/20/2023

