

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030622.D
 Acq On : 18 Apr 2023 17:04
 Operator : SY/MD
 Sample : 02360-03DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5DL

Quant Time: Apr 19 01:46:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	243365	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	234798	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108412	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	66440	37.241	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.480%
7) Chloroethane-d5	1.536	69	56301	37.659	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.320%
11) 1,1-Dichloroethene-d2	2.066	65	33835	39.991	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.980%
21) 2-Butanone-d5	3.799	46	88654	90.472	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.470%
24) Chloroform-d	4.259	84	133883	41.410	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.820%
26) 1,2-Dichloroethane-d4	4.950	65	91377	43.960	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.920%
32) Benzene-d6	4.969	84	243639	43.889	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.780%
36) 1,2-Dichloropropane-d6	5.998	67	77754	45.091	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.180%
41) Toluene-d8	7.252	98	211532	40.585	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.160%
43) trans-1,3-Dichloroprop...	7.561	79	36622	42.137	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.280%
47) 2-Hexanone-d5	8.034	63	56988	83.892	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.890%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	106375	42.513	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.020%
66) 1,2-Dichlorobenzene-d4	11.570	152	83294	48.338	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.680%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.841	95	207677	111.979	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030622.D
Acq On : 18 Apr 2023 17:04
Operator : SY/MD
Sample : 02360-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5DL


Quant Time: Apr 19 01:46:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

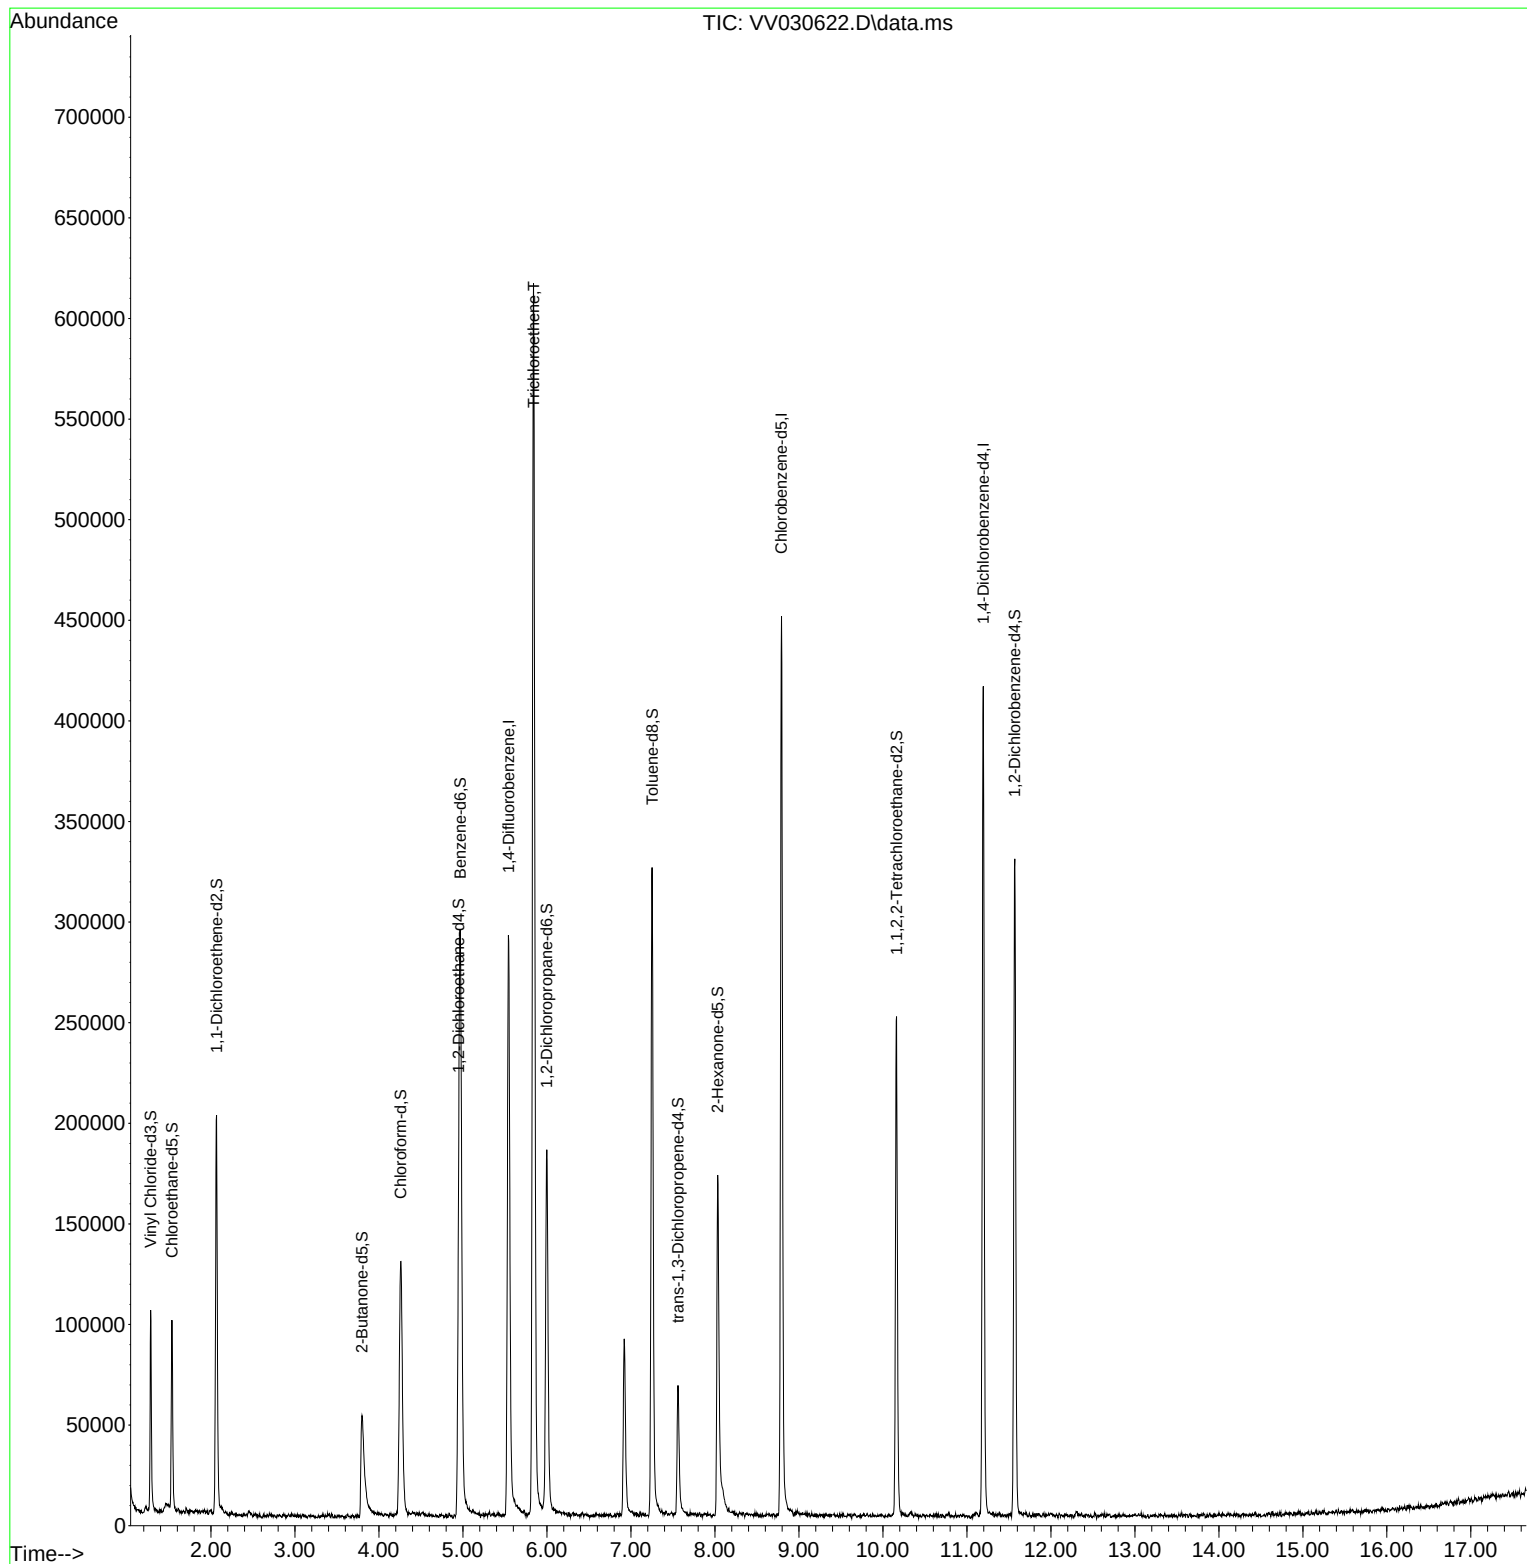

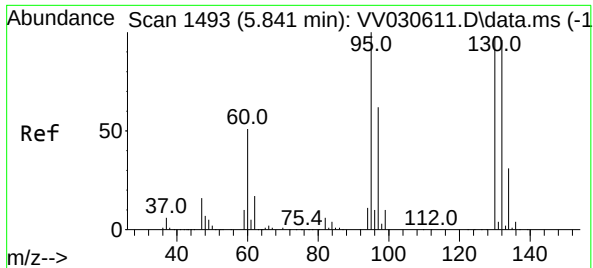

#34
 Trichloroethene
 Concen: 111.979 ug/L
 RT: 5.841 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VV030622.D
 Acq: 18 Apr 2023 17:04

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5DL

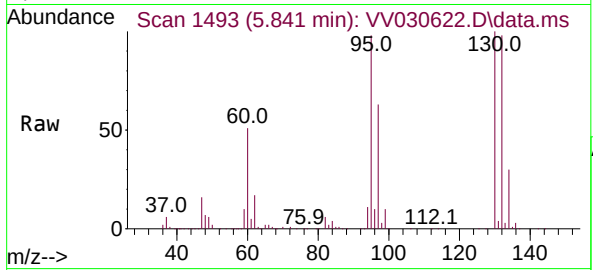

Tgt Ion: 95 Resp: 207677

Ion	Ratio	Lower	Upper
95	100		
97	64.5	45.8	85.2
132	100.0	70.6	131.2
130	102.5	70.9	131.7

