

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030614.D
 Acq On : 18 Apr 2023 13:55
 Operator : SY/MD
 Sample : 02339-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	113901	120799	14.59%	1.900%
2	1.535	148	154	168	rVB	111074	131290	15.85%	2.065%
3	2.063	310	318	333	rVB	217123	311242	37.58%	4.895%
4	2.272	380	383	385	rBV4	1204	783	0.09%	0.012%
5	2.285	385	387	391	rVB4	1990	1118	0.13%	0.018%
6	2.616	488	490	492	rBV2	1419	738	0.09%	0.012%
7	2.654	498	502	506	rVV7	1370	1285	0.16%	0.020%
8	2.744	528	530	534	rBV4	1224	992	0.12%	0.016%
9	2.831	555	557	562	rBV5	1292	775	0.09%	0.012%
10	3.008	607	612	615	rVB6	1635	1669	0.20%	0.026%
11	3.053	623	626	628	rVB4	1444	874	0.11%	0.014%
12	3.092	635	638	640	rVB4	1781	821	0.10%	0.013%
13	3.230	678	681	685	rBV5	1327	1273	0.15%	0.020%
14	3.320	703	709	711	rBV7	1416	1455	0.18%	0.023%
15	3.359	718	721	725	rBV5	1412	1492	0.18%	0.023%
16	3.391	729	731	735	rBV5	1631	946	0.11%	0.015%
17	3.432	741	744	747	rBV4	1697	976	0.12%	0.015%
18	3.487	759	761	764	rVV4	1388	765	0.09%	0.012%
19	3.519	768	771	776	rVB6	1982	1777	0.21%	0.028%
20	3.545	776	779	783	rBV7	1679	1644	0.20%	0.026%
21	3.616	799	801	804	rVB4	1693	871	0.11%	0.014%
22	3.635	804	807	813	rBV7	1572	1451	0.18%	0.023%
23	3.802	849	859	878	rBV	53369	146253	17.66%	2.300%
24	4.150	963	967	968	rBV4	1354	735	0.09%	0.012%
25	4.259	988	1001	1020	rBV	132102	330263	39.88%	5.194%
26	4.494	1071	1074	1075	rBV3	1591	940	0.11%	0.015%
27	4.728	1145	1147	1151	rBV4	1283	1091	0.13%	0.017%
28	4.831	1177	1179	1182	rBV4	1187	805	0.10%	0.013%
29	4.847	1182	1184	1191	rVV8	1305	1295	0.16%	0.020%
30	4.966	1204	1221	1245	rVV2	308176	828165	100.00%	13.025%
31	5.227	1299	1302	1303	rBV2	1899	1018	0.12%	0.016%
32	5.542	1387	1400	1422	rBV	256320	536767	64.81%	8.442%
33	5.847	1483	1495	1496	rBV	7654	11971	1.45%	0.188%
34	5.998	1530	1542	1561	rBV	184649	380626	45.96%	5.986%
35	6.407	1666	1669	1673	rVB5	1327	881	0.11%	0.014%
36	6.465	1686	1687	1691	rBV3	1115	741	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030614.D
 Acq On : 18 Apr 2023 13:55
 Operator : SY/MD
 Sample : 02339-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.558	1712	1716	1717	rBV4	2145	1229	0.15%	0.019%
38	6.664	1747	1749	1755	rBV6	1821	1550	0.19%	0.024%
39	6.744	1768	1774	1775	rBV5	1612	1106	0.13%	0.017%
40	6.857	1805	1809	1810	rBV3	1665	987	0.12%	0.016%
41	6.921	1818	1829	1844	rBV	88348	166674	20.13%	2.621%
42	7.252	1919	1932	1949	rBV	341401	610093	73.67%	9.595%
43	7.439	1988	1990	1994	rBV5	1551	1101	0.13%	0.017%
44	7.561	2018	2028	2043	rBV	68677	122928	14.84%	1.933%
45	7.783	2095	2097	2100	rVB4	2029	1254	0.15%	0.020%
46	7.966	2151	2154	2157	rVB3	1711	888	0.11%	0.014%
47	8.034	2160	2175	2202	rBV2	179431	367233	44.34%	5.776%
48	8.487	2314	2316	2318	rBV3	1562	747	0.09%	0.012%
49	8.792	2400	2411	2431	rBV	395922	664748	80.27%	10.455%
50	9.378	2590	2593	2595	rBV3	1732	999	0.12%	0.016%
51	9.455	2615	2617	2620	rVB4	1489	738	0.09%	0.012%
52	9.532	2639	2641	2644	rBV4	1302	729	0.09%	0.011%
53	9.638	2672	2674	2677	rBV3	1323	938	0.11%	0.015%
54	9.722	2694	2700	2704	rBV8	1892	1983	0.24%	0.031%
55	9.796	2721	2723	2728	rVB6	1774	738	0.09%	0.012%
56	9.902	2750	2756	2759	rBV7	2796	3087	0.37%	0.049%
57	9.931	2762	2765	2766	rBV3	1583	1018	0.12%	0.016%
58	10.095	2813	2816	2818	rBV4	1124	710	0.09%	0.011%
59	10.162	2826	2837	2857	rVB	246794	402897	48.65%	6.337%
60	10.313	2882	2884	2890	rVB6	2001	1553	0.19%	0.024%
61	10.477	2929	2935	2938	rBV7	2420	2242	0.27%	0.035%
62	10.599	2971	2973	2978	rVB6	2304	1141	0.14%	0.018%
63	10.699	3002	3004	3008	rVB5	1206	769	0.09%	0.012%
64	10.789	3030	3032	3035	rBV4	1507	753	0.09%	0.012%
65	10.998	3093	3097	3098	rBV4	977	830	0.10%	0.013%
66	11.043	3107	3111	3112	rBV4	1342	908	0.11%	0.014%
67	11.101	3126	3129	3130	rBV4	1811	972	0.12%	0.015%
68	11.194	3146	3158	3175	rBV	363128	583781	70.49%	9.182%
69	11.390	3215	3219	3220	rBV4	1402	868	0.10%	0.014%
70	11.426	3225	3230	3233	rVV6	1151	1039	0.13%	0.016%
71	11.570	3259	3275	3293	rBV	333697	547647	66.13%	8.613%
72	11.779	3337	3340	3344	rBV6	1337	1311	0.16%	0.021%
73	11.824	3352	3354	3359	rVB6	1379	1075	0.13%	0.017%
74	11.850	3359	3362	3366	rBV6	2202	1706	0.21%	0.027%
75	12.172	3458	3462	3465	rBV5	1651	1768	0.21%	0.028%
76	12.197	3467	3470	3476	rVB7	1720	1523	0.18%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030614.D
 Acq On : 18 Apr 2023 13:55
 Operator : SY/MD
 Sample : 02339-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.246	3483	3485	3488	rBV3	1199	917	0.11%	0.014%
78	12.342	3512	3515	3520	rBV6	1117	937	0.11%	0.015%
79	12.667	3613	3616	3618	rBV3	2258	1326	0.16%	0.021%
80	12.863	3675	3677	3682	rVB6	1852	1280	0.15%	0.020%
81	12.911	3689	3692	3696	rVB6	2249	1819	0.22%	0.029%
82	12.940	3699	3701	3705	rBV5	1024	865	0.10%	0.014%
83	13.072	3740	3742	3745	rBV4	1746	1051	0.13%	0.017%
84	13.104	3746	3752	3755	rVV7	2064	1872	0.23%	0.029%
85	13.162	3766	3770	3773	rBV4	1468	1104	0.13%	0.017%
86	13.181	3773	3776	3779	rBV4	1508	1155	0.14%	0.018%
87	13.265	3799	3802	3806	rBV6	1564	1081	0.13%	0.017%
88	13.348	3825	3828	3830	rBV3	1324	868	0.10%	0.014%
89	13.442	3855	3857	3858	rBV2	1550	700	0.08%	0.011%
90	13.615	3908	3911	3914	rBV5	1621	1109	0.13%	0.017%
91	13.770	3956	3959	3961	rVB4	1543	858	0.10%	0.013%
92	13.789	3961	3965	3966	rBV3	1127	707	0.09%	0.011%
93	13.844	3980	3982	3984	rBV3	1509	830	0.10%	0.013%
94	14.172	4079	4084	4087	rBV7	2068	2386	0.29%	0.038%
95	14.246	4103	4107	4110	rBV6	1410	1262	0.15%	0.020%
96	14.358	4140	4142	4145	rBV3	1244	742	0.09%	0.012%
97	14.541	4197	4199	4201	rBV3	1452	715	0.09%	0.011%
98	14.792	4275	4277	4280	rBV4	1881	1050	0.13%	0.017%
99	15.014	4343	4346	4347	rBV2	2148	1139	0.14%	0.018%
100	15.098	4367	4372	4374	rBV7	1696	1526	0.18%	0.024%



Sum of corrected areas: 6358147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030614.D
Acq On : 18 Apr 2023 13:55
Operator : SY/MD
Sample : 02339-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

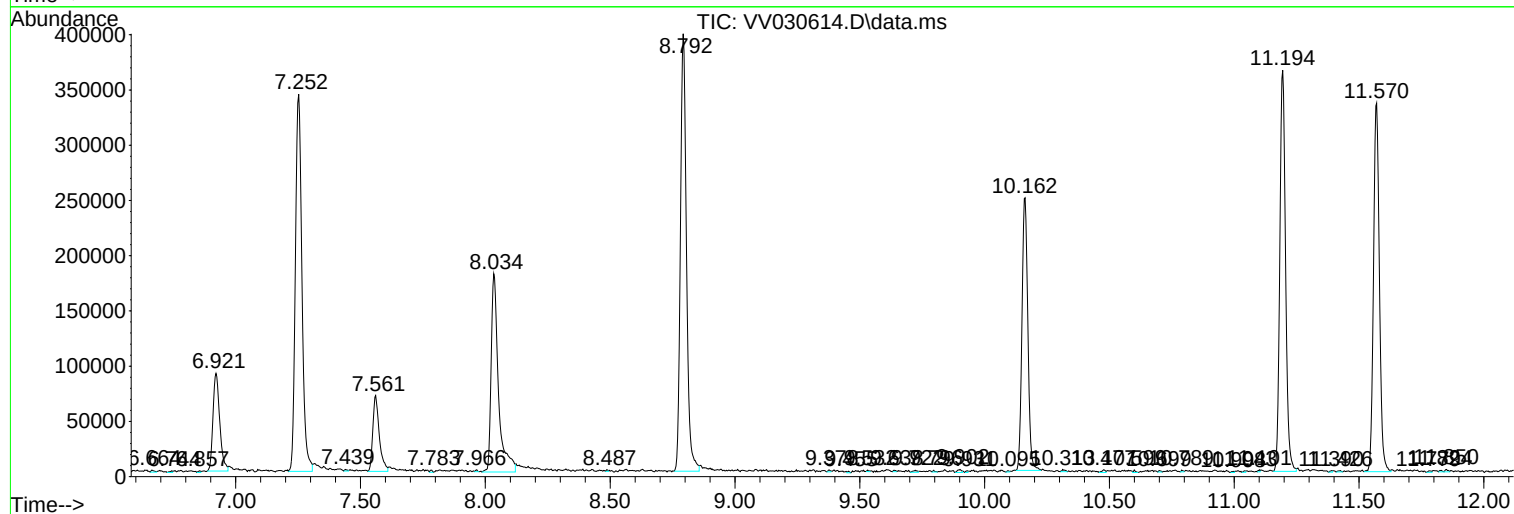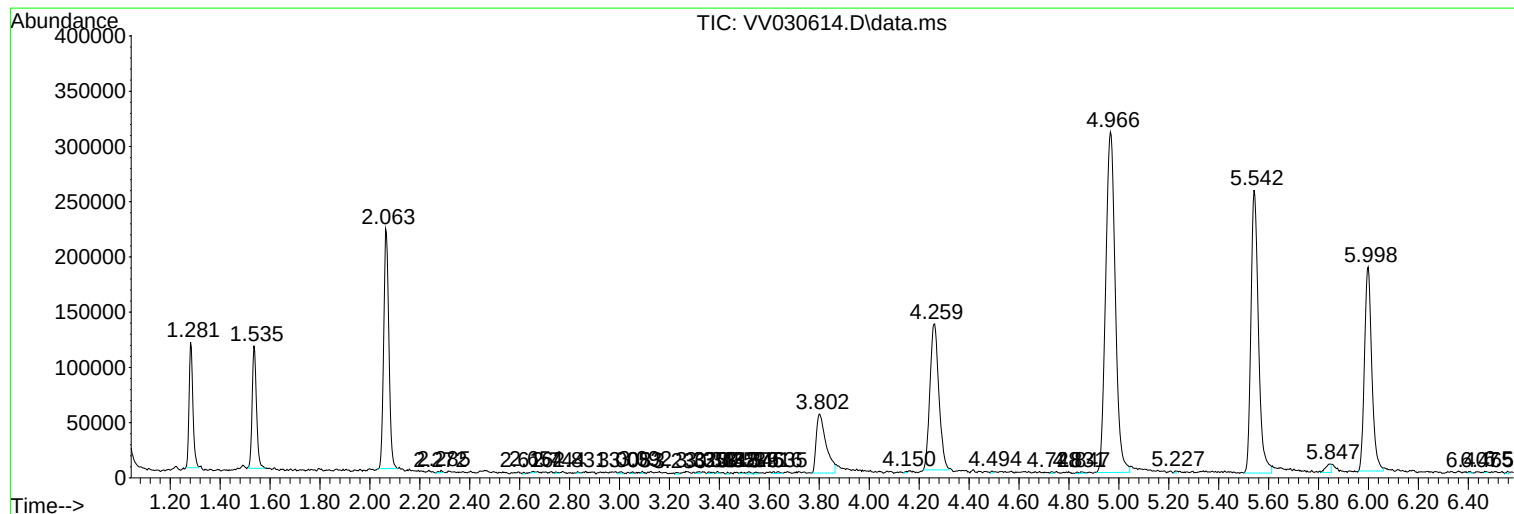

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030614.D
Acq On : 18 Apr 2023 13:55
Operator : SY/MD
Sample : 02339-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030614.D
Acq On : 18 Apr 2023 13:55
Operator : SY/MD
Sample : 02339-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------