

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030621.D
 Acq On : 18 Apr 2023 16:40
 Operator : SY/MD
 Sample : 02360-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rBV	101118	112648	11.86%	1.552%
2	1.536	148	154	169	rVB	98126	116256	12.24%	1.602%
3	2.066	310	319	337	rVB	201453	298498	31.43%	4.112%
4	2.610	485	488	489	rBV2	1268	720	0.08%	0.010%
5	2.635	493	496	500	rVB5	1631	1461	0.15%	0.020%
6	2.658	500	503	505	rBV4	1490	837	0.09%	0.012%
7	2.683	509	511	512	rVV2	1260	668	0.07%	0.009%
8	2.709	515	519	521	rBV6	1876	1391	0.15%	0.019%
9	2.799	545	547	549	rBV3	1207	677	0.07%	0.009%
10	2.892	573	576	579	rBV5	1694	1301	0.14%	0.018%
11	2.960	595	597	599	rBV3	956	603	0.06%	0.008%
12	3.008	610	612	614	rBV3	1110	586	0.06%	0.008%
13	3.053	620	626	630	rVB7	1482	1527	0.16%	0.021%
14	3.076	630	633	635	rBV4	1443	820	0.09%	0.011%
15	3.098	637	640	641	rBV3	1517	608	0.06%	0.008%
16	3.111	642	644	648	rVB4	1482	770	0.08%	0.011%
17	3.201	669	672	678	rVB8	1325	1408	0.15%	0.019%
18	3.352	715	719	722	rBV6	955	831	0.09%	0.011%
19	3.413	735	738	739	rBV3	1180	583	0.06%	0.008%
20	3.439	741	746	751	rVV9	1682	1817	0.19%	0.025%
21	3.539	769	777	779	rBV9	2531	2172	0.23%	0.030%
22	3.638	806	808	813	rVB5	1773	1223	0.13%	0.017%
23	3.671	814	818	819	rBV4	1314	959	0.10%	0.013%
24	3.754	842	844	847	rBV4	895	674	0.07%	0.009%
25	3.799	847	858	883	rBV	52295	152619	16.07%	2.103%
26	4.262	989	1002	1021	rVB	127760	316825	33.36%	4.365%
27	4.584	1100	1102	1104	rBV3	1200	615	0.06%	0.008%
28	4.674	1127	1130	1132	rBV3	1123	855	0.09%	0.012%
29	4.703	1137	1139	1143	rVV3	1557	838	0.09%	0.012%
30	4.789	1160	1166	1167	rBV6	1691	1427	0.15%	0.020%
31	4.966	1205	1221	1243	rBV2	296245	787732	82.95%	10.853%
32	5.542	1388	1400	1422	rBV	275802	573850	60.43%	7.906%
33	5.841	1480	1493	1511	rBV	483810	949596	100.00%	13.083%
34	5.998	1531	1542	1561	rVB	176136	362974	38.22%	5.001%
35	6.256	1620	1622	1624	rBV3	1819	591	0.06%	0.008%
36	6.532	1705	1708	1710	rBV4	1876	974	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030621.D
 Acq On : 18 Apr 2023 16:40
 Operator : SY/MD
 Sample : 02360-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.754	1775	1777	1780	rBV5	1395	736	0.08%	0.010%
38	6.828	1798	1800	1807	rVB8	2041	1776	0.19%	0.024%
39	6.876	1807	1815	1817	rVB9	2057	2123	0.22%	0.029%
40	6.921	1817	1829	1848	rBV	91283	180428	19.00%	2.486%
41	7.252	1918	1932	1948	rBV	332721	596298	62.79%	8.215%
42	7.561	2019	2028	2047	rBV2	63496	116156	12.23%	1.600%
43	7.780	2093	2096	2098	rBV4	1472	940	0.10%	0.013%
44	7.838	2109	2114	2117	rBV7	1822	2070	0.22%	0.029%
45	8.034	2165	2175	2208	rBV	169641	340872	35.90%	4.696%
46	8.371	2277	2280	2284	rBV6	2119	1212	0.13%	0.017%
47	8.394	2284	2287	2290	rBV5	1326	1072	0.11%	0.015%
48	8.468	2308	2310	2317	rBV8	1295	935	0.10%	0.013%
49	8.542	2330	2333	2335	rBV3	1083	655	0.07%	0.009%
50	8.793	2400	2411	2433	rBV	420156	704325	74.17%	9.704%
51	9.153	2520	2523	2526	rBV5	2089	1452	0.15%	0.020%
52	9.288	2562	2565	2566	rBV3	1377	768	0.08%	0.011%
53	9.397	2595	2599	2602	rBV6	1771	1588	0.17%	0.022%
54	9.468	2619	2621	2626	rVB4	1731	1434	0.15%	0.020%
55	9.638	2671	2674	2677	rBV4	1698	1212	0.13%	0.017%
56	9.664	2681	2682	2685	rBV3	1189	777	0.08%	0.011%
57	9.699	2689	2693	2695	rBV6	1272	928	0.10%	0.013%
58	9.812	2723	2728	2729	rBV4	1756	1496	0.16%	0.021%
59	9.854	2739	2741	2743	rBV3	1455	634	0.07%	0.009%
60	9.921	2759	2762	2766	rBV6	1649	1250	0.13%	0.017%
61	9.998	2784	2786	2791	rBV7	1200	1118	0.12%	0.015%
62	10.024	2791	2794	2797	rBV4	2000	1630	0.17%	0.022%
63	10.162	2826	2837	2851	rBV	238380	386310	40.68%	5.322%
64	10.593	2967	2971	2973	rBV5	2446	1182	0.12%	0.016%
65	10.616	2975	2978	2981	rBV5	1299	813	0.09%	0.011%
66	10.818	3039	3041	3044	rVB4	1510	923	0.10%	0.013%
67	10.870	3053	3057	3058	rBV4	1577	1132	0.12%	0.016%
68	10.892	3062	3064	3069	rVB5	1496	1186	0.12%	0.016%
69	10.944	3076	3080	3081	rBV4	1009	721	0.08%	0.010%
70	11.194	3146	3158	3174	rBV	398830	632837	66.64%	8.719%
71	11.358	3207	3209	3211	rBV3	1402	875	0.09%	0.012%
72	11.387	3217	3218	3221	rBV3	1145	641	0.07%	0.009%
73	11.571	3263	3275	3290	rBV	335628	542789	57.16%	7.478%
74	11.744	3324	3329	3330	rBV4	1452	994	0.10%	0.014%
75	12.024	3415	3416	3421	rVB4	965	731	0.08%	0.010%
76	12.050	3421	3424	3427	rBV4	1896	1527	0.16%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030621.D
 Acq On : 18 Apr 2023 16:40
 Operator : SY/MD
 Sample : 02360-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.130	3447	3449	3453	rBV4	1554	943	0.10%	0.013%
78	12.339	3511	3514	3516	rBV4	1619	710	0.07%	0.010%
79	12.802	3656	3658	3660	rVB3	1871	631	0.07%	0.009%
80	12.847	3669	3672	3673	rBV3	1477	721	0.08%	0.010%
81	13.088	3743	3747	3749	rBV5	1639	989	0.10%	0.014%
82	13.127	3754	3759	3760	rBV4	1049	854	0.09%	0.012%
83	13.275	3798	3805	3808	rBV8	2173	2230	0.23%	0.031%
84	13.342	3824	3826	3829	rBV3	1642	1302	0.14%	0.018%
85	13.381	3836	3838	3839	rBV2	2035	784	0.08%	0.011%
86	13.522	3878	3882	3884	rBV5	1395	1000	0.11%	0.014%
87	13.619	3909	3912	3915	rVB5	1349	1011	0.11%	0.014%
88	13.683	3930	3932	3933	rBV2	1506	629	0.07%	0.009%
89	13.789	3964	3965	3971	rVB5	1625	961	0.10%	0.013%
90	13.921	4004	4006	4009	rBV3	1377	979	0.10%	0.013%
91	13.976	4021	4023	4026	rBV4	1621	985	0.10%	0.014%
92	14.024	4036	4038	4042	rBV6	1505	1165	0.12%	0.016%
93	14.053	4045	4047	4051	rVB5	1869	1080	0.11%	0.015%
94	14.236	4102	4104	4106	rBV3	1735	745	0.08%	0.010%
95	14.339	4135	4136	4139	rBV3	1138	760	0.08%	0.010%
96	14.474	4176	4178	4180	rBV2	1433	577	0.06%	0.008%
97	14.590	4211	4214	4216	rBV4	1886	1198	0.13%	0.017%
98	14.757	4264	4266	4270	rVB5	1920	1022	0.11%	0.014%
99	14.876	4299	4303	4305	rBV4	2017	1785	0.19%	0.025%
100	15.008	4341	4344	4345	rBV3	1802	896	0.09%	0.012%



Sum of corrected areas: 7258437

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030621.D
Acq On : 18 Apr 2023 16:40
Operator : SY/MD
Sample : 02360-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

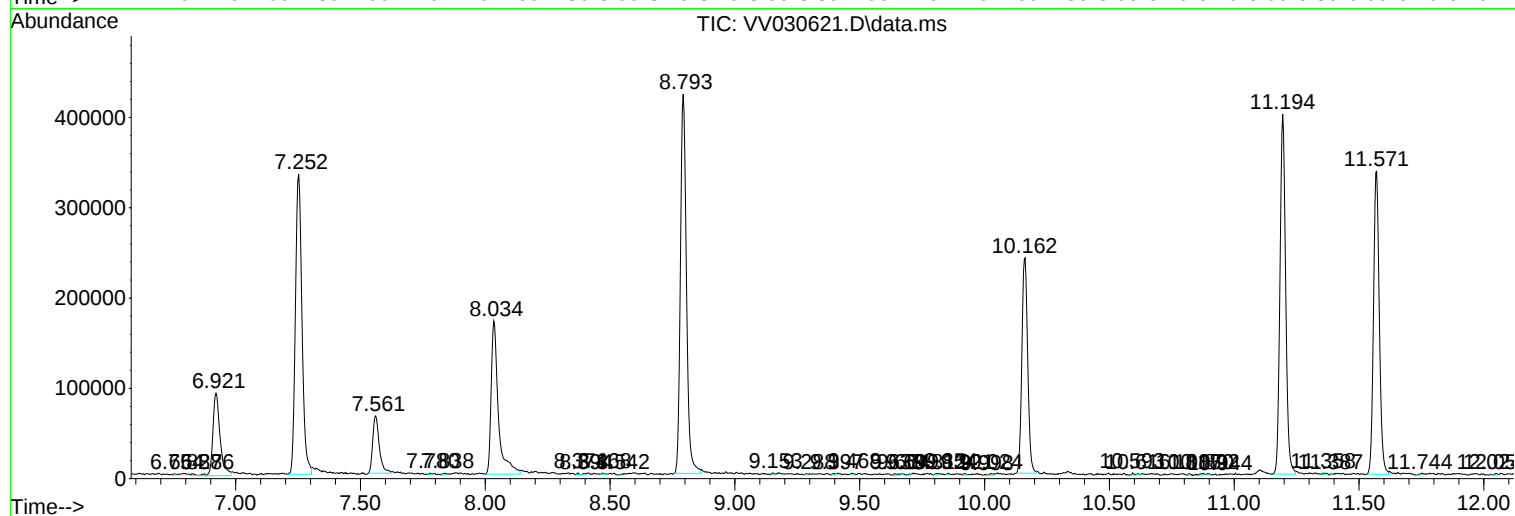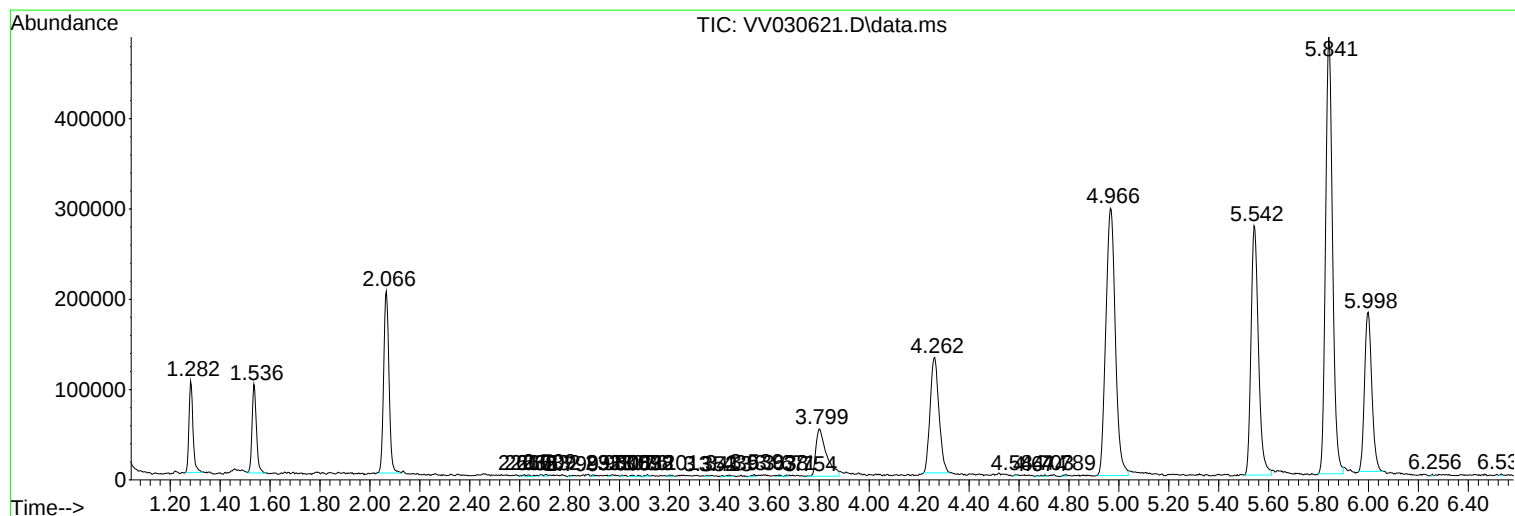

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030621.D
Acq On : 18 Apr 2023 16:40
Operator : SY/MD
Sample : 02360-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030621.D
Acq On : 18 Apr 2023 16:40
Operator : SY/MD
Sample : 02360-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------