

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030623.D
 Acq On : 18 Apr 2023 17:28
 Operator : SY/MD
 Sample : 02360-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rBV	102182	106267	13.86%	1.585%
2	1.536	147	154	165	rVB	92205	107737	14.05%	1.607%
3	2.066	310	319	331	rBV	194944	284658	37.12%	4.246%
4	2.635	493	496	501	rBV6	2112	1903	0.25%	0.028%
5	2.703	512	517	518	rBV5	1500	967	0.13%	0.014%
6	2.732	524	526	532	rVB7	1576	1349	0.18%	0.020%
7	2.870	566	569	573	rVB5	2206	1618	0.21%	0.024%
8	2.892	573	576	582	rBV8	1931	1961	0.26%	0.029%
9	2.970	595	600	602	rBV6	1485	1212	0.16%	0.018%
10	3.008	608	612	613	rBV3	1422	1081	0.14%	0.016%
11	3.082	631	635	638	rBV5	1210	1003	0.13%	0.015%
12	3.240	682	684	688	rVB5	1821	1189	0.16%	0.018%
13	3.265	688	692	693	rBV4	1967	1304	0.17%	0.019%
14	3.294	698	701	705	rVV6	1882	1078	0.14%	0.016%
15	3.349	715	718	721	rVB4	1364	800	0.10%	0.012%
16	3.378	721	727	731	rBV8	1438	1764	0.23%	0.026%
17	3.416	736	739	741	rBV4	1724	765	0.10%	0.011%
18	3.449	745	749	753	rBV7	1713	1563	0.20%	0.023%
19	3.638	804	808	812	rVB7	1781	1297	0.17%	0.019%
20	3.677	816	820	821	rBV4	1233	688	0.09%	0.010%
21	3.716	830	832	836	rBV4	1201	1063	0.14%	0.016%
22	3.802	848	859	886	rBV3	56821	198529	25.89%	2.961%
23	4.101	949	952	953	rBV3	1627	914	0.12%	0.014%
24	4.259	987	1001	1025	rBV2	124845	321196	41.89%	4.791%
25	4.645	1118	1121	1125	rBV6	1090	941	0.12%	0.014%
26	4.831	1176	1179	1180	rBV3	1083	735	0.10%	0.011%
27	4.966	1204	1221	1246	rBV3	286382	766766	100.00%	11.437%
28	5.281	1317	1319	1324	rBV6	1399	958	0.12%	0.014%
29	5.365	1342	1345	1349	rVB8	1460	1156	0.15%	0.017%
30	5.387	1349	1352	1353	rBV3	1298	696	0.09%	0.010%
31	5.471	1375	1378	1381	rBV4	1995	1898	0.25%	0.028%
32	5.542	1388	1400	1419	rBV	265541	551844	71.97%	8.231%
33	5.841	1481	1493	1514	rBV	281994	559275	72.94%	8.342%
34	5.998	1533	1542	1565	rVB	174064	347388	45.31%	5.182%
35	6.291	1630	1633	1634	rBV3	1140	700	0.09%	0.010%
36	6.429	1674	1676	1679	rBV4	1305	691	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030623.D
 Acq On : 18 Apr 2023 17:28
 Operator : SY/MD
 Sample : 02360-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.474	1687	1690	1691	rBV3	1435	856	0.11%	0.013%
38	6.571	1718	1720	1723	rBV3	1401	875	0.11%	0.013%
39	6.593	1723	1727	1731	rVB6	2518	2052	0.27%	0.031%
40	6.619	1731	1735	1736	rBV4	1246	853	0.11%	0.013%
41	6.690	1754	1757	1760	rBV4	1191	863	0.11%	0.013%
42	6.728	1766	1769	1772	rBV5	1269	1116	0.15%	0.017%
43	6.809	1788	1794	1798	rBV9	1372	1629	0.21%	0.024%
44	6.921	1819	1829	1844	rBV2	85718	156992	20.47%	2.342%
45	7.133	1891	1895	1898	rBV6	1326	1218	0.16%	0.018%
46	7.149	1898	1900	1905	rVB7	1428	946	0.12%	0.014%
47	7.252	1916	1932	1951	rBV	321002	578255	75.41%	8.625%
48	7.526	2014	2017	2018	rBV3	1291	849	0.11%	0.013%
49	7.561	2018	2028	2043	rVV	63255	113743	14.83%	1.697%
50	7.818	2106	2108	2111	rBV4	1439	923	0.12%	0.014%
51	8.034	2165	2175	2192	rBV	171145	322217	42.02%	4.806%
52	8.500	2317	2320	2324	rBV6	2433	2001	0.26%	0.030%
53	8.657	2367	2369	2375	rBV7	1819	1374	0.18%	0.020%
54	8.792	2399	2411	2431	rBV	411391	681543	88.89%	10.166%
55	9.140	2516	2519	2520	rBV3	1739	1028	0.13%	0.015%
56	9.207	2538	2540	2546	rVB5	2101	1494	0.19%	0.022%
57	9.628	2669	2671	2673	rBV3	1398	721	0.09%	0.011%
58	9.876	2746	2748	2750	rBV3	1717	845	0.11%	0.013%
59	9.927	2761	2764	2765	rBV3	1088	689	0.09%	0.010%
60	10.085	2810	2813	2815	rBV4	1229	713	0.09%	0.011%
61	10.104	2815	2819	2822	rBV6	1884	1422	0.19%	0.021%
62	10.162	2824	2837	2853	rBV	240705	385851	50.32%	5.755%
63	10.284	2871	2875	2878	rBV5	2370	1756	0.23%	0.026%
64	10.333	2886	2890	2896	rBV9	2427	2376	0.31%	0.035%
65	10.378	2901	2904	2911	rBV9	1842	1857	0.24%	0.028%
66	10.551	2950	2958	2961	rBV10	1567	1457	0.19%	0.022%
67	10.982	3089	3092	3093	rBV2	1770	784	0.10%	0.012%
68	11.194	3147	3158	3174	rBV	388198	604608	78.85%	9.018%
69	11.326	3197	3199	3200	rBV2	2232	847	0.11%	0.013%
70	11.423	3224	3229	3231	rBV5	2027	1734	0.23%	0.026%
71	11.570	3264	3275	3290	rVB	328509	519231	67.72%	7.745%
72	11.972	3394	3400	3402	rBV7	1624	1368	0.18%	0.020%
73	11.998	3405	3408	3410	rBV4	1736	1124	0.15%	0.017%
74	12.239	3481	3483	3486	rVB4	1675	803	0.10%	0.012%
75	12.255	3486	3488	3490	rBV3	1298	782	0.10%	0.012%
76	12.361	3517	3521	3523	rBV5	2212	1314	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030623.D
 Acq On : 18 Apr 2023 17:28
 Operator : SY/MD
 Sample : 02360-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.406	3531	3535	3536	rBV4	1911	1223	0.16%	0.018%
78	12.477	3553	3557	3558	rBV4	1625	862	0.11%	0.013%
79	12.619	3598	3601	3604	rBV4	1497	1034	0.13%	0.015%
80	12.731	3634	3636	3641	rBV4	1064	710	0.09%	0.011%
81	12.773	3645	3649	3650	rBV4	1723	1338	0.17%	0.020%
82	12.857	3671	3675	3677	rBV5	1006	659	0.09%	0.010%
83	13.033	3727	3730	3736	rBV7	1774	1735	0.23%	0.026%
84	13.140	3760	3763	3766	rBV5	1060	737	0.10%	0.011%
85	13.236	3786	3793	3798	rBV10	1925	3037	0.40%	0.045%
86	13.316	3817	3818	3822	rBV4	1400	746	0.10%	0.011%
87	13.390	3838	3841	3843	rBV4	1781	958	0.12%	0.014%
88	13.429	3850	3853	3854	rBV3	2007	861	0.11%	0.013%
89	13.541	3882	3888	3891	rBV7	1866	1729	0.23%	0.026%
90	13.657	3920	3924	3926	rBV5	2803	1999	0.26%	0.030%
91	13.728	3944	3946	3949	rBV4	2064	1099	0.14%	0.016%
92	13.815	3970	3973	3975	rBV4	1204	748	0.10%	0.011%
93	13.931	4005	4009	4013	rBV6	1914	1795	0.23%	0.027%
94	14.001	4027	4031	4034	rBV5	1549	1290	0.17%	0.019%
95	14.120	4065	4068	4071	rBV5	1649	1251	0.16%	0.019%
96	14.268	4111	4114	4116	rBV3	1406	805	0.10%	0.012%
97	14.323	4129	4131	4134	rVB4	1671	680	0.09%	0.010%
98	14.342	4134	4137	4138	rBV3	1697	879	0.11%	0.013%
99	14.461	4172	4174	4177	rVB4	1915	855	0.11%	0.013%
100	14.721	4253	4255	4259	rBV4	1455	1145	0.15%	0.017%




Sum of corrected areas: 6704238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030623.D
Acq On : 18 Apr 2023 17:28
Operator : SY/MD
Sample : 02360-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

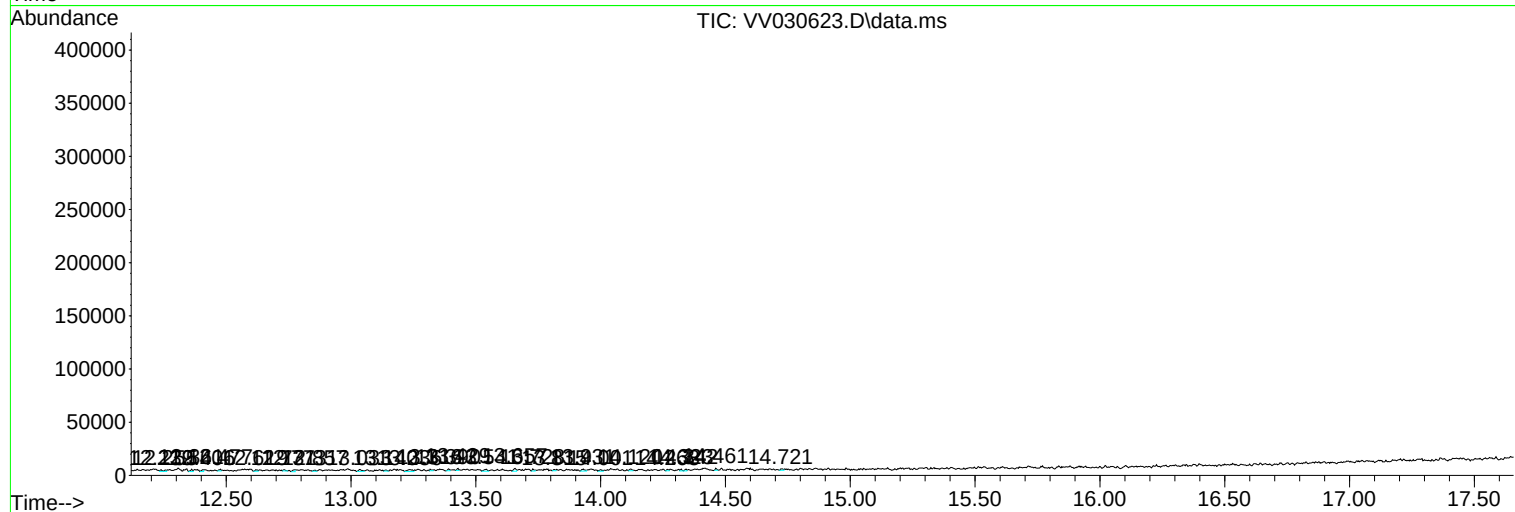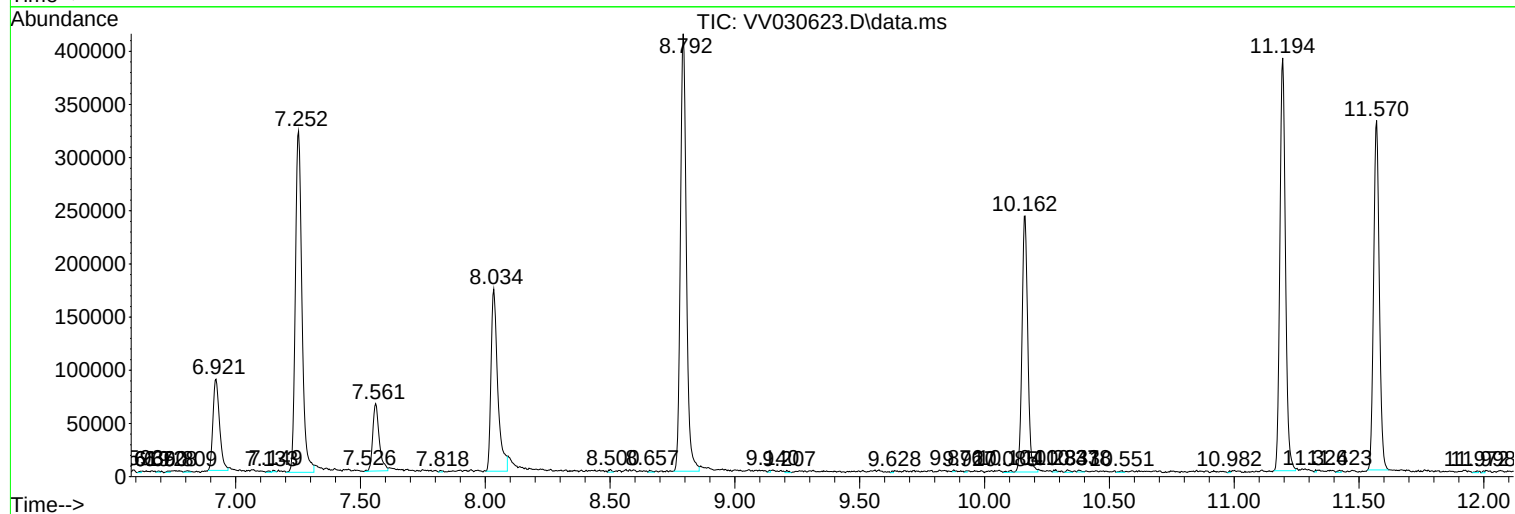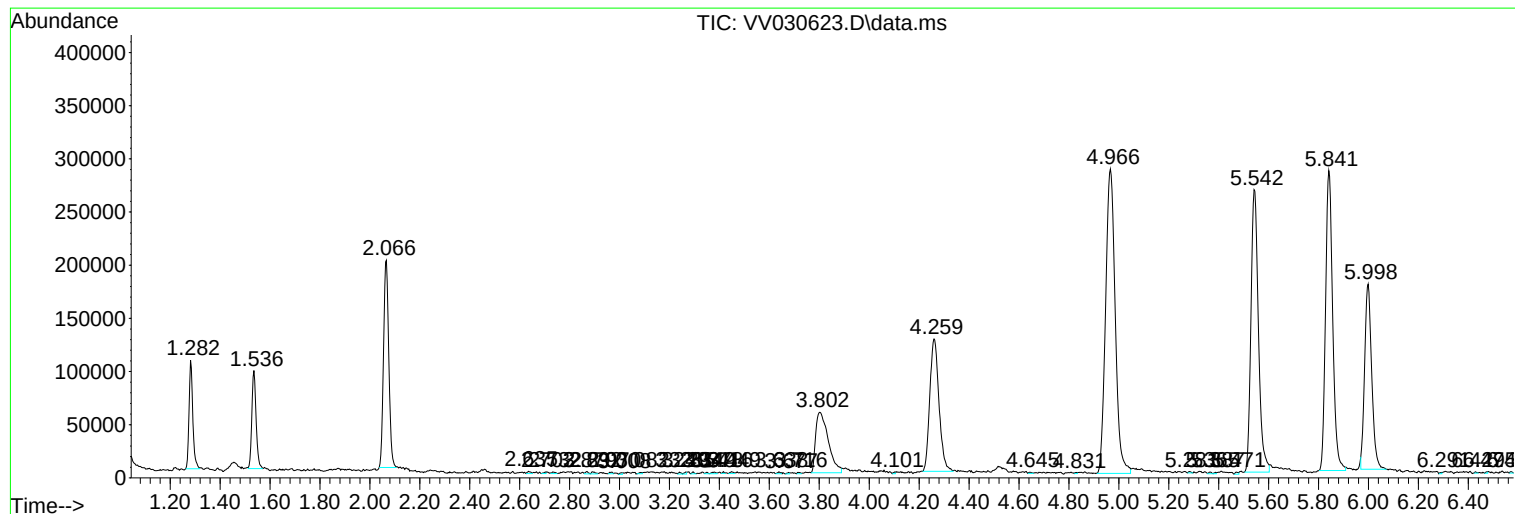

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030623.D
Acq On : 18 Apr 2023 17:28
Operator : SY/MD
Sample : 02360-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030623.D
Acq On : 18 Apr 2023 17:28
Operator : SY/MD
Sample : 02360-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------