

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030624.D
 Acq On : 18 Apr 2023 17:52
 Operator : SY/MD
 Sample : 02360-07DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rBV	94771	105914	14.44%	1.622%
2	1.536	148	154	166	rVB	90265	104745	14.28%	1.604%
3	2.066	310	319	333	rVB	190670	280839	38.29%	4.300%
4	2.561	468	473	477	rBV8	2134	2308	0.31%	0.035%
5	2.661	502	504	509	rBV4	1422	1165	0.16%	0.018%
6	2.728	522	525	530	rBV6	2377	2081	0.28%	0.032%
7	2.838	555	559	560	rBV4	1165	671	0.09%	0.010%
8	2.870	567	569	571	rBV3	1794	850	0.12%	0.013%
9	3.040	620	622	624	rBV3	1320	685	0.09%	0.010%
10	3.150	654	656	658	rBV3	1113	667	0.09%	0.010%
11	3.162	658	660	662	rVV3	1739	896	0.12%	0.014%
12	3.188	666	668	670	rBV3	1062	577	0.08%	0.009%
13	3.262	687	691	694	rBV6	1637	1243	0.17%	0.019%
14	3.445	745	748	751	rBV5	1461	1127	0.15%	0.017%
15	3.465	751	754	759	rVV8	1190	1247	0.17%	0.019%
16	3.625	801	804	808	rBV5	1193	1041	0.14%	0.016%
17	3.654	808	813	815	rVV5	2449	2231	0.30%	0.034%
18	3.687	819	823	824	rBV4	1228	738	0.10%	0.011%
19	3.802	848	859	884	rBV3	54084	197606	26.94%	3.026%
20	4.259	988	1001	1022	rBV	124641	310230	42.29%	4.750%
21	4.642	1118	1120	1123	rBV4	1103	717	0.10%	0.011%
22	4.693	1134	1136	1144	rVB7	1628	1611	0.22%	0.025%
23	4.777	1160	1162	1164	rBV3	1237	593	0.08%	0.009%
24	4.818	1173	1175	1176	rBV2	1195	573	0.08%	0.009%
25	4.870	1187	1191	1193	rBV5	1458	1214	0.17%	0.019%
26	4.966	1205	1221	1242	rBV3	277149	733515	100.00%	11.232%
27	5.278	1316	1318	1320	rBV3	1210	620	0.08%	0.009%
28	5.542	1389	1400	1420	rBV	270041	554957	75.66%	8.498%
29	5.841	1482	1493	1515	rBV	230734	458595	62.52%	7.022%
30	5.998	1531	1542	1564	rVB	173877	351857	47.97%	5.388%
31	6.294	1632	1634	1636	rVB3	1718	616	0.08%	0.009%
32	6.465	1681	1687	1688	rBV5	1810	1507	0.21%	0.023%
33	6.715	1762	1765	1766	rBV3	1347	745	0.10%	0.011%
34	6.780	1782	1785	1788	rBV4	1176	868	0.12%	0.013%
35	6.812	1793	1795	1797	rBV3	1429	676	0.09%	0.010%
36	6.921	1818	1829	1850	rBV	86329	162907	22.21%	2.494%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030624.D
 Acq On : 18 Apr 2023 17:52
 Operator : SY/MD
 Sample : 02360-07DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.085	1878	1880	1881	rBV2	1575	674	0.09%	0.010%
38	7.204	1914	1917	1920	rBV4	2007	1301	0.18%	0.020%
39	7.252	1921	1932	1959	rVV	309729	561389	76.53%	8.596%
40	7.561	2020	2028	2042	rBV	59457	100064	13.64%	1.532%
41	7.789	2097	2099	2101	rBV3	1233	557	0.08%	0.009%
42	7.879	2123	2127	2129	rBV5	2848	2239	0.31%	0.034%
43	8.034	2163	2175	2200	rBV	165418	325196	44.33%	4.979%
44	8.583	2344	2346	2349	rVB3	1443	534	0.07%	0.008%
45	8.619	2353	2357	2358	rBV3	1583	1021	0.14%	0.016%
46	8.667	2370	2372	2373	rBV2	1166	538	0.07%	0.008%
47	8.686	2375	2378	2380	rVB4	1727	844	0.12%	0.013%
48	8.728	2388	2391	2394	rBV4	2398	2042	0.28%	0.031%
49	8.792	2400	2411	2431	rBV	412129	690150	94.09%	10.568%
50	9.223	2542	2545	2546	rBV3	1142	588	0.08%	0.009%
51	9.317	2569	2574	2578	rBV7	2943	2685	0.37%	0.041%
52	9.387	2592	2596	2598	rVB4	1514	975	0.13%	0.015%
53	9.410	2601	2603	2606	rBV3	2058	1628	0.22%	0.025%
54	9.519	2635	2637	2640	rBV3	1466	945	0.13%	0.014%
55	9.664	2680	2682	2684	rBV3	1373	554	0.08%	0.008%
56	9.696	2688	2692	2696	rVB7	1796	1469	0.20%	0.022%
57	9.725	2696	2701	2702	rBV5	2436	1883	0.26%	0.029%
58	9.918	2760	2761	2763	rBV2	1051	491	0.07%	0.008%
59	9.960	2772	2774	2779	rVB6	1442	1007	0.14%	0.015%
60	10.162	2826	2837	2852	rVB	229123	369720	50.40%	5.661%
61	10.329	2885	2889	2892	rBV5	2294	2048	0.28%	0.031%
62	10.603	2970	2974	2975	rBV4	1063	631	0.09%	0.010%
63	10.661	2990	2992	2996	rBV5	1582	1005	0.14%	0.015%
64	10.780	3026	3029	3031	rVB3	1775	910	0.12%	0.014%
65	10.792	3031	3033	3037	rBV3	1316	744	0.10%	0.011%
66	10.911	3067	3070	3073	rBV4	1703	1027	0.14%	0.016%
67	10.963	3084	3086	3092	rVB8	1226	893	0.12%	0.014%
68	11.011	3097	3101	3103	rBV4	1980	1644	0.22%	0.025%
69	11.072	3118	3120	3124	rVB5	2529	1538	0.21%	0.024%
70	11.098	3124	3128	3131	rBV6	2522	2573	0.35%	0.039%
71	11.194	3147	3158	3175	rBV	386530	617190	84.14%	9.450%
72	11.300	3189	3191	3194	rBV3	1312	545	0.07%	0.008%
73	11.474	3240	3245	3249	rBV6	1626	1567	0.21%	0.024%
74	11.516	3253	3258	3262	rBV7	2049	1999	0.27%	0.031%
75	11.571	3262	3275	3292	rBV	315159	512951	69.93%	7.854%
76	11.725	3321	3323	3324	rBV2	1946	827	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030624.D
 Acq On : 18 Apr 2023 17:52
 Operator : SY/MD
 Sample : 02360-07DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.905	3376	3379	3380	rBV4	1670	956	0.13%	0.015%
78	12.066	3428	3429	3431	rVB3	1802	461	0.06%	0.007%
79	12.082	3431	3434	3436	rBV4	1868	1368	0.19%	0.021%
80	12.152	3452	3456	3458	rBV5	1536	1113	0.15%	0.017%
81	12.361	3520	3521	3523	rBV2	1119	575	0.08%	0.009%
82	12.435	3542	3544	3546	rBV4	1087	657	0.09%	0.010%
83	12.448	3546	3548	3551	rVB4	2015	1104	0.15%	0.017%
84	12.538	3574	3576	3578	rBV3	1349	734	0.10%	0.011%
85	12.606	3595	3597	3601	rBV5	1329	1007	0.14%	0.015%
86	12.770	3645	3648	3652	rBV5	1244	1203	0.16%	0.018%
87	12.808	3657	3660	3661	rBV3	1811	993	0.14%	0.015%
88	12.857	3672	3675	3676	rBV3	1836	1172	0.16%	0.018%
89	12.905	3689	3690	3692	rBV2	1209	495	0.07%	0.008%
90	13.091	3745	3748	3752	rVB6	1519	1155	0.16%	0.018%
91	13.111	3752	3754	3756	rVB3	1272	685	0.09%	0.010%
92	13.130	3756	3760	3762	rBV4	1700	1499	0.20%	0.023%
93	13.287	3806	3809	3811	rBV5	867	701	0.10%	0.011%
94	13.352	3825	3829	3832	rBV4	1867	1818	0.25%	0.028%
95	13.496	3871	3874	3875	rBV3	1059	462	0.06%	0.007%
96	13.876	3989	3992	3996	rBV6	1398	1491	0.20%	0.023%
97	13.905	3999	4001	4004	rBV4	1371	1131	0.15%	0.017%
98	14.316	4126	4129	4133	rBV5	1803	1551	0.21%	0.024%
99	14.554	4199	4203	4208	rBV8	2346	2179	0.30%	0.033%
100	15.046	4354	4356	4360	rVB5	2336	1280	0.17%	0.020%




Sum of corrected areas: 6530808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030624.D
Acq On : 18 Apr 2023 17:52
Operator : SY/MD
Sample : 02360-07DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

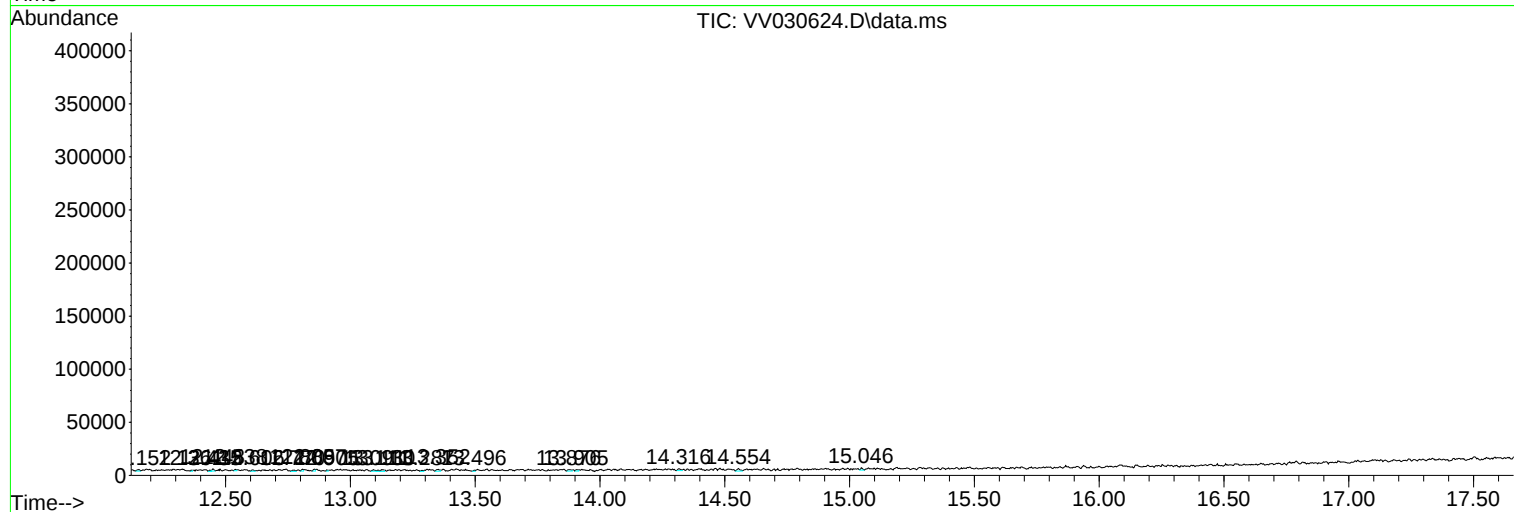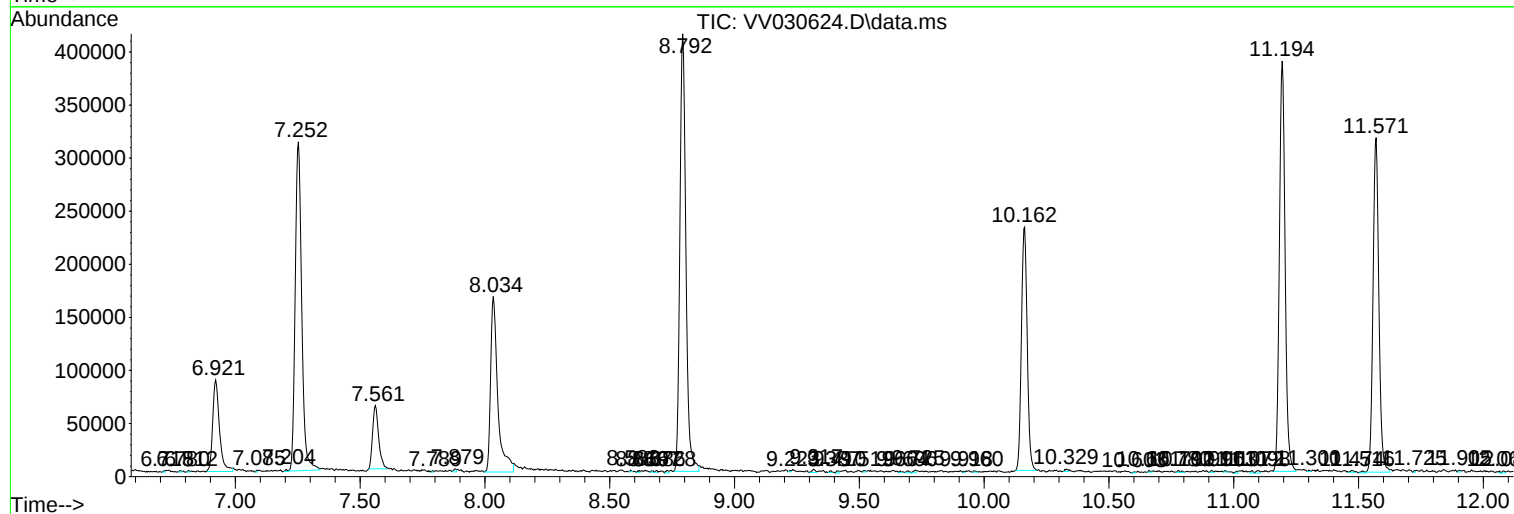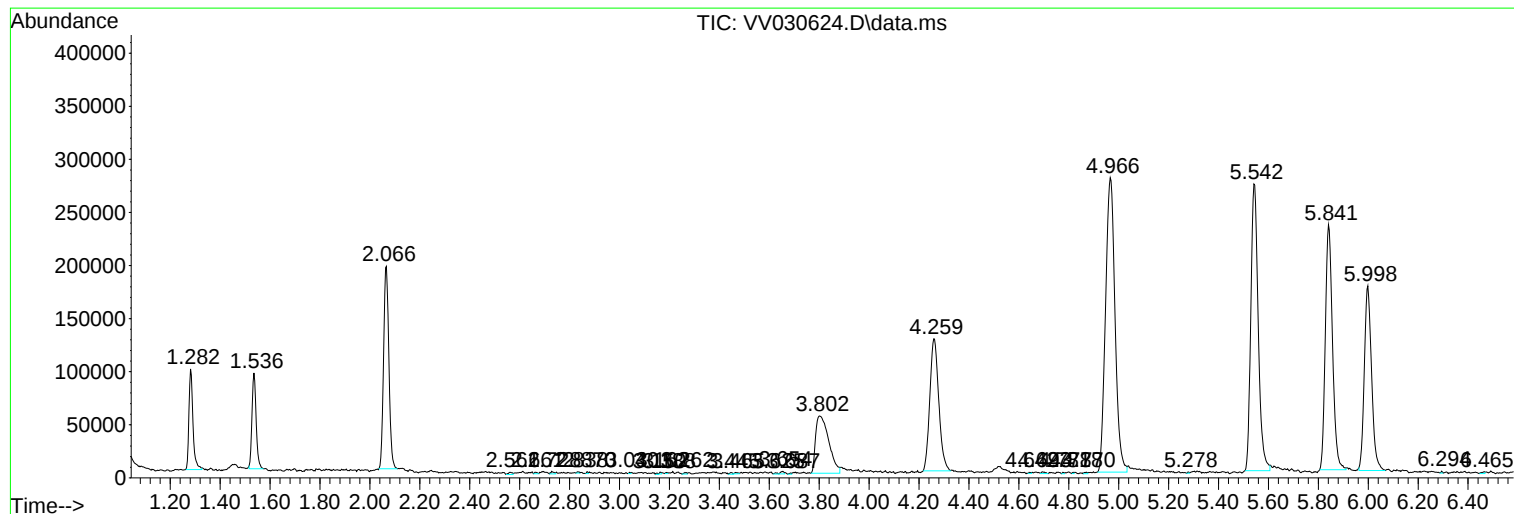

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030624.D
Acq On : 18 Apr 2023 17:52
Operator : SY/MD
Sample : 02360-07DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030624.D
Acq On : 18 Apr 2023 17:52
Operator : SY/MD
Sample : 02360-07DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------