

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030625.D
 Acq On : 18 Apr 2023 18:16
 Operator : SY/MD
 Sample : 02360-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	96083	105932	14.48%	1.632%
2	1.536	147	154	166	rVB	90741	107148	14.65%	1.651%
3	2.066	310	319	334	rVB	192271	282732	38.66%	4.357%
4	2.394	417	421	424	rVB4	2057	1457	0.20%	0.022%
5	2.446	431	437	439	rBV7	2757	2520	0.34%	0.039%
6	2.690	508	513	514	rBV6	1774	1569	0.21%	0.024%
7	2.767	534	537	541	rBV6	1299	997	0.14%	0.015%
8	2.925	580	586	592	rBV10	2456	2513	0.34%	0.039%
9	3.163	656	660	667	rBV9	1973	2502	0.34%	0.039%
10	3.211	672	675	679	rBV6	1494	1294	0.18%	0.020%
11	3.262	688	691	695	rBV6	2078	1787	0.24%	0.028%
12	3.294	698	701	707	rVB7	2357	1947	0.27%	0.030%
13	3.381	726	728	729	rBV2	1525	618	0.08%	0.010%
14	3.452	747	750	751	rBV3	1040	641	0.09%	0.010%
15	3.497	760	764	767	rBV5	1135	1277	0.17%	0.020%
16	3.532	772	775	779	rVB6	938	613	0.08%	0.009%
17	3.555	779	782	785	rBV5	1356	1037	0.14%	0.016%
18	3.606	790	798	800	rBV9	1882	1664	0.23%	0.026%
19	3.716	829	832	835	rVB5	1299	684	0.09%	0.011%
20	3.732	835	837	839	rVB2	1430	541	0.07%	0.008%
21	3.802	848	859	862	rBV	59647	110307	15.08%	1.700%
22	4.037	930	932	934	rBV3	1415	607	0.08%	0.009%
23	4.208	983	985	986	rBV2	1686	706	0.10%	0.011%
24	4.259	987	1001	1022	rVV	123879	317800	43.45%	4.897%
25	4.619	1110	1113	1115	rBV3	1746	1111	0.15%	0.017%
26	4.699	1134	1138	1143	rVB8	2031	1724	0.24%	0.027%
27	4.966	1206	1221	1241	rBV2	279278	731383	100.00%	11.270%
28	5.542	1388	1400	1420	rBV	266794	552440	75.53%	8.513%
29	5.841	1482	1493	1514	rBV	240135	476105	65.10%	7.337%
30	5.995	1531	1541	1560	rVB	168567	343088	46.91%	5.287%
31	6.391	1661	1664	1665	rBV3	1560	827	0.11%	0.013%
32	6.449	1680	1682	1686	rVB4	1110	583	0.08%	0.009%
33	6.539	1708	1710	1712	rBV3	1277	639	0.09%	0.010%
34	6.658	1744	1747	1751	rBV6	1337	1280	0.18%	0.020%
35	6.751	1774	1776	1779	rBV3	2030	1280	0.18%	0.020%
36	6.847	1804	1806	1809	rBV4	2076	1672	0.23%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030625.D
 Acq On : 18 Apr 2023 18:16
 Operator : SY/MD
 Sample : 02360-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1848	rBV	86300	161525	22.08%	2.489%
38	7.195	1910	1914	1918	rBV7	1474	1319	0.18%	0.020%
39	7.252	1920	1932	1956	rBV	314404	571094	78.08%	8.800%
40	7.561	2018	2028	2044	rBV	62744	116274	15.90%	1.792%
41	7.838	2112	2114	2116	rBV3	1525	557	0.08%	0.009%
42	8.034	2166	2175	2202	rBV	164741	324389	44.35%	4.999%
43	8.304	2257	2259	2261	rVB2	1675	561	0.08%	0.009%
44	8.477	2310	2313	2314	rBV3	1607	926	0.13%	0.014%
45	8.731	2391	2392	2395	rVB3	1351	611	0.08%	0.009%
46	8.748	2395	2397	2398	rBV2	1374	687	0.09%	0.011%
47	8.793	2399	2411	2434	rVV	409108	685062	93.67%	10.557%
48	9.217	2541	2543	2548	rVB5	2089	973	0.13%	0.015%
49	9.297	2563	2568	2571	rBV6	1995	1717	0.23%	0.026%
50	9.320	2573	2575	2577	rBV2	1630	810	0.11%	0.012%
51	9.484	2624	2626	2628	rVB2	1653	600	0.08%	0.009%
52	9.519	2634	2637	2639	rBV4	2030	1504	0.21%	0.023%
53	9.584	2655	2657	2660	rBV5	1460	926	0.13%	0.014%
54	9.632	2666	2672	2674	rBV7	1635	1652	0.23%	0.025%
55	9.921	2759	2762	2764	rBV4	1070	744	0.10%	0.011%
56	10.063	2804	2806	2807	rBV2	1339	583	0.08%	0.009%
57	10.162	2825	2837	2855	rBV	229157	371983	50.86%	5.732%
58	10.407	2910	2913	2917	rBV7	2176	2029	0.28%	0.031%
59	10.458	2927	2929	2930	rBV2	1738	753	0.10%	0.012%
60	10.561	2959	2961	2965	rVB4	1550	780	0.11%	0.012%
61	10.580	2965	2967	2970	rBV4	1138	841	0.11%	0.013%
62	10.661	2991	2992	2996	rVB4	2348	926	0.13%	0.014%
63	10.776	3025	3028	3030	rBV3	1799	1187	0.16%	0.018%
64	10.796	3031	3034	3037	rVV5	1520	1268	0.17%	0.020%
65	11.037	3107	3109	3112	rBV4	1464	1032	0.14%	0.016%
66	11.114	3130	3133	3134	rBV3	1070	529	0.07%	0.008%
67	11.194	3147	3158	3177	rBV	384716	610739	83.50%	9.411%
68	11.458	3235	3240	3242	rVB5	1437	983	0.13%	0.015%
69	11.484	3242	3248	3251	rVB6	2594	1889	0.26%	0.029%
70	11.571	3258	3275	3291	rBV	327592	527784	72.16%	8.133%
71	11.992	3401	3406	3407	rBV4	2279	1678	0.23%	0.026%
72	12.034	3416	3419	3420	rBV3	946	592	0.08%	0.009%
73	12.114	3442	3444	3447	rBV4	1372	706	0.10%	0.011%
74	12.130	3447	3449	3452	rBV4	1659	1274	0.17%	0.020%
75	12.223	3474	3478	3480	rBV5	2064	1291	0.18%	0.020%
76	12.243	3480	3484	3486	rBV5	1291	1000	0.14%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030625.D
 Acq On : 18 Apr 2023 18:16
 Operator : SY/MD
 Sample : 02360-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.349	3513	3517	3520	rBV7	1378	1568	0.21%	0.024%
78	12.403	3531	3534	3535	rBV2	1285	538	0.07%	0.008%
79	12.532	3572	3574	3577	rBV4	851	586	0.08%	0.009%
80	12.606	3594	3597	3598	rBV3	1440	692	0.09%	0.011%
81	12.690	3620	3623	3626	rBV5	974	755	0.10%	0.012%
82	12.805	3656	3659	3661	rBV4	1546	866	0.12%	0.013%
83	12.834	3666	3668	3673	rVB5	1943	1724	0.24%	0.027%
84	12.908	3687	3691	3692	rBV4	1173	763	0.10%	0.012%
85	12.940	3698	3701	3704	rBV6	1406	1213	0.17%	0.019%
86	13.210	3782	3785	3786	rBV3	1262	797	0.11%	0.012%
87	13.271	3802	3804	3805	rBV2	1251	648	0.09%	0.010%
88	13.307	3813	3815	3819	rVB5	1901	1138	0.16%	0.018%
89	13.352	3824	3829	3831	rBV6	1261	1139	0.16%	0.018%
90	13.497	3872	3874	3875	rBV2	1679	808	0.11%	0.012%
91	13.538	3883	3887	3888	rBV4	2954	2016	0.28%	0.031%
92	13.677	3924	3930	3932	rBV7	2436	2088	0.29%	0.032%
93	13.799	3964	3968	3969	rBV4	1623	1159	0.16%	0.018%
94	14.046	4043	4045	4046	rBV2	1355	585	0.08%	0.009%
95	14.091	4055	4059	4061	rBV4	1945	1683	0.23%	0.026%
96	14.329	4128	4133	4136	rBV7	1393	1616	0.22%	0.025%
97	14.361	4141	4143	4147	rBV5	1721	1154	0.16%	0.018%
98	14.468	4172	4176	4178	rBV5	1283	1092	0.15%	0.017%
99	14.522	4191	4193	4194	rBV2	1335	702	0.10%	0.011%
100	14.548	4198	4201	4206	rVV6	1615	1296	0.18%	0.020%




Sum of corrected areas: 6489429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030625.D
Acq On : 18 Apr 2023 18:16
Operator : SY/MD
Sample : 02360-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

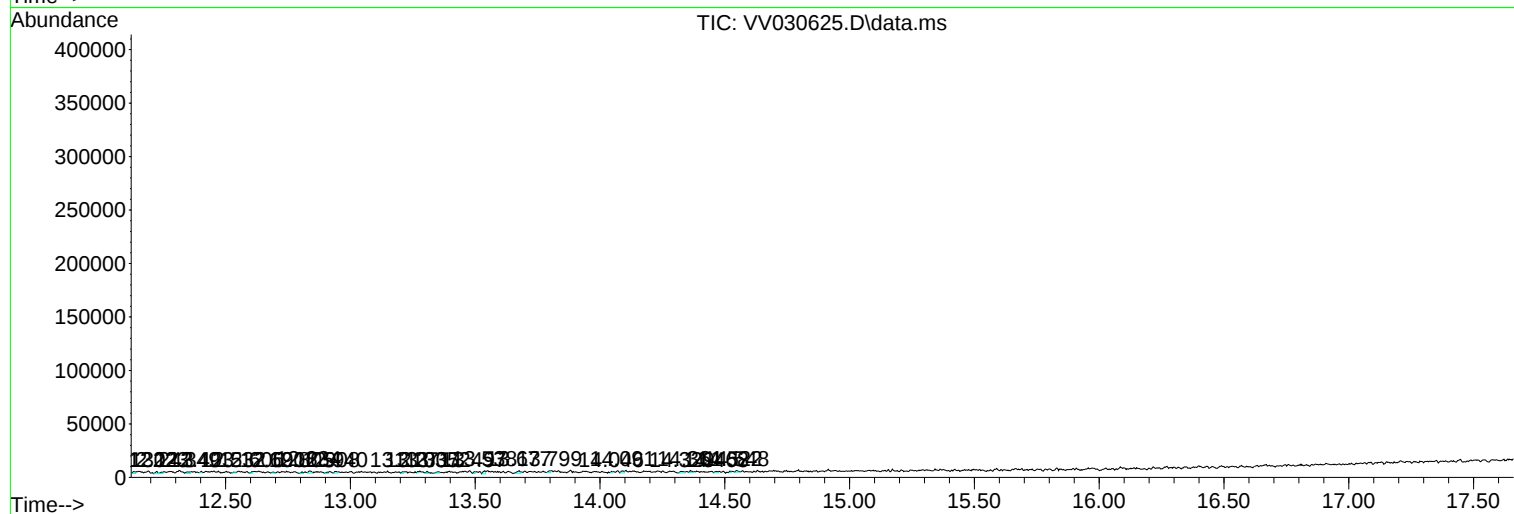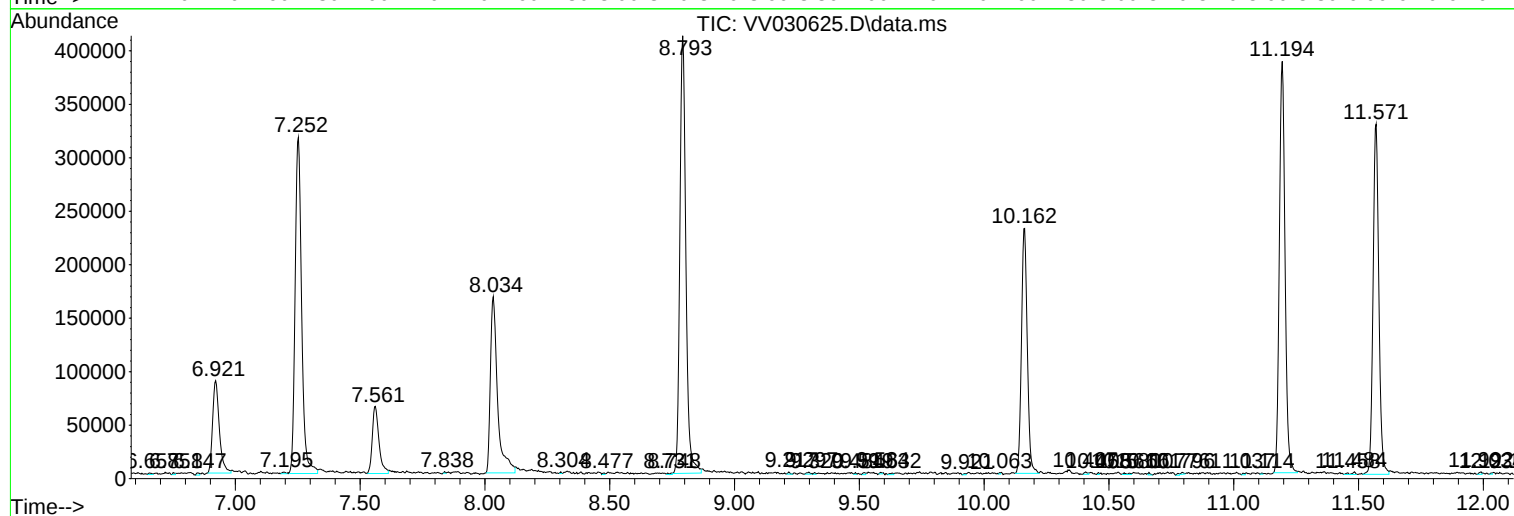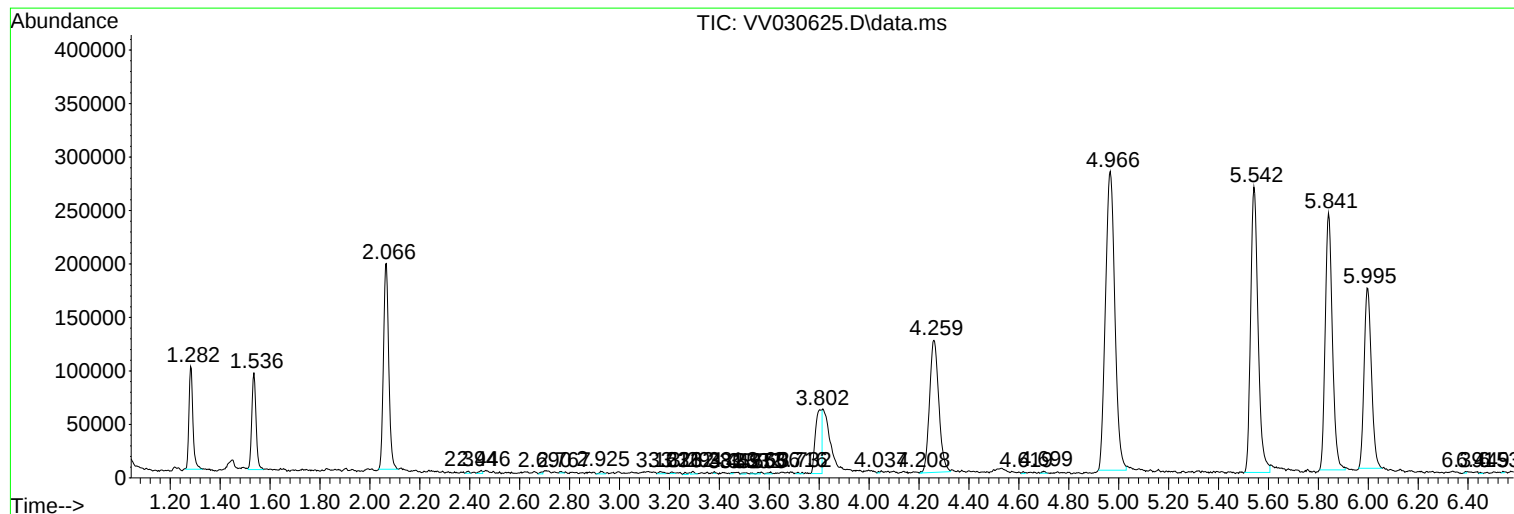

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030625.D
Acq On : 18 Apr 2023 18:16
Operator : SY/MD
Sample : 02360-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030625.D
Acq On : 18 Apr 2023 18:16
Operator : SY/MD
Sample : 02360-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------