

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030626.D
 Acq On : 18 Apr 2023 18:40
 Operator : SY/MD
 Sample : 02360-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	91	rVB	93780	102326	11.47%	1.560%
2	1.535	148	154	165	rVB	88934	101538	11.38%	1.548%
3	2.066	310	319	335	rVB	186610	273603	30.67%	4.171%
4	2.506	453	456	459	rBV4	1819	1118	0.13%	0.017%
5	2.535	464	465	468	rVB2	1170	530	0.06%	0.008%
6	2.558	468	472	474	rBV5	1686	1137	0.13%	0.017%
7	2.632	493	495	498	rBV4	1282	678	0.08%	0.010%
8	2.680	508	510	513	rBV4	1478	1039	0.12%	0.016%
9	2.937	588	590	592	rBV2	1074	361	0.04%	0.006%
10	3.008	611	612	616	rBV4	1164	786	0.09%	0.012%
11	3.037	618	621	626	rBV5	1727	1764	0.20%	0.027%
12	3.063	627	629	633	rBV5	1371	623	0.07%	0.009%
13	3.121	642	647	650	rBV6	1680	2093	0.23%	0.032%
14	3.182	664	666	669	rVB4	1044	591	0.07%	0.009%
15	3.198	669	671	672	rBV2	978	498	0.06%	0.008%
16	3.207	672	674	680	rVB6	3113	2553	0.29%	0.039%
17	3.233	680	682	683	rBV2	1866	904	0.10%	0.014%
18	3.301	701	703	704	rBV2	1069	434	0.05%	0.007%
19	3.384	727	729	733	rVB5	1106	460	0.05%	0.007%
20	3.432	741	744	747	rBV5	1750	1046	0.12%	0.016%
21	3.500	763	765	768	rBV4	1892	809	0.09%	0.012%
22	3.561	782	784	787	rBV3	900	342	0.04%	0.005%
23	3.574	787	788	792	rVB4	1093	371	0.04%	0.006%
24	3.635	803	807	810	rBV5	1775	1755	0.20%	0.027%
25	3.699	825	827	828	rBV2	1382	611	0.07%	0.009%
26	3.760	844	846	849	rVB4	1585	671	0.08%	0.010%
27	3.799	849	858	890	rBV	50276	149906	16.80%	2.285%
28	4.494	1070	1074	1077	rBV4	1548	1316	0.15%	0.020%
29	4.741	1149	1151	1152	rBV2	1135	504	0.06%	0.008%
30	4.776	1159	1162	1165	rBV5	1446	928	0.10%	0.014%
31	4.844	1181	1183	1186	rBV4	1040	522	0.06%	0.008%
32	4.879	1192	1194	1199	rVB5	1317	765	0.09%	0.012%
33	4.966	1205	1221	1246	rBV2	280728	742702	83.25%	11.322%
34	5.394	1350	1354	1357	rBV6	1859	1188	0.13%	0.018%
35	5.542	1389	1400	1418	rBV	270855	557598	62.50%	8.500%
36	5.841	1481	1493	1517	rBV	453851	892142	100.00%	13.600%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030626.D
 Acq On : 18 Apr 2023 18:40
 Operator : SY/MD
 Sample : 02360-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.998	1531	1542	1560	rBV	168369	337443	37.82%	5.144%
38	6.339	1646	1648	1650	rBV4	1393	637	0.07%	0.010%
39	6.400	1663	1667	1668	rBV4	1554	994	0.11%	0.015%
40	6.429	1673	1676	1680	rVB5	1828	1612	0.18%	0.025%
41	6.712	1761	1764	1765	rBV3	1603	928	0.10%	0.014%
42	6.738	1770	1772	1773	rBV2	1167	615	0.07%	0.009%
43	6.776	1781	1784	1786	rBV4	1395	1061	0.12%	0.016%
44	6.873	1809	1814	1816	rBV6	1592	1631	0.18%	0.025%
45	6.921	1820	1829	1843	rVV	81419	146761	16.45%	2.237%
46	7.252	1921	1932	1952	rBV	310626	550744	61.73%	8.395%
47	7.513	2011	2013	2015	rBV3	1583	702	0.08%	0.011%
48	7.561	2019	2028	2043	rVV	61516	107190	12.01%	1.634%
49	7.892	2127	2131	2133	rBV5	1835	1345	0.15%	0.021%
50	7.956	2149	2151	2154	rBV4	2091	1324	0.15%	0.020%
51	8.034	2166	2175	2208	rBV	158810	324360	36.36%	4.944%
52	8.394	2285	2287	2288	rBV2	1461	681	0.08%	0.010%
53	8.609	2350	2354	2357	rBV6	1917	1481	0.17%	0.023%
54	8.792	2400	2411	2435	rBV	421655	698406	78.28%	10.646%
55	8.979	2467	2469	2472	rBV3	1658	684	0.08%	0.010%
56	9.323	2574	2576	2579	rVB3	1694	650	0.07%	0.010%
57	9.352	2582	2585	2590	rVB8	1867	1171	0.13%	0.018%
58	9.394	2596	2598	2600	rVB4	1598	500	0.06%	0.008%
59	9.419	2602	2606	2608	rBV5	1461	1283	0.14%	0.020%
60	9.461	2615	2619	2621	rBV4	1667	1342	0.15%	0.020%
61	9.548	2638	2646	2647	rBV7	2485	2821	0.32%	0.043%
62	9.593	2657	2660	2662	rBV4	1387	1050	0.12%	0.016%
63	9.731	2701	2703	2705	rBV3	1183	422	0.05%	0.006%
64	9.808	2725	2727	2732	rBV5	1553	1344	0.15%	0.020%
65	9.960	2773	2774	2777	rBV3	1351	707	0.08%	0.011%
66	10.082	2809	2812	2813	rBV2	1416	582	0.07%	0.009%
67	10.162	2826	2837	2852	rBV	228611	363679	40.76%	5.544%
68	10.445	2921	2925	2926	rBV4	1709	902	0.10%	0.014%
69	10.558	2957	2960	2961	rBV2	1066	698	0.08%	0.011%
70	10.641	2984	2986	2990	rVB6	1753	1138	0.13%	0.017%
71	10.667	2990	2994	2995	rBV4	1665	929	0.10%	0.014%
72	10.779	3028	3029	3031	rBV	1509	818	0.09%	0.012%
73	10.895	3062	3065	3066	rBV2	1037	631	0.07%	0.010%
74	11.024	3102	3105	3108	rBV5	2046	1664	0.19%	0.025%
75	11.040	3108	3110	3116	rBV7	929	959	0.11%	0.015%
76	11.069	3116	3119	3120	rBV3	1657	940	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030626.D
 Acq On : 18 Apr 2023 18:40
 Operator : SY/MD
 Sample : 02360-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3147	3158	3180	rVB	388238	622160	69.74%	9.484%
78	11.570	3264	3275	3293	rVB	322529	506369	56.76%	7.719%
79	11.792	3342	3344	3347	rVB3	1981	1031	0.12%	0.016%
80	11.895	3374	3376	3378	rBV3	1493	610	0.07%	0.009%
81	12.046	3421	3423	3427	rBV4	1603	932	0.10%	0.014%
82	12.265	3489	3491	3496	rBV5	1611	1023	0.11%	0.016%
83	12.291	3496	3499	3500	rBV3	1979	1073	0.12%	0.016%
84	12.516	3566	3569	3572	rBV4	2162	1471	0.16%	0.022%
85	12.564	3581	3584	3585	rBV3	1741	1019	0.11%	0.016%
86	12.728	3633	3635	3637	rBV3	810	430	0.05%	0.007%
87	13.320	3816	3819	3822	rBV5	1773	1357	0.15%	0.021%
88	13.393	3840	3842	3845	rBV4	1420	677	0.08%	0.010%
89	13.516	3876	3880	3882	rBV4	2157	1431	0.16%	0.022%
90	13.670	3927	3928	3931	rVB3	1103	497	0.06%	0.008%
91	13.744	3948	3951	3957	rVB7	1480	1388	0.16%	0.021%
92	13.924	4005	4007	4008	rBV2	2130	899	0.10%	0.014%
93	14.130	4067	4071	4073	rBV4	1192	883	0.10%	0.013%
94	14.156	4077	4079	4083	rVB5	1887	1193	0.13%	0.018%
95	14.204	4092	4094	4095	rBV2	974	361	0.04%	0.006%
96	14.258	4109	4111	4115	rBV5	1671	1369	0.15%	0.021%
97	14.564	4204	4206	4207	rBV2	1542	558	0.06%	0.009%
98	14.709	4246	4251	4255	rVB6	2237	2199	0.25%	0.034%
99	14.728	4255	4257	4260	rBV4	1647	1092	0.12%	0.017%
100	14.792	4275	4277	4279	rBV3	2278	976	0.11%	0.015%




Sum of corrected areas: 6560039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030626.D
Acq On : 18 Apr 2023 18:40
Operator : SY/MD
Sample : 02360-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

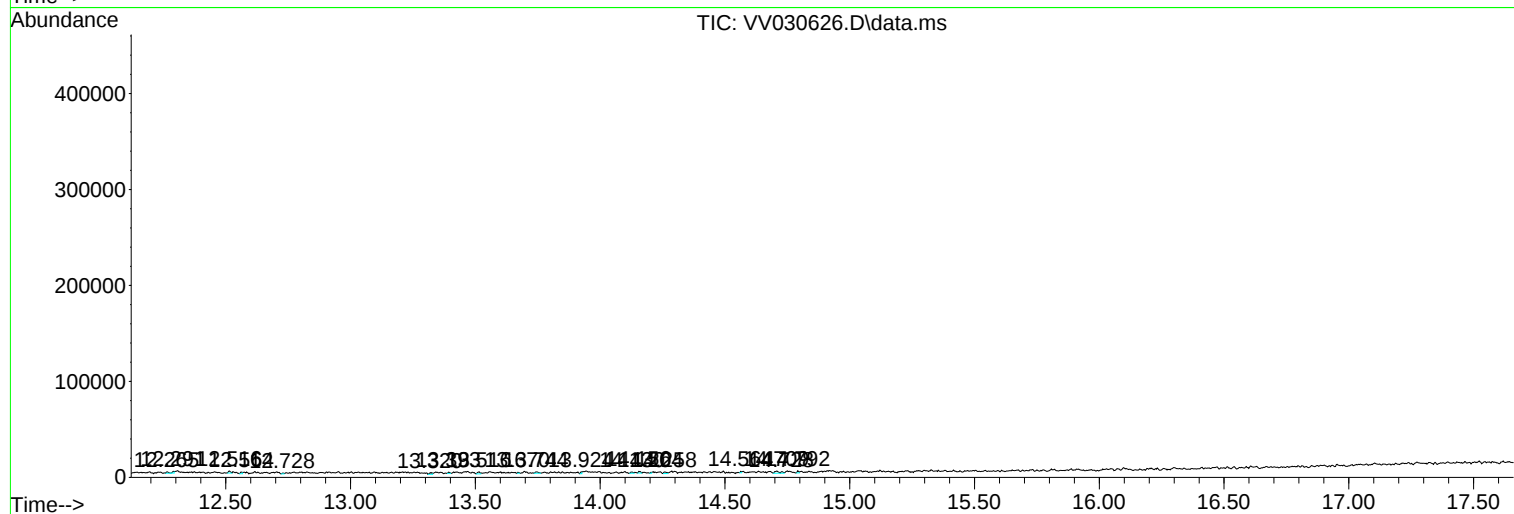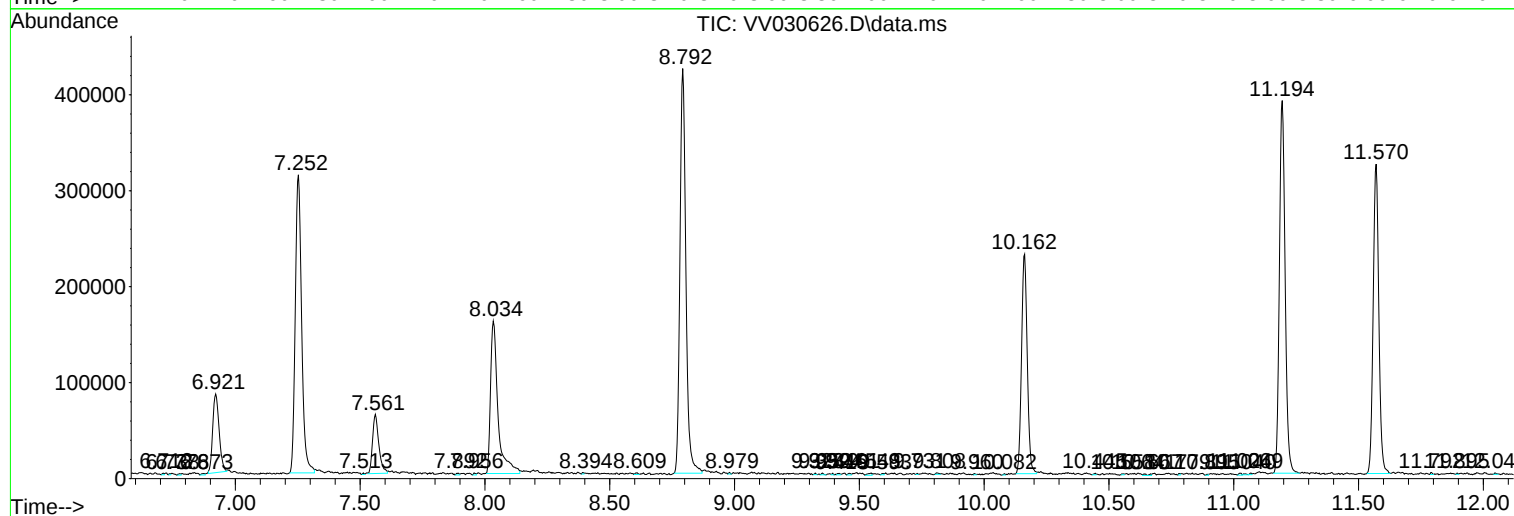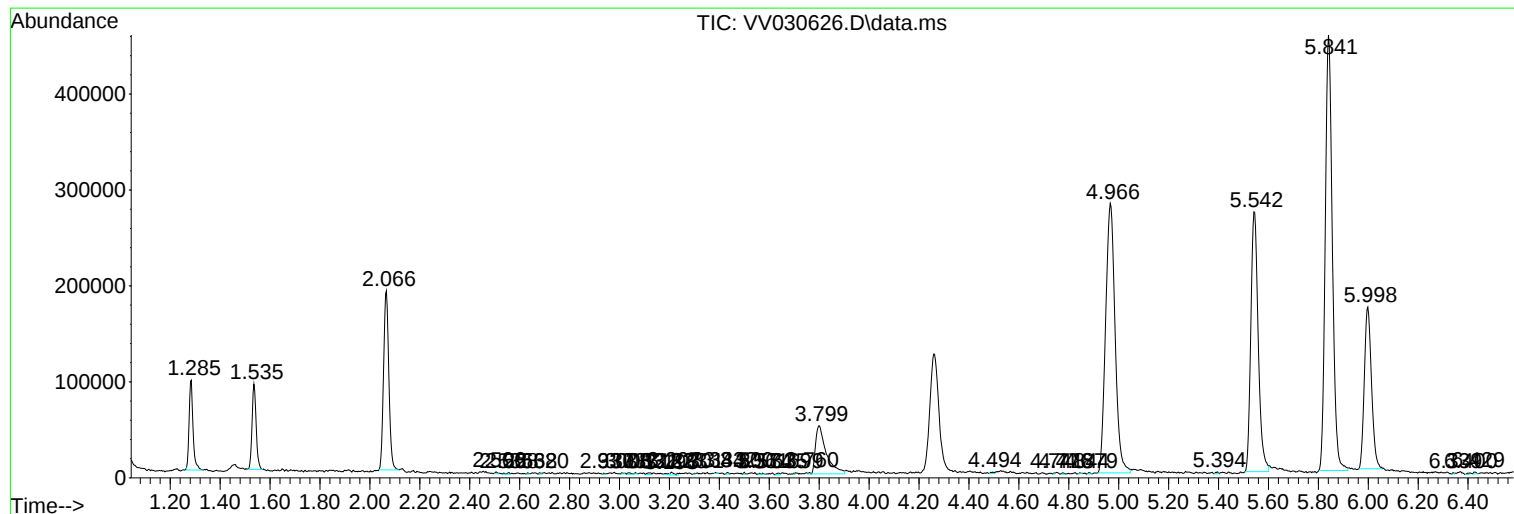

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030626.D
Acq On : 18 Apr 2023 18:40
Operator : SY/MD
Sample : 02360-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030626.D
Acq On : 18 Apr 2023 18:40
Operator : SY/MD
Sample : 02360-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------