

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030627.D
 Acq On : 18 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02360-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	86	rVB	100095	102770	12.65%	1.515%
2	1.535	148	154	165	rVB	90322	105918	13.04%	1.561%
3	2.066	310	319	333	rBV	188655	275723	33.94%	4.064%
4	2.709	513	519	523	rBV7	2302	2204	0.27%	0.032%
5	2.744	529	530	535	rVB4	1906	1003	0.12%	0.015%
6	2.838	557	559	563	rVB5	1711	1231	0.15%	0.018%
7	2.947	590	593	595	rBV4	1627	920	0.11%	0.014%
8	2.969	598	600	601	rBV2	2015	962	0.12%	0.014%
9	3.011	611	613	618	rBV6	1678	1572	0.19%	0.023%
10	3.079	630	634	637	rBV5	1542	1471	0.18%	0.022%
11	3.143	651	654	656	rBV4	1593	992	0.12%	0.015%
12	3.188	664	668	670	rBV5	1449	1223	0.15%	0.018%
13	3.265	690	692	694	rBV4	1432	881	0.11%	0.013%
14	3.281	694	697	700	rVV5	1419	968	0.12%	0.014%
15	3.326	708	711	712	rBV3	1230	769	0.09%	0.011%
16	3.355	716	720	721	rBV4	1936	1173	0.14%	0.017%
17	3.545	777	779	782	rVB4	1976	948	0.12%	0.014%
18	3.571	782	787	788	rBV5	1507	1412	0.17%	0.021%
19	3.651	809	812	818	rBV7	1378	1829	0.23%	0.027%
20	3.706	827	829	833	rVB4	2694	1365	0.17%	0.020%
21	3.731	833	837	838	rBV4	1514	1180	0.15%	0.017%
22	3.799	847	858	884	rBV	51293	144914	17.84%	2.136%
23	4.121	957	958	962	rBV4	1228	1085	0.13%	0.016%
24	4.259	989	1001	1026	rVB	120840	310663	38.24%	4.579%
25	4.645	1117	1121	1126	rVB7	1278	1222	0.15%	0.018%
26	4.712	1138	1142	1144	rBV5	1577	936	0.12%	0.014%
27	4.741	1149	1151	1154	rVB4	1491	616	0.08%	0.009%
28	4.760	1154	1157	1159	rBV4	962	625	0.08%	0.009%
29	4.818	1174	1175	1177	rBV2	1631	789	0.10%	0.012%
30	4.966	1204	1221	1246	rBV2	277501	747667	92.02%	11.021%
31	5.259	1310	1312	1314	rBV3	1620	844	0.10%	0.012%
32	5.384	1349	1351	1353	rBV2	1769	985	0.12%	0.015%
33	5.542	1388	1400	1421	rBV	264780	555646	68.39%	8.190%
34	5.841	1481	1493	1513	rBV2	415171	812479	100.00%	11.976%
35	5.998	1531	1542	1561	rVB	167124	342381	42.14%	5.047%
36	6.625	1734	1737	1739	rBV4	1051	802	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030627.D
 Acq On : 18 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02360-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.709	1761	1763	1766	rBV4	1597	1081	0.13%	0.016%
38	6.773	1780	1783	1788	rVB7	2176	1977	0.24%	0.029%
39	6.799	1788	1791	1793	rBV3	1370	783	0.10%	0.012%
40	6.921	1817	1829	1846	rBV	84643	163977	20.18%	2.417%
41	7.124	1890	1892	1894	rBV3	1889	840	0.10%	0.012%
42	7.191	1911	1913	1916	rBV4	933	673	0.08%	0.010%
43	7.252	1921	1932	1948	rBV	309777	551200	67.84%	8.125%
44	7.561	2019	2028	2047	rBV	60890	111309	13.70%	1.641%
45	7.857	2118	2120	2124	rBV4	1330	710	0.09%	0.010%
46	7.899	2130	2133	2136	rBV5	1512	1269	0.16%	0.019%
47	7.979	2156	2158	2161	rBV4	974	817	0.10%	0.012%
48	8.034	2165	2175	2192	rBV2	160730	305554	37.61%	4.504%
49	8.336	2265	2269	2272	rBV5	1893	1493	0.18%	0.022%
50	8.390	2284	2286	2290	rBV5	1121	1065	0.13%	0.016%
51	8.542	2330	2333	2335	rBV4	1593	1157	0.14%	0.017%
52	8.673	2368	2374	2377	rBV8	1435	1446	0.18%	0.021%
53	8.792	2400	2411	2432	rBV	405932	678703	83.53%	10.004%
54	9.535	2640	2642	2645	rVB4	1329	763	0.09%	0.011%
55	9.554	2645	2648	2650	rBV4	1751	1280	0.16%	0.019%
56	9.641	2669	2675	2679	rBV8	1915	2318	0.29%	0.034%
57	9.857	2739	2742	2743	rBV2	1568	830	0.10%	0.012%
58	10.011	2786	2790	2793	rBV6	1633	1299	0.16%	0.019%
59	10.062	2804	2806	2808	rVV3	1639	621	0.08%	0.009%
60	10.104	2811	2819	2822	rBV10	2217	2945	0.36%	0.043%
61	10.162	2826	2837	2856	rVV	227838	369574	45.49%	5.448%
62	10.513	2943	2946	2950	rVB6	2335	1238	0.15%	0.018%
63	10.574	2961	2965	2966	rBV4	1539	1151	0.14%	0.017%
64	10.644	2983	2987	2991	rVB7	2010	1613	0.20%	0.024%
65	11.021	3101	3104	3108	rBV6	2357	1629	0.20%	0.024%
66	11.107	3128	3131	3133	rVB4	2056	1107	0.14%	0.016%
67	11.194	3147	3158	3177	rVB	378705	603870	74.32%	8.901%
68	11.400	3220	3222	3223	rBV2	1116	610	0.08%	0.009%
69	11.570	3263	3275	3295	rVB	311067	507180	62.42%	7.476%
70	11.641	3295	3297	3299	rBV3	1439	813	0.10%	0.012%
71	11.808	3346	3349	3351	rBV3	1309	773	0.10%	0.011%
72	11.821	3351	3353	3357	rVB5	1201	720	0.09%	0.011%
73	11.844	3357	3360	3362	rBV3	1602	977	0.12%	0.014%
74	12.030	3415	3418	3420	rBV3	1727	1207	0.15%	0.018%
75	12.078	3430	3433	3435	rBV4	1962	1233	0.15%	0.018%
76	12.136	3448	3451	3453	rBV3	1458	738	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030627.D
 Acq On : 18 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02360-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.213	3473	3475	3478	rVV4	1674	984	0.12%	0.015%
78	12.249	3482	3486	3488	rBV4	1324	999	0.12%	0.015%
79	12.461	3547	3552	3553	rBV5	1793	1552	0.19%	0.023%
80	12.532	3572	3574	3577	rBV3	1017	682	0.08%	0.010%
81	12.570	3582	3586	3589	rBV6	1893	1454	0.18%	0.021%
82	12.657	3611	3613	3615	rBV3	1383	812	0.10%	0.012%
83	12.673	3616	3618	3622	rVV5	1848	1223	0.15%	0.018%
84	12.905	3688	3690	3693	rVB3	2079	1105	0.14%	0.016%
85	12.924	3693	3696	3701	rBV6	2128	2481	0.31%	0.037%
86	12.998	3717	3719	3721	rBV3	1322	675	0.08%	0.010%
87	13.033	3728	3730	3733	rBV4	1424	911	0.11%	0.013%
88	13.075	3740	3743	3746	rBV5	1664	1231	0.15%	0.018%
89	13.117	3753	3756	3757	rBV3	1760	1011	0.12%	0.015%
90	13.184	3775	3777	3780	rBV4	1496	713	0.09%	0.011%
91	13.352	3825	3829	3831	rBV4	1273	746	0.09%	0.011%
92	13.824	3973	3976	3978	rBV4	2142	1089	0.13%	0.016%
93	13.837	3978	3980	3982	rBV3	2018	1281	0.16%	0.019%
94	13.869	3988	3990	3993	rBV3	1647	1157	0.14%	0.017%
95	14.319	4128	4130	4131	rBV2	2170	969	0.12%	0.014%
96	14.368	4141	4145	4147	rBV5	2175	1697	0.21%	0.025%
97	14.409	4156	4158	4160	rBV3	1796	905	0.11%	0.013%
98	14.545	4199	4200	4204	rBV4	1418	999	0.12%	0.015%
99	14.869	4297	4301	4304	rBV6	1976	1523	0.19%	0.022%
100	14.950	4323	4326	4328	rBV4	1713	1139	0.14%	0.017%




Sum of corrected areas: 6784049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030627.D
Acq On : 18 Apr 2023 19:04
Operator : SY/MD
Sample : 02360-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

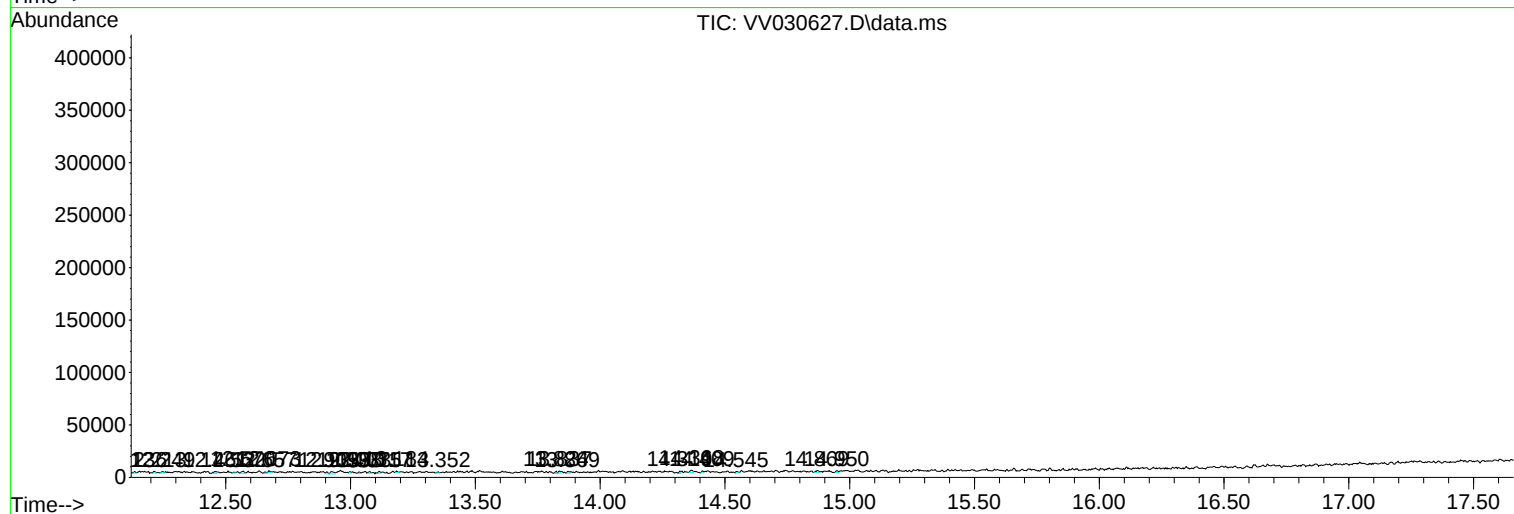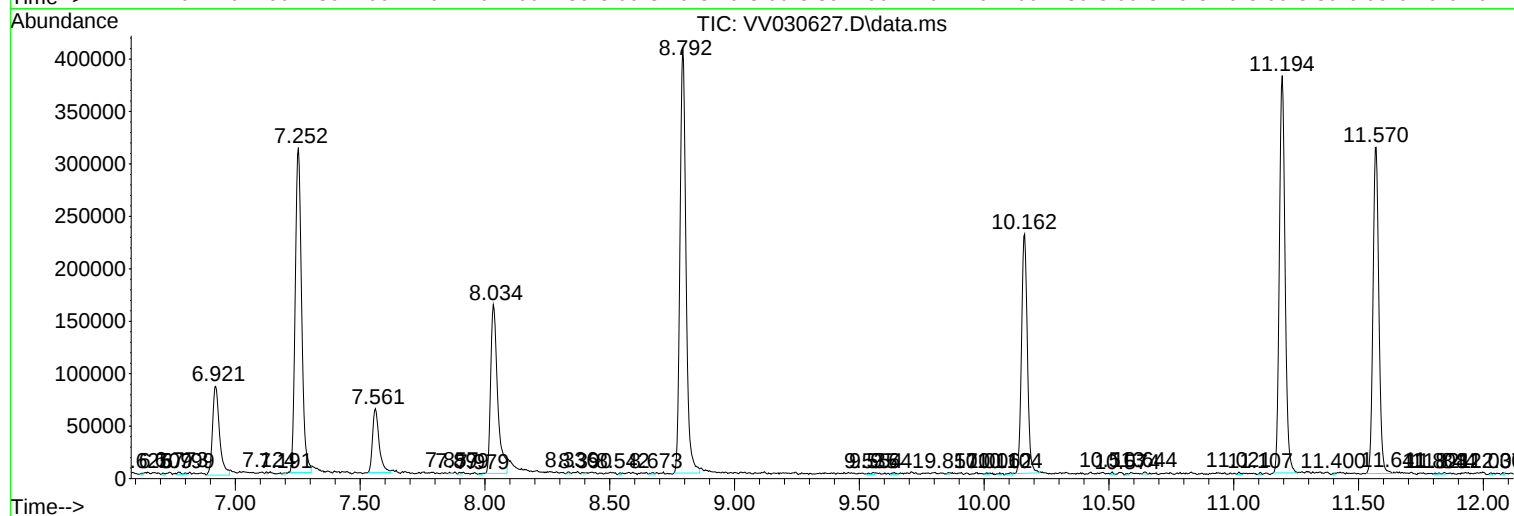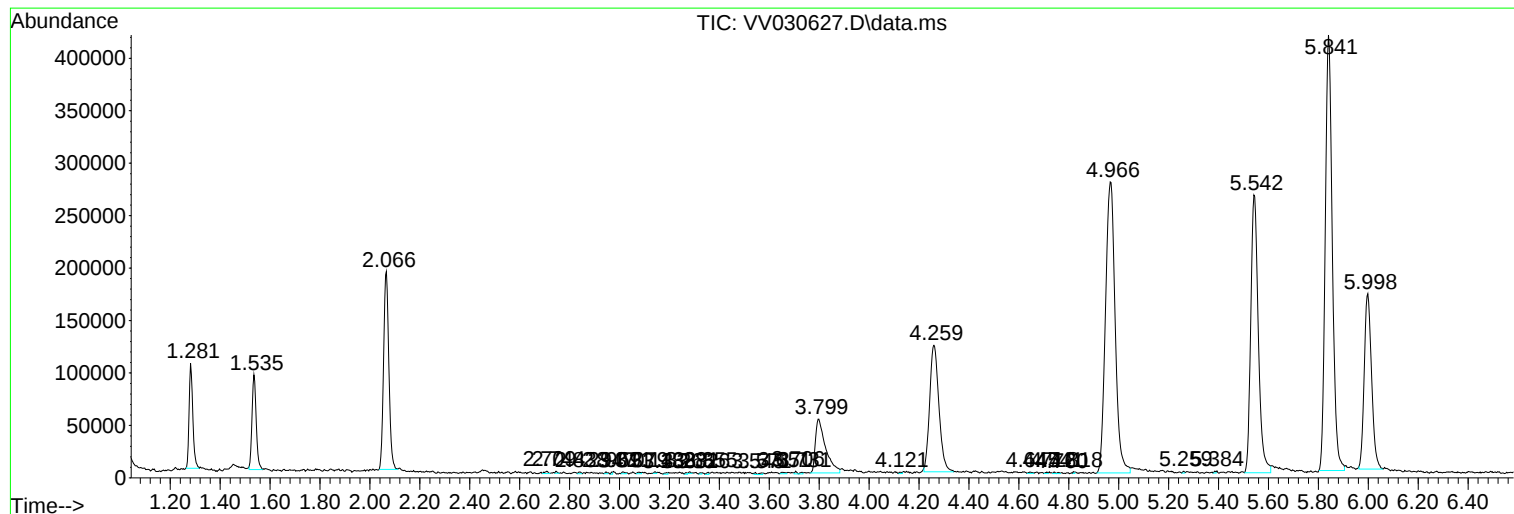

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030627.D
Acq On : 18 Apr 2023 19:04
Operator : SY/MD
Sample : 02360-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030627.D
Acq On : 18 Apr 2023 19:04
Operator : SY/MD
Sample : 02360-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc