

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030628.D
 Acq On : 18 Apr 2023 19:28
 Operator : SY/MD
 Sample : 02360-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	91	rVB	89681	100724	13.78%	1.590%
2	1.535	148	154	165	rVB	88549	102103	13.96%	1.612%
3	2.066	310	319	332	rVB	182160	266472	36.45%	4.207%
4	2.529	457	463	464	rVB5	2553	1793	0.25%	0.028%
5	2.542	464	467	468	rBV3	1641	876	0.12%	0.014%
6	2.571	472	476	480	rBV7	1322	1138	0.16%	0.018%
7	2.841	556	560	561	rBV3	1251	950	0.13%	0.015%
8	3.204	670	673	677	rBV6	1477	917	0.13%	0.014%
9	3.265	689	692	695	rVB5	1701	940	0.13%	0.015%
10	3.403	733	735	738	rBV3	1647	1148	0.16%	0.018%
11	3.487	759	761	764	rBV4	1342	865	0.12%	0.014%
12	3.535	772	776	779	rBV7	1125	862	0.12%	0.014%
13	3.558	779	783	786	rVV5	1071	890	0.12%	0.014%
14	3.670	814	818	819	rBV4	1355	785	0.11%	0.012%
15	3.715	828	832	835	rVB5	1321	846	0.12%	0.013%
16	3.764	843	847	849	rBV4	1132	867	0.12%	0.014%
17	3.799	849	858	880	rBV2	50404	140773	19.25%	2.223%
18	4.111	952	955	960	rBV6	1307	1083	0.15%	0.017%
19	4.262	985	1002	1023	rBV	121566	314181	42.97%	4.961%
20	4.522	1078	1083	1086	rBV7	2551	1965	0.27%	0.031%
21	4.741	1146	1151	1152	rBV5	1571	1252	0.17%	0.020%
22	4.966	1204	1221	1244	rBV2	274759	731138	100.00%	11.544%
23	5.281	1315	1319	1321	rBV5	1785	1602	0.22%	0.025%
24	5.349	1338	1340	1342	rBV3	1433	942	0.13%	0.015%
25	5.436	1365	1367	1369	rBV3	1446	958	0.13%	0.015%
26	5.477	1376	1380	1381	rBV4	1276	897	0.12%	0.014%
27	5.542	1386	1400	1423	rBV	262015	547306	74.86%	8.641%
28	5.841	1482	1493	1514	rBV	207492	413088	56.50%	6.522%
29	5.998	1531	1542	1562	rVB2	165532	340039	46.51%	5.369%
30	6.362	1653	1655	1657	rVV3	1481	847	0.12%	0.013%
31	6.500	1695	1698	1701	rVV5	1818	1017	0.14%	0.016%
32	6.522	1701	1705	1707	rVV4	1216	942	0.13%	0.015%
33	6.645	1741	1743	1748	rVB4	1686	1128	0.15%	0.018%
34	6.770	1780	1782	1787	rVB6	1417	1023	0.14%	0.016%
35	6.796	1787	1790	1792	rVB4	1533	937	0.13%	0.015%
36	6.837	1801	1803	1806	rVB4	1760	898	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030628.D
 Acq On : 18 Apr 2023 19:28
 Operator : SY/MD
 Sample : 02360-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1850	rBV	81354	157146	21.49%	2.481%
38	7.181	1907	1910	1912	rBV4	1644	817	0.11%	0.013%
39	7.252	1921	1932	1957	rBV	308589	547292	74.85%	8.641%
40	7.561	2017	2028	2044	rBV2	61290	110294	15.09%	1.741%
41	7.686	2065	2067	2068	rBV2	1763	793	0.11%	0.013%
42	8.034	2166	2175	2206	rBV	161276	315234	43.12%	4.977%
43	8.612	2350	2355	2358	rVB7	1715	1503	0.21%	0.024%
44	8.751	2394	2398	2399	rBV4	2029	1398	0.19%	0.022%
45	8.792	2400	2411	2430	rVV	407018	670813	91.75%	10.592%
46	9.030	2481	2485	2487	rBV5	1671	1523	0.21%	0.024%
47	9.062	2493	2495	2497	rBV3	1907	1100	0.15%	0.017%
48	9.246	2547	2552	2554	rBV5	1461	1574	0.22%	0.025%
49	9.590	2657	2659	2661	rVB2	1831	790	0.11%	0.012%
50	9.741	2702	2706	2709	rBV6	1720	1541	0.21%	0.024%
51	9.889	2750	2752	2754	rBV3	1369	769	0.11%	0.012%
52	10.066	2805	2807	2809	rBV3	1301	811	0.11%	0.013%
53	10.162	2826	2837	2852	rVV	228230	368069	50.34%	5.811%
54	10.255	2863	2866	2868	rVB4	1899	811	0.11%	0.013%
55	10.310	2879	2883	2884	rBV3	1567	1029	0.14%	0.016%
56	10.426	2917	2919	2921	rBV3	1397	953	0.13%	0.015%
57	10.657	2989	2991	3000	rVB9	1279	1461	0.20%	0.023%
58	10.722	3008	3011	3013	rBV4	1734	775	0.11%	0.012%
59	10.763	3021	3024	3027	rBV4	1606	1256	0.17%	0.020%
60	10.914	3067	3071	3074	rBV6	1613	1538	0.21%	0.024%
61	10.982	3090	3092	3096	rVB5	1293	860	0.12%	0.014%
62	11.024	3103	3105	3107	rVB3	1872	844	0.12%	0.013%
63	11.136	3137	3140	3143	rVB4	1400	951	0.13%	0.015%
64	11.194	3147	3158	3176	rVV	375031	604710	82.71%	9.548%
65	11.484	3246	3248	3252	rVB4	3278	2650	0.36%	0.042%
66	11.570	3263	3275	3290	rBV	315145	505770	69.18%	7.986%
67	11.651	3298	3300	3303	rBV4	1747	959	0.13%	0.015%
68	11.747	3327	3330	3334	rVB6	2559	1609	0.22%	0.025%
69	11.763	3334	3335	3337	rBV2	1698	791	0.11%	0.012%
70	11.857	3361	3364	3366	rBV3	1569	1103	0.15%	0.017%
71	11.921	3379	3384	3388	rBV8	1427	1191	0.16%	0.019%
72	12.053	3422	3425	3427	rBV3	1913	1235	0.17%	0.019%
73	12.120	3443	3446	3448	rBV4	1777	991	0.14%	0.016%
74	12.181	3464	3465	3470	rBV5	1311	1040	0.14%	0.016%
75	12.271	3491	3493	3497	rVB4	1847	1015	0.14%	0.016%
76	12.342	3514	3515	3518	rBV2	1507	825	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030628.D
 Acq On : 18 Apr 2023 19:28
 Operator : SY/MD
 Sample : 02360-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.496	3558	3563	3569	rVB10	1672	2004	0.27%	0.032%
78	12.570	3583	3586	3589	rVB5	1951	1245	0.17%	0.020%
79	12.657	3607	3613	3616	rVB7	1847	1925	0.26%	0.030%
80	12.680	3616	3620	3623	rBV7	1831	1824	0.25%	0.029%
81	12.779	3644	3651	3658	rVB7	2135	2968	0.41%	0.047%
82	12.808	3658	3660	3663	rBV4	1318	894	0.12%	0.014%
83	12.876	3677	3681	3683	rBV5	1665	1290	0.18%	0.020%
84	12.927	3695	3697	3701	rVB5	1626	1040	0.14%	0.016%
85	13.085	3744	3746	3749	rBV4	1511	880	0.12%	0.014%
86	13.120	3755	3757	3760	rVB4	2100	1027	0.14%	0.016%
87	13.139	3760	3763	3768	rVB6	1630	1215	0.17%	0.019%
88	13.191	3776	3779	3781	rBV3	1950	1482	0.20%	0.023%
89	13.242	3792	3795	3801	rBV7	1797	1464	0.20%	0.023%
90	13.271	3801	3804	3806	rBV4	1804	1076	0.15%	0.017%
91	13.631	3913	3916	3919	rBV3	1727	1065	0.15%	0.017%
92	13.766	3955	3958	3961	rBV4	1097	898	0.12%	0.014%
93	13.818	3971	3974	3975	rBV3	1564	1009	0.14%	0.016%
94	14.056	4045	4048	4053	rVB7	1997	1291	0.18%	0.020%
95	14.233	4100	4103	4106	rBV4	1846	1461	0.20%	0.023%
96	14.284	4116	4119	4122	rBV5	1921	1451	0.20%	0.023%
97	14.432	4163	4165	4171	rVB6	2272	2227	0.30%	0.035%
98	14.876	4299	4303	4307	rVB7	1290	1232	0.17%	0.019%
99	14.901	4307	4311	4312	rBV4	2185	1259	0.17%	0.020%
100	15.406	4465	4468	4470	rBV3	2131	1222	0.17%	0.019%




Sum of corrected areas: 6333475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030628.D
Acq On : 18 Apr 2023 19:28
Operator : SY/MD
Sample : 02360-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

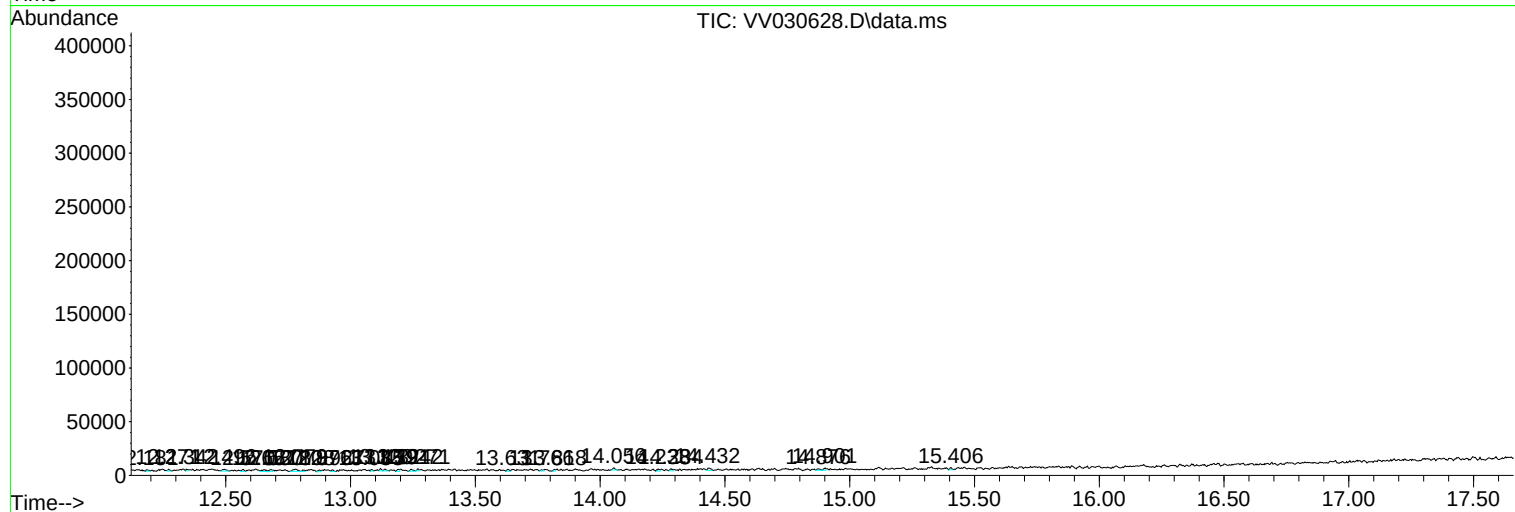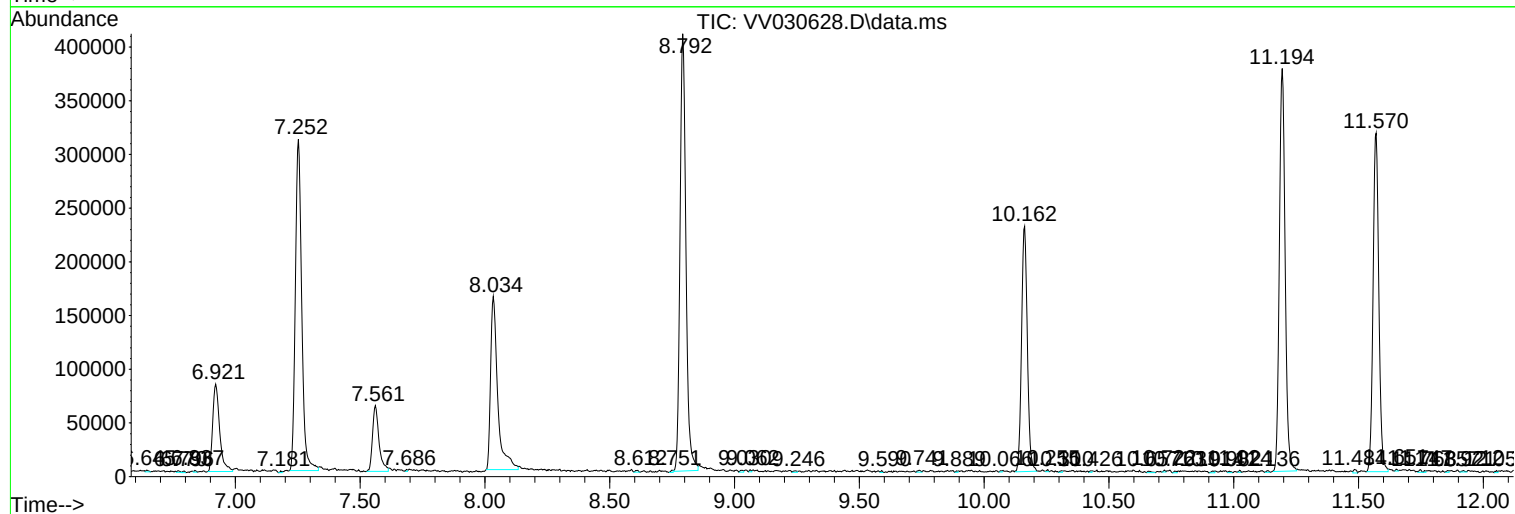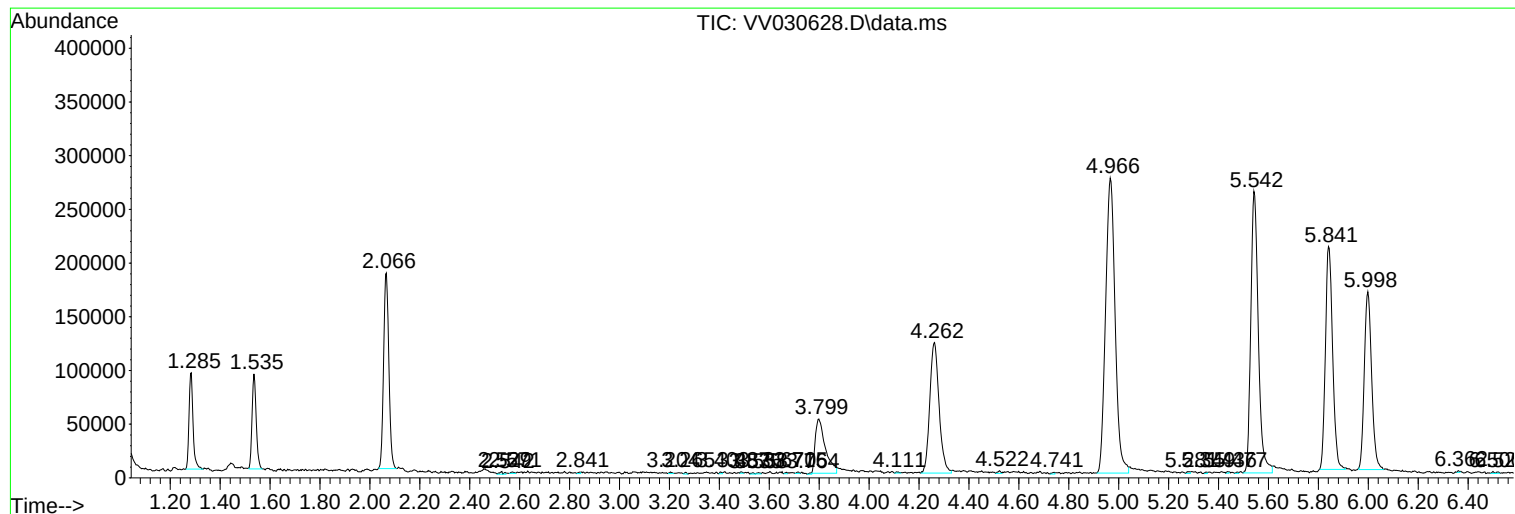

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030628.D
Acq On : 18 Apr 2023 19:28
Operator : SY/MD
Sample : 02360-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030628.D
Acq On : 18 Apr 2023 19:28
Operator : SY/MD
Sample : 02360-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------