

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030630.D
 Acq On : 18 Apr 2023 20:16
 Operator : SY/MD
 Sample : 02360-01DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	86	rBV	98653	108235	13.63%	1.606%
2	1.535	148	154	166	rVB	91801	112444	14.16%	1.668%
3	2.066	309	319	334	rBV	196087	288864	36.38%	4.286%
4	2.362	406	411	414	rBV6	1689	1257	0.16%	0.019%
5	2.677	506	509	512	rVB5	1185	857	0.11%	0.013%
6	2.715	518	521	525	rBV5	2325	1525	0.19%	0.023%
7	2.828	553	556	557	rBV3	1296	703	0.09%	0.010%
8	3.047	620	624	628	rBV7	1214	1115	0.14%	0.017%
9	3.175	660	664	668	rBV7	1486	1472	0.19%	0.022%
10	3.262	687	691	694	rBV7	2141	1494	0.19%	0.022%
11	3.375	722	726	730	rBV6	1711	1645	0.21%	0.024%
12	3.400	730	734	736	rBV4	1629	1264	0.16%	0.019%
13	3.439	744	746	749	rVV4	1475	847	0.11%	0.013%
14	3.539	774	777	779	rBV4	1843	1125	0.14%	0.017%
15	3.696	824	826	828	rBV3	2256	1225	0.15%	0.018%
16	3.799	848	858	883	rBV	52597	147732	18.61%	2.192%
17	4.156	964	969	973	rBV8	2000	1709	0.22%	0.025%
18	4.262	989	1002	1022	rVB	129178	327625	41.26%	4.861%
19	4.674	1128	1130	1132	rVB3	1925	905	0.11%	0.013%
20	4.966	1203	1221	1246	rBV3	299625	794030	100.00%	11.782%
21	5.436	1365	1367	1370	rVB3	1979	796	0.10%	0.012%
22	5.542	1388	1400	1422	rBV	269422	559183	70.42%	8.297%
23	5.841	1480	1493	1515	rBV2	235076	458133	57.70%	6.798%
24	5.998	1530	1542	1563	rVB2	176318	362331	45.63%	5.376%
25	6.342	1645	1649	1651	rBV5	1362	954	0.12%	0.014%
26	6.490	1693	1695	1697	rBV3	1377	828	0.10%	0.012%
27	6.600	1726	1729	1736	rBV7	2029	2522	0.32%	0.037%
28	6.706	1760	1762	1766	rVB3	1249	761	0.10%	0.011%
29	6.757	1776	1778	1784	rVB7	1380	927	0.12%	0.014%
30	6.921	1818	1829	1843	rBV	90345	171680	21.62%	2.547%
31	7.120	1887	1891	1895	rVV6	1668	1780	0.22%	0.026%
32	7.252	1920	1932	1955	rBV	332464	594358	74.85%	8.819%
33	7.561	2019	2028	2048	rBV	64716	120257	15.15%	1.784%
34	7.696	2067	2070	2072	rBV4	1310	797	0.10%	0.012%
35	7.773	2092	2094	2099	rVB6	2782	1927	0.24%	0.029%
36	8.034	2166	2175	2203	rVV	171881	342334	43.11%	5.080%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030630.D
 Acq On : 18 Apr 2023 20:16
 Operator : SY/MD
 Sample : 02360-01DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.352	2271	2274	2276	rBV4	1272	813	0.10%	0.012%
38	8.410	2289	2292	2294	rBV4	1519	1046	0.13%	0.016%
39	8.680	2373	2376	2377	rBV3	1460	747	0.09%	0.011%
40	8.792	2398	2411	2433	rBV	421814	700818	88.26%	10.399%
41	9.233	2545	2548	2549	rBV3	1604	942	0.12%	0.014%
42	9.381	2593	2594	2598	rBV3	1241	774	0.10%	0.011%
43	9.686	2685	2689	2690	rBV4	1594	1097	0.14%	0.016%
44	9.747	2705	2708	2711	rBV4	1314	974	0.12%	0.014%
45	9.776	2715	2717	2722	rVB5	1709	1260	0.16%	0.019%
46	9.805	2722	2726	2727	rBV4	1320	865	0.11%	0.013%
47	9.889	2747	2752	2755	rBV6	1512	1262	0.16%	0.019%
48	9.956	2769	2773	2774	rBV3	1602	923	0.12%	0.014%
49	10.059	2802	2805	2807	rBV4	1835	1159	0.15%	0.017%
50	10.162	2822	2837	2854	rBV	241598	392239	49.40%	5.820%
51	10.262	2865	2868	2869	rBV2	1541	897	0.11%	0.013%
52	10.310	2881	2883	2887	rBV4	2283	1847	0.23%	0.027%
53	10.423	2914	2918	2919	rBV4	1877	1207	0.15%	0.018%
54	10.535	2950	2953	2954	rBV2	2247	1115	0.14%	0.017%
55	10.632	2979	2983	2985	rBV5	1911	1442	0.18%	0.021%
56	10.731	3012	3014	3016	rBV2	1248	721	0.09%	0.011%
57	10.844	3047	3049	3052	rVV3	1449	849	0.11%	0.013%
58	10.863	3052	3055	3056	rVV3	1670	939	0.12%	0.014%
59	10.889	3060	3063	3064	rVV3	1650	869	0.11%	0.013%
60	10.915	3068	3071	3074	rVV4	1596	920	0.12%	0.014%
61	10.937	3076	3078	3081	rVB4	2020	1017	0.13%	0.015%
62	10.960	3081	3085	3088	rBV6	1824	1666	0.21%	0.025%
63	11.072	3116	3120	3123	rBV5	1761	1330	0.17%	0.020%
64	11.194	3146	3158	3176	rBV	389783	625950	78.83%	9.288%
65	11.371	3208	3213	3216	rVB6	1747	1649	0.21%	0.024%
66	11.570	3264	3275	3296	rVB	332083	535695	67.47%	7.949%
67	11.779	3337	3340	3342	rBV4	1459	935	0.12%	0.014%
68	11.795	3343	3345	3349	rVB5	1842	1377	0.17%	0.020%
69	11.818	3349	3352	3356	rBV6	1723	1276	0.16%	0.019%
70	11.921	3381	3384	3388	rBV6	1433	1229	0.15%	0.018%
71	12.004	3405	3410	3412	rBV6	2158	1688	0.21%	0.025%
72	12.046	3420	3423	3424	rBV3	1926	1087	0.14%	0.016%
73	12.313	3502	3506	3508	rBV4	1537	1117	0.14%	0.017%
74	12.368	3520	3523	3525	rBV4	1348	927	0.12%	0.014%
75	12.455	3547	3550	3555	rVB6	1387	1219	0.15%	0.018%
76	12.480	3555	3558	3560	rBV4	1946	1479	0.19%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030630.D
 Acq On : 18 Apr 2023 20:16
 Operator : SY/MD
 Sample : 02360-01DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.635	3604	3606	3609	rVB4	1620	850	0.11%	0.013%
78	12.696	3623	3625	3629	rVB4	1487	796	0.10%	0.012%
79	12.760	3641	3645	3648	rBV5	1610	1184	0.15%	0.018%
80	12.969	3706	3710	3712	rBV4	1956	1459	0.18%	0.022%
81	13.004	3718	3721	3722	rBV3	1519	796	0.10%	0.012%
82	13.033	3727	3730	3732	rVB4	1439	750	0.09%	0.011%
83	13.053	3732	3736	3738	rBV4	2000	1325	0.17%	0.020%
84	13.104	3749	3752	3754	rBV4	1477	728	0.09%	0.011%
85	13.287	3806	3809	3814	rVB6	2417	1689	0.21%	0.025%
86	13.316	3814	3818	3819	rBV4	1328	865	0.11%	0.013%
87	13.358	3829	3831	3837	rVB7	1486	1258	0.16%	0.019%
88	13.384	3837	3839	3841	rBV3	1220	720	0.09%	0.011%
89	13.551	3887	3891	3894	rVV5	1604	1398	0.18%	0.021%
90	13.799	3964	3968	3972	rBV6	1302	1446	0.18%	0.021%
91	13.873	3990	3991	3995	rVB4	1993	951	0.12%	0.014%
92	13.895	3995	3998	4000	rBV4	2684	1868	0.24%	0.028%
93	14.033	4038	4041	4044	rBV4	1364	1034	0.13%	0.015%
94	14.049	4044	4046	4051	rBV6	1368	1050	0.13%	0.016%
95	14.252	4103	4109	4110	rBV5	1508	1345	0.17%	0.020%
96	14.300	4122	4124	4128	rBV4	1819	1286	0.16%	0.019%
97	14.397	4151	4154	4161	rBV9	2023	1959	0.25%	0.029%
98	14.474	4175	4178	4180	rBV5	2136	1520	0.19%	0.023%
99	14.927	4317	4319	4321	rBV4	1619	723	0.09%	0.011%
100	15.133	4379	4383	4384	rBV4	1953	1231	0.16%	0.018%




Sum of corrected areas: 6739238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030630.D
Acq On : 18 Apr 2023 20:16
Operator : SY/MD
Sample : 02360-01DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

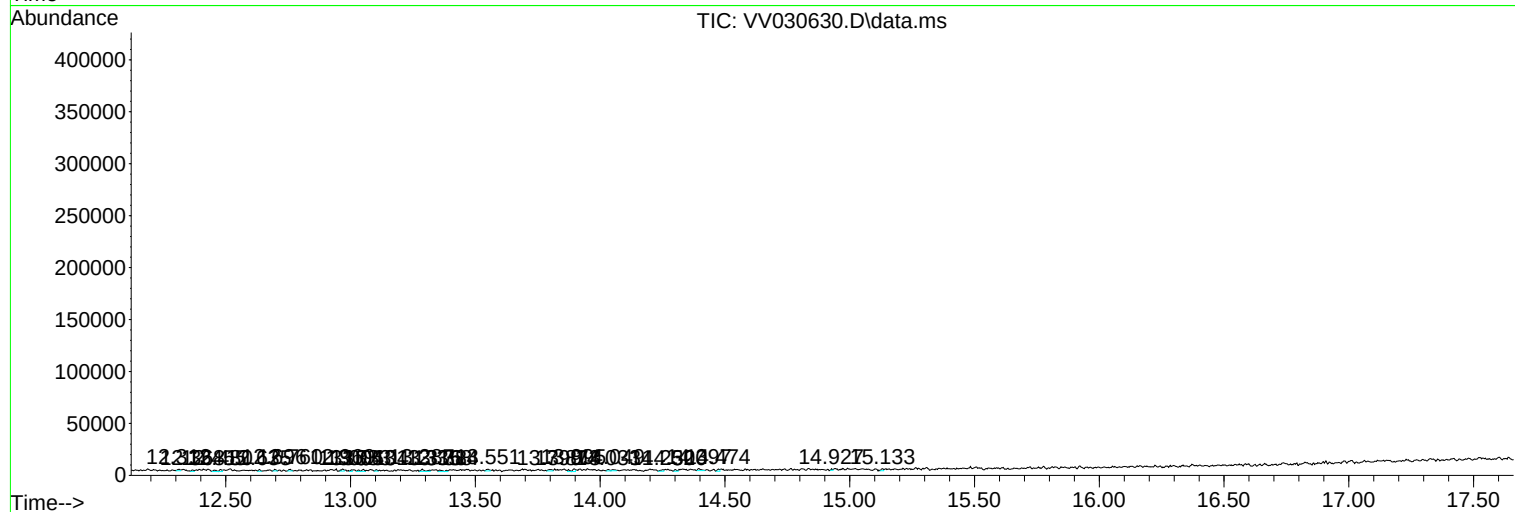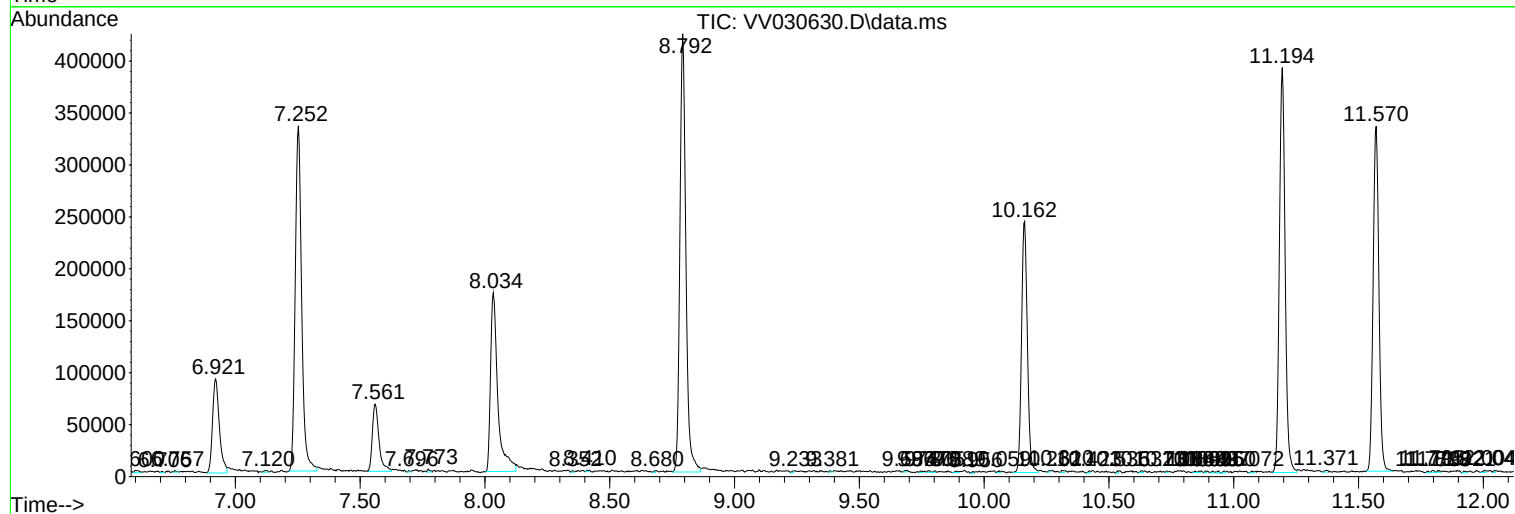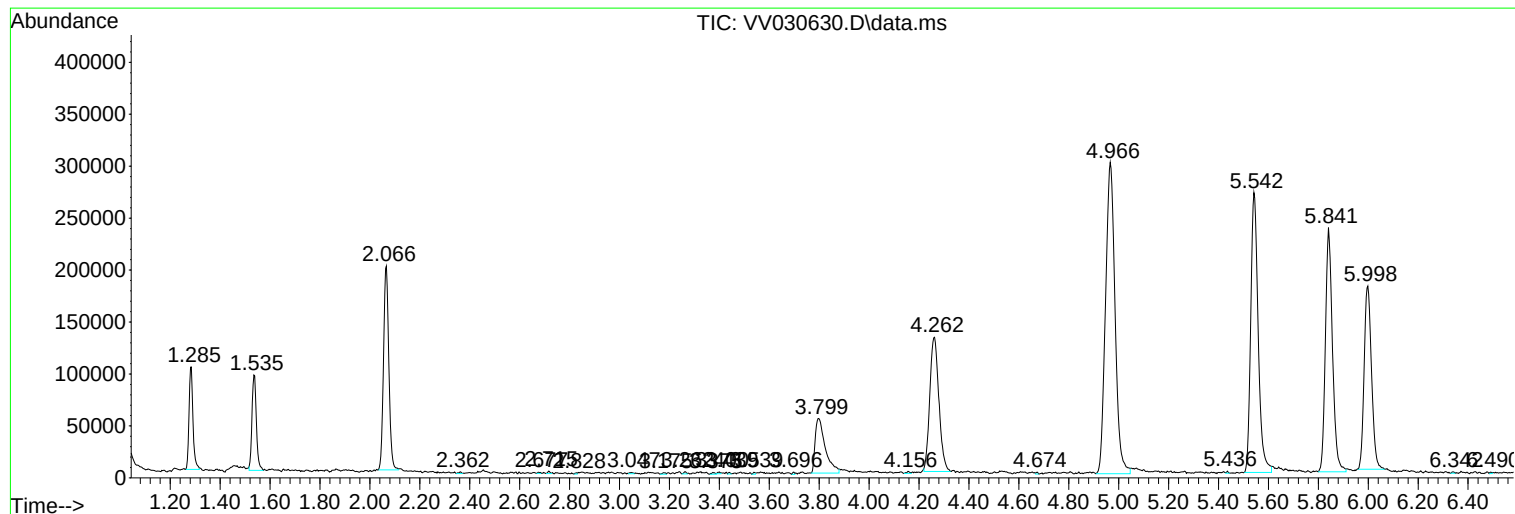

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030630.D
Acq On : 18 Apr 2023 20:16
Operator : SY/MD
Sample : 02360-01DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030630.D
Acq On : 18 Apr 2023 20:16
Operator : SY/MD
Sample : 02360-01DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------