

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030632.D
 Acq On : 18 Apr 2023 21:04
 Operator : SY/MD
 Sample : 02334-01 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	88	rVB	89396	97963	13.57%	1.664%
2	1.536	148	154	169	rVB	83339	105530	14.62%	1.792%
3	2.066	310	319	333	rBV	182534	262983	36.43%	4.466%
4	2.365	407	412	417	rBV8	2497	2656	0.37%	0.045%
5	2.581	474	479	481	rBV6	1651	1503	0.21%	0.026%
6	2.764	534	536	538	rBV2	1278	661	0.09%	0.011%
7	2.825	554	555	557	rBV2	1198	474	0.07%	0.008%
8	2.892	574	576	579	rVB4	1537	772	0.11%	0.013%
9	2.995	605	608	611	rBV4	2020	1375	0.19%	0.023%
10	3.134	646	651	652	rBV4	933	802	0.11%	0.014%
11	3.191	666	669	671	rBV4	1909	1406	0.19%	0.024%
12	3.269	690	693	696	rBV4	1365	1050	0.15%	0.018%
13	3.330	707	712	714	rBV4	2340	1516	0.21%	0.026%
14	3.516	768	770	771	rBV3	715	265	0.04%	0.005%
15	3.558	780	783	784	rBV3	1068	649	0.09%	0.011%
16	3.693	822	825	826	rBV3	1793	941	0.13%	0.016%
17	3.799	848	858	875	rBV	49281	131759	18.25%	2.237%
18	4.130	958	961	963	rBV3	2690	1644	0.23%	0.028%
19	4.262	991	1002	1021	rVB2	117953	293825	40.70%	4.990%
20	4.558	1092	1094	1096	rBV3	1420	700	0.10%	0.012%
21	4.580	1099	1101	1102	rBV	1369	492	0.07%	0.008%
22	4.712	1140	1142	1143	rBV2	1166	423	0.06%	0.007%
23	4.761	1154	1157	1158	rBV3	1851	956	0.13%	0.016%
24	4.844	1180	1183	1185	rBV4	1487	888	0.12%	0.015%
25	4.886	1192	1196	1199	rBV5	1659	1111	0.15%	0.019%
26	4.966	1206	1221	1248	rBV2	269313	721926	100.00%	12.260%
27	5.542	1386	1400	1423	rBV	273633	571679	79.19%	9.708%
28	5.998	1529	1542	1561	rBV	166810	344756	47.76%	5.855%
29	6.230	1611	1614	1618	rBV5	1867	1420	0.20%	0.024%
30	6.696	1756	1759	1760	rBV3	1671	845	0.12%	0.014%
31	6.783	1783	1786	1789	rBV4	1338	1153	0.16%	0.020%
32	6.841	1802	1804	1807	rVB3	1509	865	0.12%	0.015%
33	6.863	1807	1811	1813	rBV5	1702	1171	0.16%	0.020%
34	6.921	1818	1829	1847	rBV	81967	154161	21.35%	2.618%
35	7.153	1899	1901	1902	rBV2	1722	753	0.10%	0.013%
36	7.162	1902	1904	1908	rVV5	1745	1053	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030632.D
 Acq On : 18 Apr 2023 21:04
 Operator : SY/MD
 Sample : 02334-01 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1918	1932	1951	rBV	309533	551940	76.45%	9.373%
38	7.522	2013	2016	2018	rBV5	2058	1400	0.19%	0.024%
39	7.561	2018	2028	2046	rVV2	60338	113834	15.77%	1.933%
40	7.757	2087	2089	2090	rBV2	1279	385	0.05%	0.007%
41	7.854	2118	2119	2122	rBV3	1397	819	0.11%	0.014%
42	7.947	2145	2148	2149	rBV2	1202	626	0.09%	0.011%
43	7.989	2159	2161	2162	rBV2	1533	737	0.10%	0.013%
44	8.034	2166	2175	2192	rBV	159213	298775	41.39%	5.074%
45	8.641	2362	2364	2365	rBV2	1409	471	0.07%	0.008%
46	8.702	2380	2383	2386	rBV5	2135	1355	0.19%	0.023%
47	8.793	2400	2411	2428	rBV	415669	688714	95.40%	11.696%
48	9.185	2530	2533	2534	rBV3	1319	729	0.10%	0.012%
49	9.217	2540	2543	2546	rBV5	1950	1611	0.22%	0.027%
50	9.706	2693	2695	2696	rBV2	840	279	0.04%	0.005%
51	9.738	2703	2705	2707	rBV3	1433	664	0.09%	0.011%
52	9.992	2783	2784	2786	rBV2	1031	509	0.07%	0.009%
53	10.021	2790	2793	2796	rBV5	1235	951	0.13%	0.016%
54	10.159	2827	2836	2850	rBV	234097	359174	49.75%	6.099%
55	10.246	2861	2863	2868	rBV5	1583	925	0.13%	0.016%
56	10.410	2912	2914	2915	rBV2	1083	570	0.08%	0.010%
57	10.503	2941	2943	2945	rBV3	1417	715	0.10%	0.012%
58	10.600	2970	2973	2975	rBV4	1522	931	0.13%	0.016%
59	10.680	2996	2998	3000	rBV4	1033	390	0.05%	0.007%
60	10.757	3020	3022	3023	rBV2	1168	556	0.08%	0.009%
61	11.130	3136	3138	3141	rBV5	1536	1015	0.14%	0.017%
62	11.194	3147	3158	3174	rBV	391382	625280	86.61%	10.618%
63	11.571	3264	3275	3289	rBV	312000	497938	68.97%	8.456%
64	11.725	3321	3323	3324	rBV	1739	817	0.11%	0.014%
65	11.796	3343	3345	3347	rBV2	1287	588	0.08%	0.010%
66	11.853	3362	3363	3368	rBV5	1116	1011	0.14%	0.017%
67	11.921	3382	3384	3386	rBV3	1584	875	0.12%	0.015%
68	12.056	3424	3426	3427	rBV2	958	323	0.04%	0.005%
69	12.185	3462	3466	3467	rBV4	1858	1480	0.21%	0.025%
70	12.744	3638	3640	3641	rBV2	1282	671	0.09%	0.011%
71	12.776	3647	3650	3652	rVB4	2438	1332	0.18%	0.023%
72	12.799	3652	3657	3661	rBV7	1768	2221	0.31%	0.038%
73	12.841	3665	3670	3672	rBV6	2233	2264	0.31%	0.038%
74	12.882	3681	3683	3685	rBV3	1262	648	0.09%	0.011%
75	12.918	3693	3694	3696	rBV2	1408	401	0.06%	0.007%
76	12.982	3712	3714	3715	rBV2	911	302	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030632.D
 Acq On : 18 Apr 2023 21:04
 Operator : SY/MD
 Sample : 02334-01 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

77	13.069	3738	3741	3744	rBV5	1316	894	0.12%	0.015%
78	13.204	3781	3783	3786	rBV4	1341	771	0.11%	0.013%
79	13.316	3815	3818	3822	rBV4	2462	1847	0.26%	0.031%
80	13.394	3839	3842	3843	rBV3	1437	791	0.11%	0.013%
81	13.429	3850	3853	3857	rVB5	2008	1314	0.18%	0.022%
82	13.628	3911	3915	3920	rBV7	1928	2239	0.31%	0.038%
83	13.779	3959	3962	3963	rBV3	1208	494	0.07%	0.008%
84	13.808	3967	3971	3973	rBV5	1409	1126	0.16%	0.019%
85	14.046	4043	4045	4048	rBV4	1239	743	0.10%	0.013%
86	14.387	4150	4151	4152	rBV	1127	430	0.06%	0.007%
87	14.583	4209	4212	4213	rBV3	1288	813	0.11%	0.014%
88	14.869	4299	4301	4303	rBV3	1610	877	0.12%	0.015%




Sum of corrected areas: 5888691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030632.D
Acq On : 18 Apr 2023 21:04
Operator : SY/MD
Sample : 02334-01 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

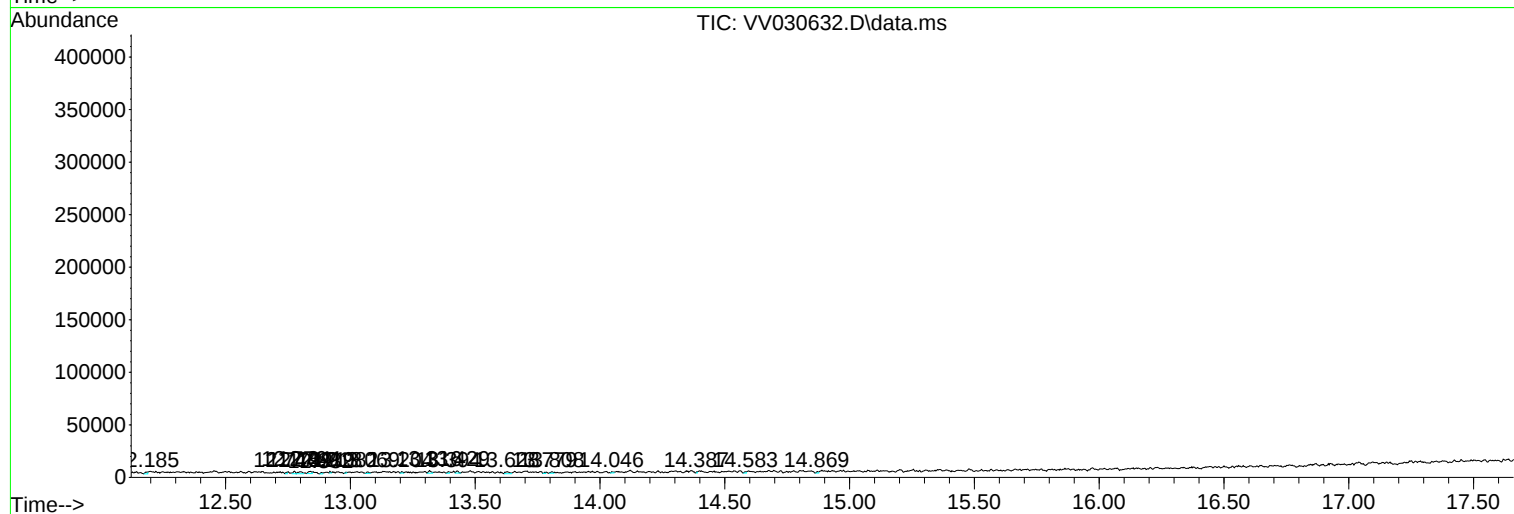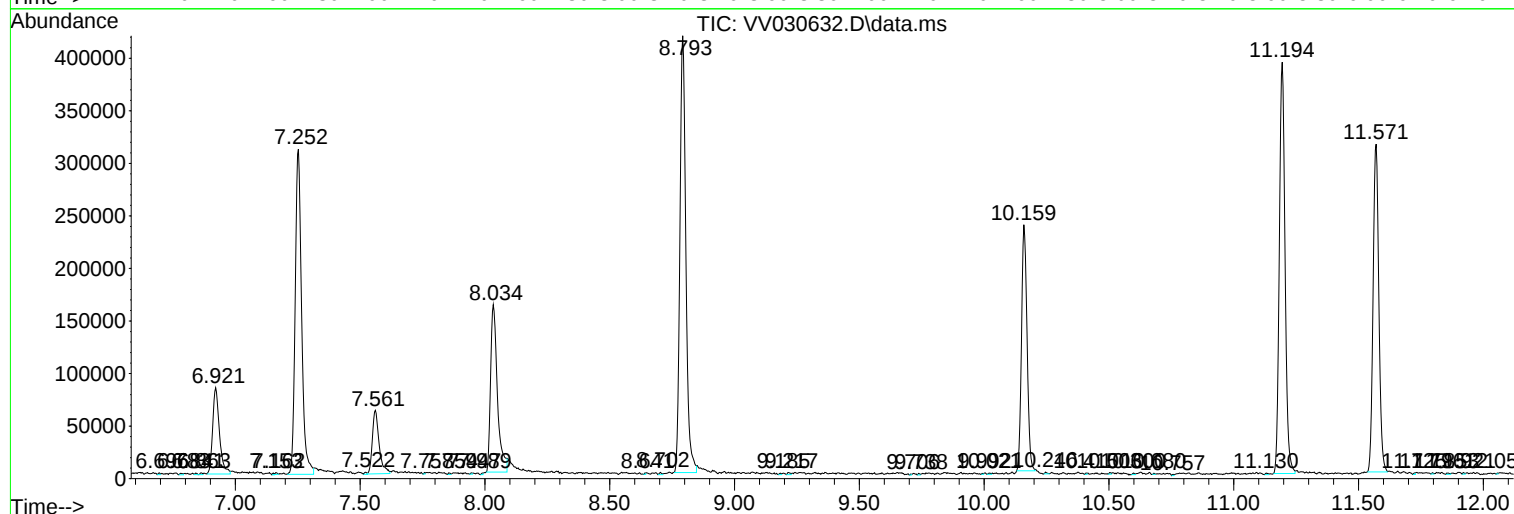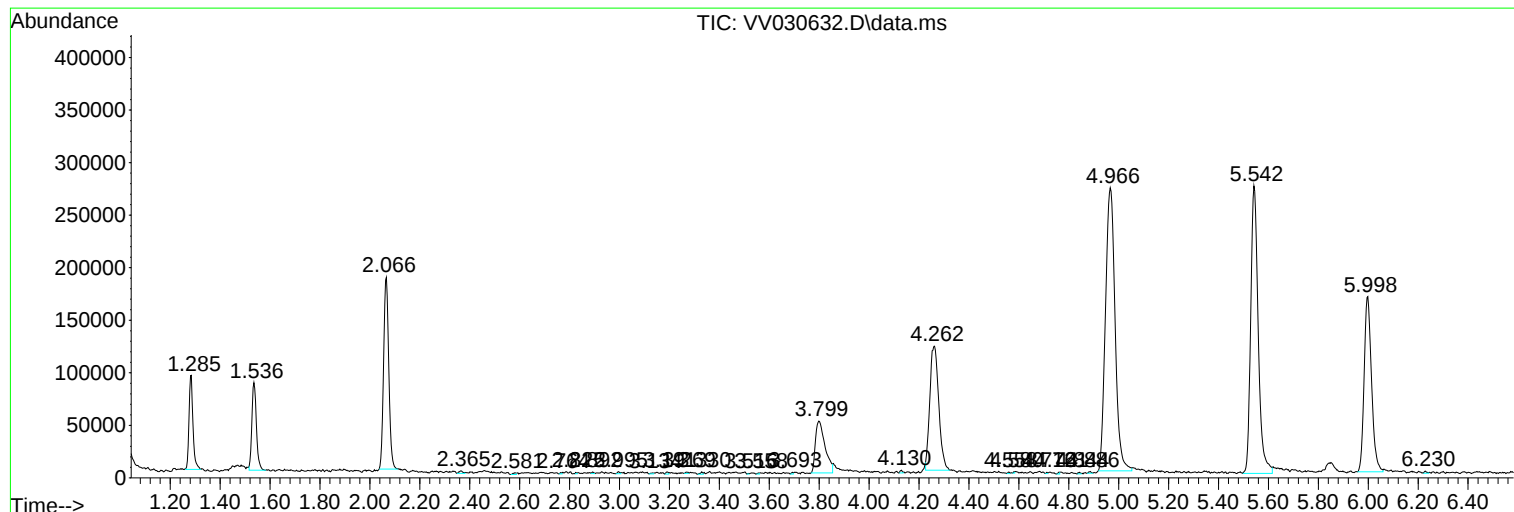

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030632.D
Acq On : 18 Apr 2023 21:04
Operator : SY/MD
Sample : 02334-01 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030632.D
Acq On : 18 Apr 2023 21:04
Operator : SY/MD
Sample : 02334-01 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------