

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030633.D
 Acq On : 18 Apr 2023 21:28
 Operator : SY/MD
 Sample : 02334-03 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	90	rVB	89769	100858	13.66%	1.713%
2	1.536	148	154	167	rVB	87476	101277	13.72%	1.720%
3	2.066	310	319	332	rBV	185399	268939	36.43%	4.567%
4	2.545	465	468	470	rBV4	2181	1681	0.23%	0.029%
5	2.671	505	507	509	rBV3	1134	423	0.06%	0.007%
6	2.889	573	575	577	rBV3	1266	648	0.09%	0.011%
7	2.986	603	605	606	rBV	832	305	0.04%	0.005%
8	3.050	623	625	626	rBV2	844	340	0.05%	0.006%
9	3.134	649	651	653	rBV3	1184	546	0.07%	0.009%
10	3.275	692	695	698	rVB4	1617	990	0.13%	0.017%
11	3.359	714	721	725	rBV9	2205	2722	0.37%	0.046%
12	3.535	774	776	778	rBV3	1236	457	0.06%	0.008%
13	3.799	849	858	877	rBV2	48880	132528	17.95%	2.251%
14	4.085	944	947	949	rBV5	2190	1403	0.19%	0.024%
15	4.259	989	1001	1024	rVB	121174	301037	40.77%	5.112%
16	4.548	1087	1091	1092	rBV4	1236	670	0.09%	0.011%
17	4.616	1110	1112	1114	rBV3	2323	1040	0.14%	0.018%
18	4.799	1167	1169	1172	rBV4	1385	617	0.08%	0.010%
19	4.966	1203	1221	1244	rBV2	278329	738318	100.00%	12.538%
20	5.429	1363	1365	1367	rBV3	1621	950	0.13%	0.016%
21	5.542	1388	1400	1419	rBV	268589	556066	75.32%	9.443%
22	5.998	1529	1542	1564	rBV2	163503	347473	47.06%	5.901%
23	6.217	1608	1610	1613	rBV4	1437	868	0.12%	0.015%
24	6.256	1620	1622	1623	rBV2	1616	498	0.07%	0.008%
25	6.291	1632	1633	1635	rBV2	1434	722	0.10%	0.012%
26	6.494	1694	1696	1701	rVB4	1701	1096	0.15%	0.019%
27	6.580	1721	1723	1726	rBV3	1879	1172	0.16%	0.020%
28	6.744	1772	1774	1775	rBV2	1263	486	0.07%	0.008%
29	6.921	1821	1829	1846	rVB	78681	138958	18.82%	2.360%
30	7.252	1921	1932	1959	rBV	299087	547749	74.19%	9.302%
31	7.503	2006	2010	2014	rVB6	2284	2184	0.30%	0.037%
32	7.561	2020	2028	2048	rVB2	57679	105827	14.33%	1.797%
33	7.844	2114	2116	2117	rBV2	1195	461	0.06%	0.008%
34	7.873	2122	2125	2128	rBV3	2701	2145	0.29%	0.036%
35	7.905	2133	2135	2137	rBV4	1184	694	0.09%	0.012%
36	8.034	2166	2175	2191	rBV	164371	299799	40.61%	5.091%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030633.D
 Acq On : 18 Apr 2023 21:28
 Operator : SY/MD
 Sample : 02334-03 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.487	2314	2316	2319	rVB4	1640	808	0.11%	0.014%
38	8.661	2368	2370	2374	rVB5	1847	1000	0.14%	0.017%
39	8.747	2395	2397	2398	rBV3	1257	489	0.07%	0.008%
40	8.792	2400	2411	2434	rVV	419636	693510	93.93%	11.777%
41	9.606	2662	2664	2667	rVB4	2006	798	0.11%	0.014%
42	9.619	2667	2668	2670	rBV2	1372	678	0.09%	0.012%
43	9.889	2751	2752	2753	rBV	1151	378	0.05%	0.006%
44	9.979	2779	2780	2782	rBV2	651	255	0.03%	0.004%
45	10.120	2820	2824	2825	rBV4	1885	1292	0.17%	0.022%
46	10.162	2826	2837	2851	rVV	225411	367076	49.72%	6.234%
47	10.436	2915	2922	2923	rBV8	1503	1433	0.19%	0.024%
48	10.532	2950	2952	2954	rBV3	1373	745	0.10%	0.013%
49	10.596	2970	2972	2974	rBV2	2093	1202	0.16%	0.020%
50	10.622	2976	2980	2981	rVV4	1674	1227	0.17%	0.021%
51	10.683	2996	2999	3003	rBV6	1463	1313	0.18%	0.022%
52	10.747	3014	3019	3021	rBV5	1558	1518	0.21%	0.026%
53	10.879	3058	3060	3065	rVB7	1414	932	0.13%	0.016%
54	10.911	3065	3070	3071	rBV5	1735	1506	0.20%	0.026%
55	10.937	3076	3078	3080	rVB2	1068	394	0.05%	0.007%
56	11.030	3103	3107	3109	rBV4	1342	1024	0.14%	0.017%
57	11.194	3146	3158	3176	rBV	381309	620980	84.11%	10.545%
58	11.519	3254	3259	3262	rBV7	2593	2089	0.28%	0.035%
59	11.571	3262	3275	3290	rBV	315477	512678	69.44%	8.706%
60	11.815	3348	3351	3352	rBV3	1192	695	0.09%	0.012%
61	12.442	3545	3546	3547	rBV	1055	366	0.05%	0.006%
62	12.542	3574	3577	3580	rBV4	2124	1240	0.17%	0.021%
63	12.580	3587	3589	3592	rBV4	1442	909	0.12%	0.015%
64	12.625	3600	3603	3604	rBV3	1273	690	0.09%	0.012%
65	12.857	3671	3675	3676	rBV3	1623	1050	0.14%	0.018%
66	12.966	3707	3709	3710	rBV2	1206	379	0.05%	0.006%
67	13.223	3787	3789	3792	rBV3	1349	808	0.11%	0.014%
68	13.451	3858	3860	3861	rBV2	1260	509	0.07%	0.009%
69	13.564	3893	3895	3896	rBV2	1547	614	0.08%	0.010%
70	13.850	3982	3984	3986	rBV2	1837	1136	0.15%	0.019%
71	14.043	4042	4044	4047	rBV4	1485	732	0.10%	0.012%
72	14.217	4096	4098	4100	rBV3	1407	722	0.10%	0.012%
73	14.268	4112	4114	4117	rBV4	2273	1486	0.20%	0.025%
74	14.323	4128	4131	4133	rBV4	1911	1143	0.15%	0.019%
75	15.037	4351	4353	4355	rBV3	2071	867	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030633.D
Acq On : 18 Apr 2023 21:28
Operator : SY/MD
Sample : 02334-03 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis




Sum of corrected areas: 5888618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030633.D
Acq On : 18 Apr 2023 21:28
Operator : SY/MD
Sample : 02334-03 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

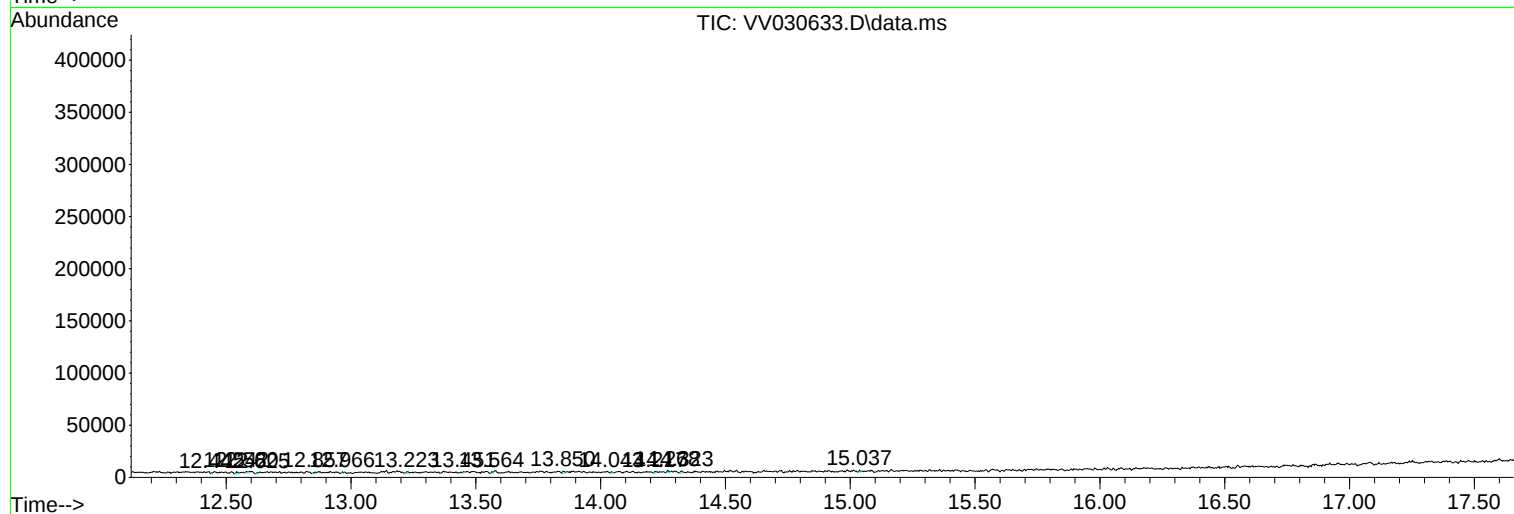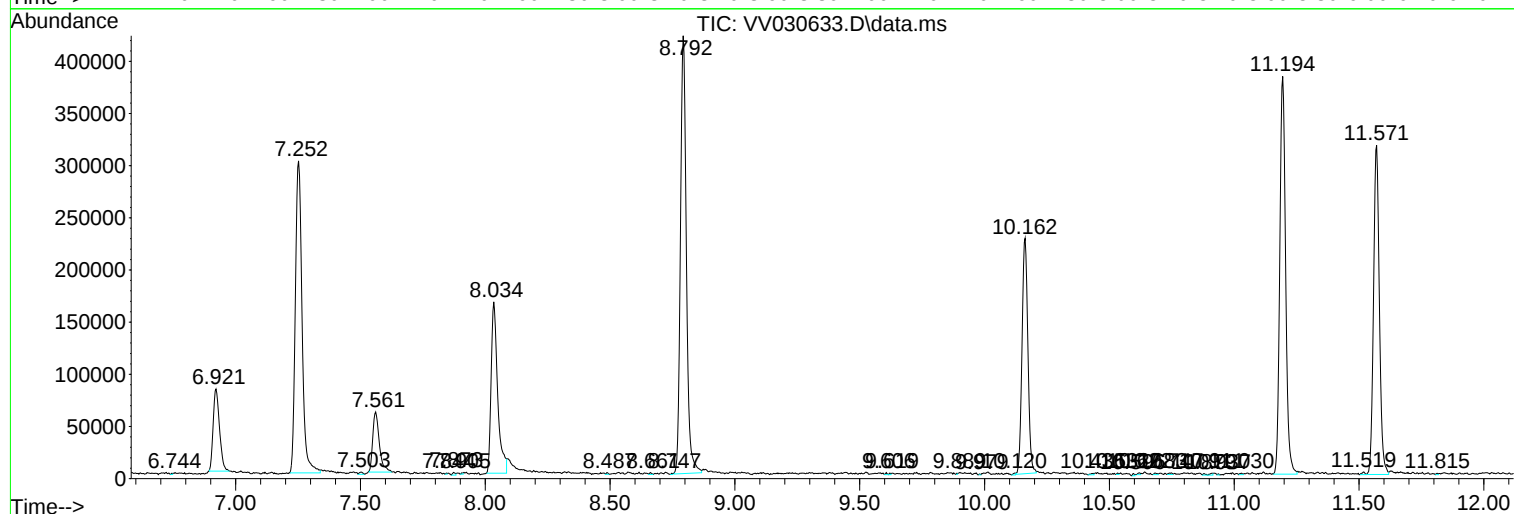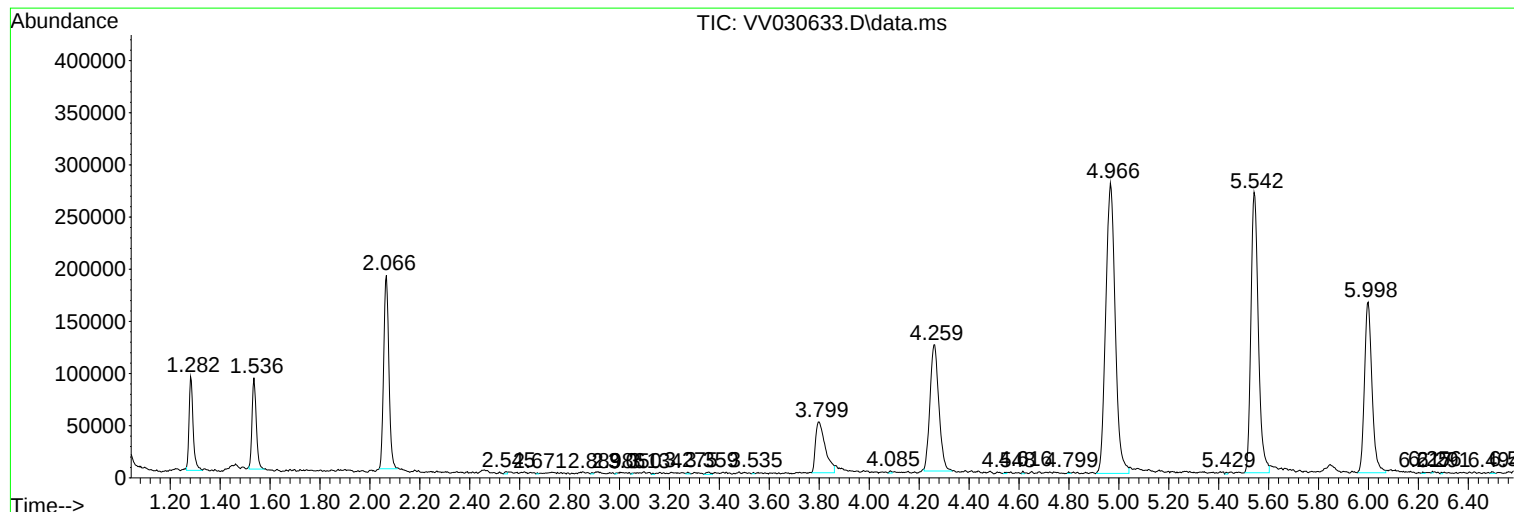

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030633.D
Acq On : 18 Apr 2023 21:28
Operator : SY/MD
Sample : 02334-03 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030633.D
Acq On : 18 Apr 2023 21:28
Operator : SY/MD
Sample : 02334-03 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------