

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030639.D
 Acq On : 19 Apr 2023 00:16
 Operator : SY/MD
 Sample : 02333-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	90	rVB	80998	89365	12.85%	1.516%
2	1.535	148	154	164	rVB	79380	90406	13.00%	1.534%
3	2.066	310	319	333	rBV	171391	240379	34.57%	4.079%
4	2.433	429	433	434	rBV4	2085	1636	0.24%	0.028%
5	2.445	436	437	439	rBV2	1805	920	0.13%	0.016%
6	2.568	473	475	478	rBV4	1158	715	0.10%	0.012%
7	2.609	487	488	492	rVB3	1311	791	0.11%	0.013%
8	2.899	576	578	582	rBV5	1091	923	0.13%	0.016%
9	2.963	596	598	602	rBV5	1893	1415	0.20%	0.024%
10	3.008	609	612	615	rVB5	1713	824	0.12%	0.014%
11	3.066	628	630	637	rVB7	1318	925	0.13%	0.016%
12	3.388	727	730	731	rBV3	1357	727	0.10%	0.012%
13	3.487	759	761	764	rBV4	1274	677	0.10%	0.011%
14	3.542	776	778	783	rVB5	1302	905	0.13%	0.015%
15	3.590	791	793	798	rBV4	1170	981	0.14%	0.017%
16	3.712	828	831	833	rBV3	1577	834	0.12%	0.014%
17	3.799	848	858	887	rBV2	54210	157200	22.61%	2.668%
18	4.259	989	1001	1024	rVB	117510	298272	42.90%	5.062%
19	4.523	1081	1083	1087	rBV5	2109	1159	0.17%	0.020%
20	4.616	1110	1112	1115	rBV4	1213	705	0.10%	0.012%
21	4.664	1120	1127	1128	rBV5	1992	1584	0.23%	0.027%
22	4.767	1156	1159	1161	rBV5	1709	970	0.14%	0.016%
23	4.831	1176	1179	1182	rBV5	1298	1028	0.15%	0.017%
24	4.857	1182	1187	1188	rBV4	2319	1453	0.21%	0.025%
25	4.966	1206	1221	1247	rVV2	260715	695339	100.00%	11.800%
26	5.227	1300	1302	1304	rBV3	1671	658	0.09%	0.011%
27	5.542	1387	1400	1427	rBV	271805	576914	82.97%	9.790%
28	5.998	1530	1542	1562	rBV2	162230	336386	48.38%	5.708%
29	6.188	1599	1601	1603	rBV2	1418	733	0.11%	0.012%
30	6.423	1671	1674	1677	rBV5	1811	1273	0.18%	0.022%
31	6.661	1742	1748	1750	rBV6	2095	2079	0.30%	0.035%
32	6.715	1762	1765	1768	rBV5	1502	884	0.13%	0.015%
33	6.921	1820	1829	1843	rBV	76534	138888	19.97%	2.357%
34	7.252	1921	1932	1950	rBV	280110	494180	71.07%	8.386%
35	7.561	2019	2028	2044	rBV2	56533	100821	14.50%	1.711%
36	7.982	2156	2159	2161	rBV3	1388	700	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030639.D
 Acq On : 19 Apr 2023 00:16
 Operator : SY/MD
 Sample : 02333-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.034	2165	2175	2205	rBV	175512	357644	51.43%	6.069%
38	8.362	2274	2277	2278	rBV3	1546	668	0.10%	0.011%
39	8.603	2346	2352	2353	rVV5	1228	1256	0.18%	0.021%
40	8.686	2376	2378	2382	rVB5	2392	1291	0.19%	0.022%
41	8.792	2400	2411	2431	rBV	417451	687332	98.85%	11.664%
42	9.043	2486	2489	2491	rBV3	1594	1037	0.15%	0.018%
43	9.124	2511	2514	2519	rBV7	1066	1132	0.16%	0.019%
44	9.185	2529	2533	2535	rVV4	1267	1071	0.15%	0.018%
45	9.278	2557	2562	2565	rBV7	2094	1968	0.28%	0.033%
46	9.519	2633	2637	2641	rBV6	2065	1714	0.25%	0.029%
47	9.548	2644	2646	2648	rBV3	1565	784	0.11%	0.013%
48	9.593	2656	2660	2662	rBV5	2229	1579	0.23%	0.027%
49	9.792	2720	2722	2724	rVV4	1524	646	0.09%	0.011%
50	9.812	2726	2728	2731	rVV3	1685	761	0.11%	0.013%
51	9.866	2742	2745	2747	rBV5	1987	830	0.12%	0.014%
52	9.966	2774	2776	2778	rBV3	1317	753	0.11%	0.013%
53	9.995	2781	2785	2788	rBV6	1392	1237	0.18%	0.021%
54	10.062	2804	2806	2809	rVB4	1136	611	0.09%	0.010%
55	10.082	2809	2812	2817	rBV6	1717	1618	0.23%	0.027%
56	10.162	2824	2837	2850	rBV	242361	393164	56.54%	6.672%
57	10.333	2887	2890	2893	rBV5	1332	994	0.14%	0.017%
58	10.480	2934	2936	2941	rBV6	1169	863	0.12%	0.015%
59	10.554	2955	2959	2960	rBV3	1260	784	0.11%	0.013%
60	10.583	2965	2968	2970	rBV4	2049	1146	0.16%	0.019%
61	10.632	2980	2983	2986	rVB5	1503	1034	0.15%	0.018%
62	10.651	2986	2989	2993	rBV6	2177	1552	0.22%	0.026%
63	10.683	2997	2999	3002	rBV4	974	651	0.09%	0.011%
64	10.760	3022	3023	3027	rVB3	1700	725	0.10%	0.012%
65	10.783	3027	3030	3031	rBV3	1697	819	0.12%	0.014%
66	10.818	3038	3041	3045	rBV6	1347	1054	0.15%	0.018%
67	10.876	3057	3059	3063	rBV4	1736	1014	0.15%	0.017%
68	10.947	3077	3081	3084	rBV6	1129	764	0.11%	0.013%
69	11.072	3116	3120	3125	rVB8	1525	1408	0.20%	0.024%
70	11.101	3125	3129	3133	rBV7	1138	1265	0.18%	0.021%
71	11.194	3146	3158	3178	rBV	393132	630587	90.69%	10.701%
72	11.423	3228	3229	3232	rBV3	1636	853	0.12%	0.014%
73	11.567	3262	3274	3288	rBV	323676	516286	74.25%	8.761%
74	11.799	3344	3346	3347	rBV2	1428	752	0.11%	0.013%
75	11.869	3366	3368	3372	rVB5	1635	699	0.10%	0.012%
76	11.927	3383	3386	3389	rVB5	1353	952	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030639.D
 Acq On : 19 Apr 2023 00:16
 Operator : SY/MD
 Sample : 02333-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.947	3389	3392	3395	rBV4	1561	1167	0.17%	0.020%
78	12.091	3434	3437	3439	rBV3	1371	787	0.11%	0.013%
79	12.123	3444	3447	3452	rBV6	1681	1261	0.18%	0.021%
80	12.146	3452	3454	3456	rBV4	1822	971	0.14%	0.016%
81	12.239	3482	3483	3486	rVB3	1998	698	0.10%	0.012%
82	12.259	3486	3489	3491	rBV4	1759	1106	0.16%	0.019%
83	12.294	3497	3500	3505	rVV6	1393	1049	0.15%	0.018%
84	12.702	3624	3627	3628	rBV4	1406	698	0.10%	0.012%
85	12.731	3632	3636	3639	rBV6	1739	1445	0.21%	0.025%
86	12.802	3653	3658	3663	rVB8	1974	2008	0.29%	0.034%
87	12.821	3663	3664	3667	rBV3	1870	944	0.14%	0.016%
88	12.892	3682	3686	3692	rBV8	2009	2360	0.34%	0.040%
89	13.107	3750	3753	3755	rBV4	1829	857	0.12%	0.015%
90	13.384	3835	3839	3840	rBV4	1438	1089	0.16%	0.018%
91	13.554	3888	3892	3893	rBV3	1066	743	0.11%	0.013%
92	13.577	3897	3899	3902	rBV4	1068	831	0.12%	0.014%
93	13.612	3908	3910	3912	rBV3	1864	843	0.12%	0.014%
94	13.834	3974	3979	3981	rBV7	2282	2065	0.30%	0.035%
95	14.024	4035	4038	4040	rBV4	1620	919	0.13%	0.016%
96	14.268	4110	4114	4115	rBV4	1315	916	0.13%	0.016%
97	14.403	4154	4156	4160	rVB6	1728	1141	0.16%	0.019%
98	14.429	4160	4164	4167	rBV6	1970	1398	0.20%	0.024%
99	14.471	4175	4177	4182	rVB5	1659	895	0.13%	0.015%
100	14.969	4329	4332	4337	rBV7	2344	1751	0.25%	0.030%




Sum of corrected areas: 5892889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030639.D
Acq On : 19 Apr 2023 00:16
Operator : SY/MD
Sample : 02333-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

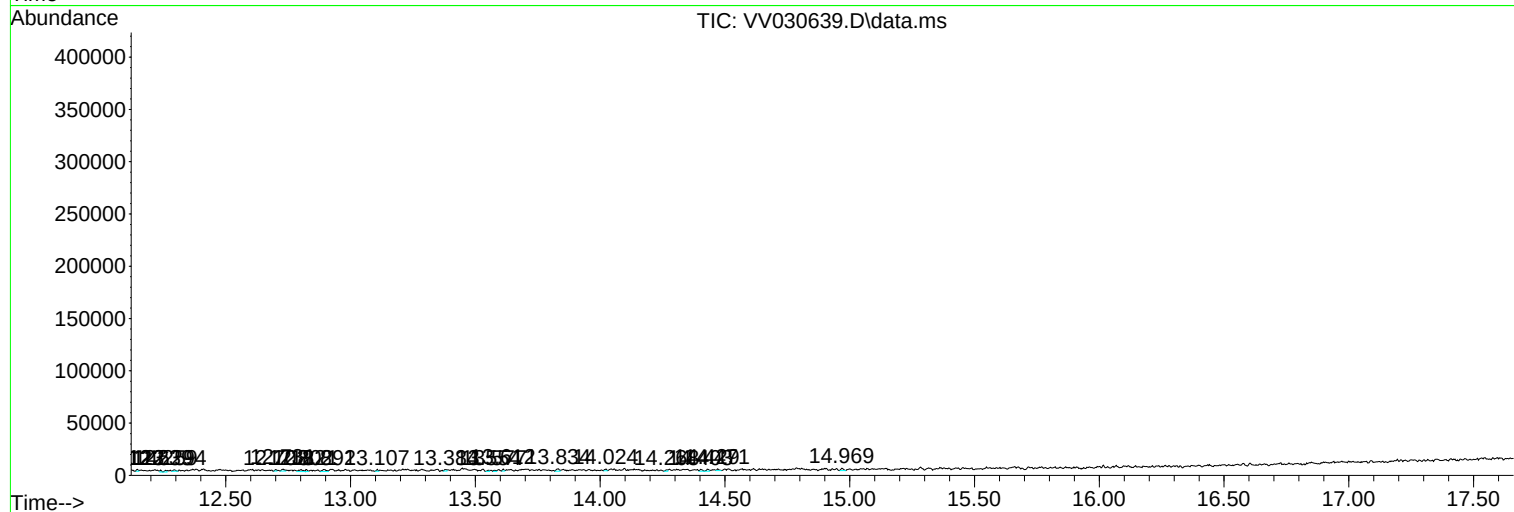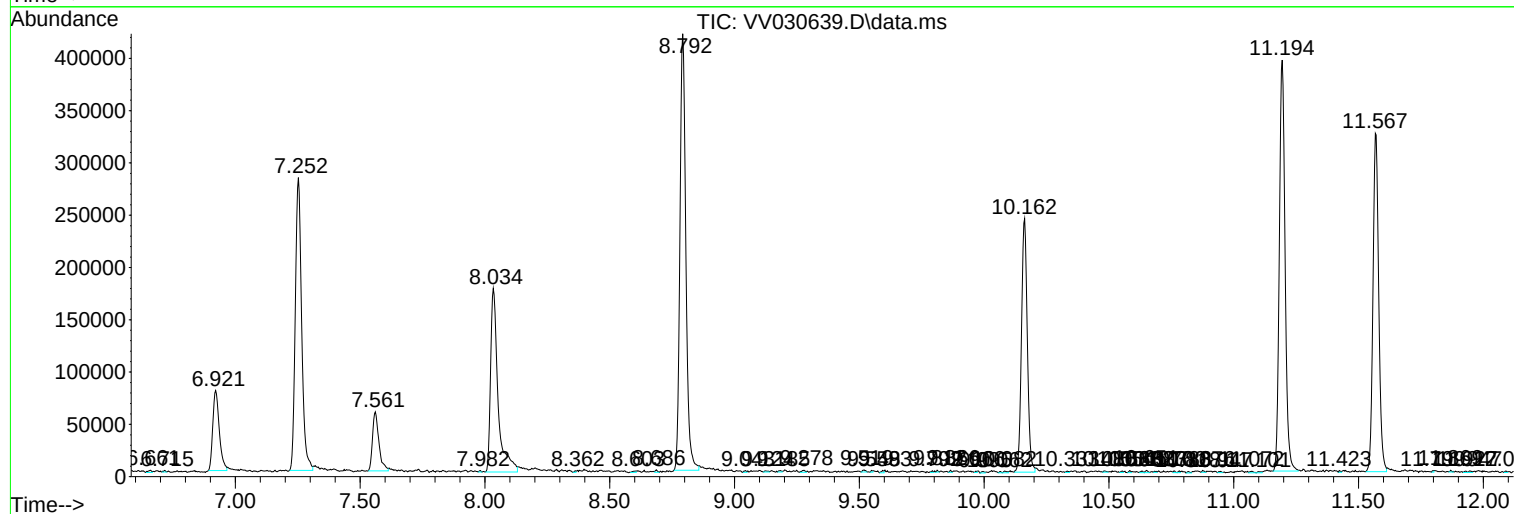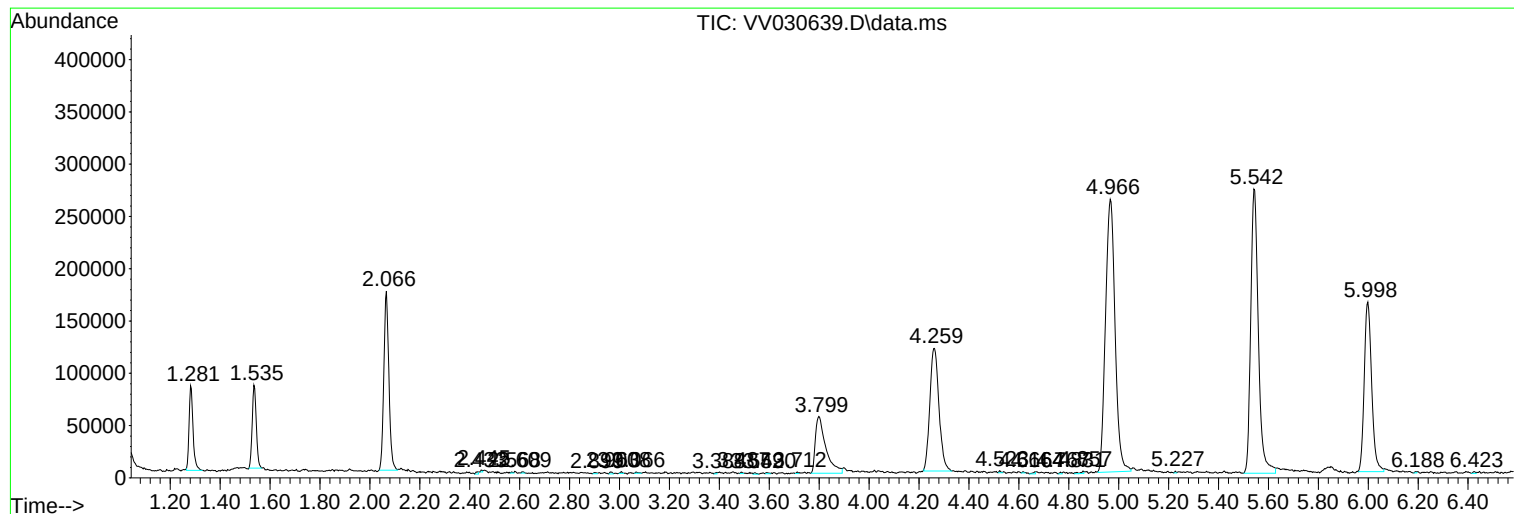

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030639.D
Acq On : 19 Apr 2023 00:16
Operator : SY/MD
Sample : 02333-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030639.D
Acq On : 19 Apr 2023 00:16
Operator : SY/MD
Sample : 02333-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------