

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030640.D
 Acq On : 19 Apr 2023 00:40
 Operator : SY/MD
 Sample : 02333-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	87	rBV	81711	88878	12.91%	1.540%
2	1.536	148	154	163	rVB	79337	89364	12.99%	1.548%
3	1.870	256	258	259	rBV	2037	767	0.11%	0.013%
4	2.063	310	318	335	rVB	164784	233207	33.89%	4.041%
5	2.163	346	349	351	rBV4	2637	1892	0.27%	0.033%
6	2.333	400	402	404	rBV3	1477	670	0.10%	0.012%
7	2.548	467	469	473	rVB5	2465	1286	0.19%	0.022%
8	2.568	473	475	477	rBV3	1119	647	0.09%	0.011%
9	2.635	493	496	499	rBV5	2007	1276	0.19%	0.022%
10	2.751	528	532	535	rBV5	1726	1226	0.18%	0.021%
11	2.976	598	602	606	rVB5	1436	1073	0.16%	0.019%
12	2.999	606	609	610	rBV3	1453	903	0.13%	0.016%
13	3.056	624	627	632	rBV7	1656	1667	0.24%	0.029%
14	3.291	697	700	703	rBV5	1285	781	0.11%	0.014%
15	3.310	703	706	709	rBV5	993	704	0.10%	0.012%
16	3.381	725	728	732	rBV6	1763	1216	0.18%	0.021%
17	3.478	752	758	761	rVB7	2003	1921	0.28%	0.033%
18	3.497	761	764	765	rBV3	1644	945	0.14%	0.016%
19	3.597	793	795	797	rBV3	1449	857	0.12%	0.015%
20	3.654	808	813	815	rBV5	1299	1423	0.21%	0.025%
21	3.674	817	819	822	rBV3	1970	1130	0.16%	0.020%
22	3.706	826	829	833	rBV6	1551	1194	0.17%	0.021%
23	3.732	833	837	839	rBV5	1531	847	0.12%	0.015%
24	3.764	843	847	849	rBV5	1735	1475	0.21%	0.026%
25	3.799	849	858	889	rBV2	52732	157457	22.88%	2.728%
26	4.037	929	932	937	rVB6	1760	1762	0.26%	0.031%
27	4.150	964	967	969	rBV3	2388	1454	0.21%	0.025%
28	4.188	977	979	982	rBV4	1369	723	0.11%	0.013%
29	4.259	989	1001	1030	rVB2	117077	298270	43.34%	5.168%
30	4.471	1065	1067	1068	rBV2	1991	909	0.13%	0.016%
31	4.577	1095	1100	1102	rBV5	1626	1563	0.23%	0.027%
32	4.966	1205	1221	1240	rBV2	259784	688194	100.00%	11.924%
33	5.246	1305	1308	1310	rBV4	1525	992	0.14%	0.017%
34	5.407	1355	1358	1360	rBV3	1857	1027	0.15%	0.018%
35	5.542	1389	1400	1420	rBV	258426	527457	76.64%	9.139%
36	5.995	1528	1541	1558	rBV	161646	343154	49.86%	5.946%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030640.D
 Acq On : 19 Apr 2023 00:40
 Operator : SY/MD
 Sample : 02333-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.474	1687	1690	1691	rBV3	1228	612	0.09%	0.011%
38	6.510	1697	1701	1704	rBV5	1549	1245	0.18%	0.022%
39	6.613	1730	1733	1738	rBV7	1613	1526	0.22%	0.026%
40	6.854	1805	1808	1809	rBV3	1936	847	0.12%	0.015%
41	6.921	1818	1829	1849	rBV2	77324	148332	21.55%	2.570%
42	7.111	1884	1888	1894	rBV7	2615	3639	0.53%	0.063%
43	7.207	1916	1918	1920	rBV3	2090	1009	0.15%	0.017%
44	7.252	1920	1932	1949	rVV	278855	490114	71.22%	8.492%
45	7.484	2002	2004	2009	rBV6	1779	1243	0.18%	0.022%
46	7.561	2019	2028	2048	rVV2	56474	104311	15.16%	1.807%
47	7.831	2108	2112	2115	rBV6	1768	1724	0.25%	0.030%
48	7.886	2127	2129	2132	rBV4	1668	877	0.13%	0.015%
49	8.034	2166	2175	2206	rBV	174547	340727	49.51%	5.904%
50	8.330	2265	2267	2269	rBV2	1574	691	0.10%	0.012%
51	8.606	2348	2353	2355	rBV6	2146	1946	0.28%	0.034%
52	8.793	2399	2411	2430	rBV	404133	671078	97.51%	11.628%
53	9.056	2491	2493	2495	rBV3	1428	687	0.10%	0.012%
54	9.114	2508	2511	2512	rVV2	1586	1094	0.16%	0.019%
55	9.182	2528	2532	2535	rBV6	1595	1549	0.23%	0.027%
56	9.252	2552	2554	2560	rVB6	1724	1418	0.21%	0.025%
57	9.503	2629	2632	2634	rBV4	1668	863	0.13%	0.015%
58	9.741	2704	2706	2712	rBV7	1796	1640	0.24%	0.028%
59	9.866	2742	2745	2746	rBV3	1586	1004	0.15%	0.017%
60	9.899	2753	2755	2756	rBV2	1560	695	0.10%	0.012%
61	9.944	2766	2769	2771	rBV4	1231	654	0.10%	0.011%
62	9.969	2775	2777	2780	rBV3	1000	686	0.10%	0.012%
63	10.030	2793	2796	2801	rBV6	1511	1555	0.23%	0.027%
64	10.079	2808	2811	2814	rBV5	926	666	0.10%	0.012%
65	10.159	2826	2836	2850	rBV	246159	382653	55.60%	6.630%
66	10.259	2865	2867	2870	rVB4	1656	647	0.09%	0.011%
67	10.481	2931	2936	2938	rBV5	2358	2017	0.29%	0.035%
68	10.548	2953	2957	2958	rBV4	1176	829	0.12%	0.014%
69	10.590	2967	2970	2972	rBV4	1109	634	0.09%	0.011%
70	10.657	2988	2991	2994	rBV4	1749	1054	0.15%	0.018%
71	10.792	3026	3033	3036	rBV9	1759	2508	0.36%	0.043%
72	10.892	3060	3064	3065	rBV4	1485	902	0.13%	0.016%
73	10.911	3068	3070	3073	rVV4	1296	749	0.11%	0.013%
74	10.979	3089	3091	3094	rBV4	1888	981	0.14%	0.017%
75	11.194	3147	3158	3180	rVB	369481	594039	86.32%	10.293%
76	11.445	3234	3236	3238	rBV3	1897	928	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030640.D
 Acq On : 19 Apr 2023 00:40
 Operator : SY/MD
 Sample : 02333-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3292	rBV	317911	515045	74.84%	8.924%
78	11.747	3328	3330	3332	rBV3	1366	786	0.11%	0.014%
79	11.899	3374	3377	3381	rBV5	1770	1936	0.28%	0.034%
80	11.963	3394	3397	3400	rBV4	2013	1241	0.18%	0.022%
81	12.005	3407	3410	3414	rBV5	2160	1721	0.25%	0.030%
82	12.426	3539	3541	3543	rBV3	1276	778	0.11%	0.013%
83	12.599	3591	3595	3599	rBV7	2296	1688	0.25%	0.029%
84	12.664	3611	3615	3617	rBV5	1785	1670	0.24%	0.029%
85	12.818	3661	3663	3665	rBV3	1153	639	0.09%	0.011%
86	12.889	3683	3685	3691	rBV6	991	801	0.12%	0.014%
87	12.937	3697	3700	3702	rBV4	1709	1299	0.19%	0.023%
88	12.998	3716	3719	3721	rVV3	1057	669	0.10%	0.012%
89	13.024	3724	3727	3730	rBV5	1345	960	0.14%	0.017%
90	13.127	3756	3759	3760	rBV3	1560	959	0.14%	0.017%
91	13.587	3898	3902	3906	rBV7	1523	1237	0.18%	0.021%
92	13.693	3933	3935	3938	rVB4	1479	777	0.11%	0.013%
93	13.770	3956	3959	3961	rBV4	1465	778	0.11%	0.013%
94	13.873	3988	3991	3994	rBV5	1029	673	0.10%	0.012%
95	13.892	3994	3997	4004	rVV8	1996	2562	0.37%	0.044%
96	13.918	4004	4005	4009	rVB3	1696	1135	0.16%	0.020%
97	14.046	4043	4045	4047	rBV3	1427	818	0.12%	0.014%
98	14.117	4063	4067	4069	rBV5	1353	1239	0.18%	0.021%
99	14.365	4141	4144	4146	rBV3	2994	2363	0.34%	0.041%
100	15.037	4351	4353	4356	rBV4	2085	886	0.13%	0.015%




Sum of corrected areas: 5771344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030640.D
Acq On : 19 Apr 2023 00:40
Operator : SY/MD
Sample : 02333-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

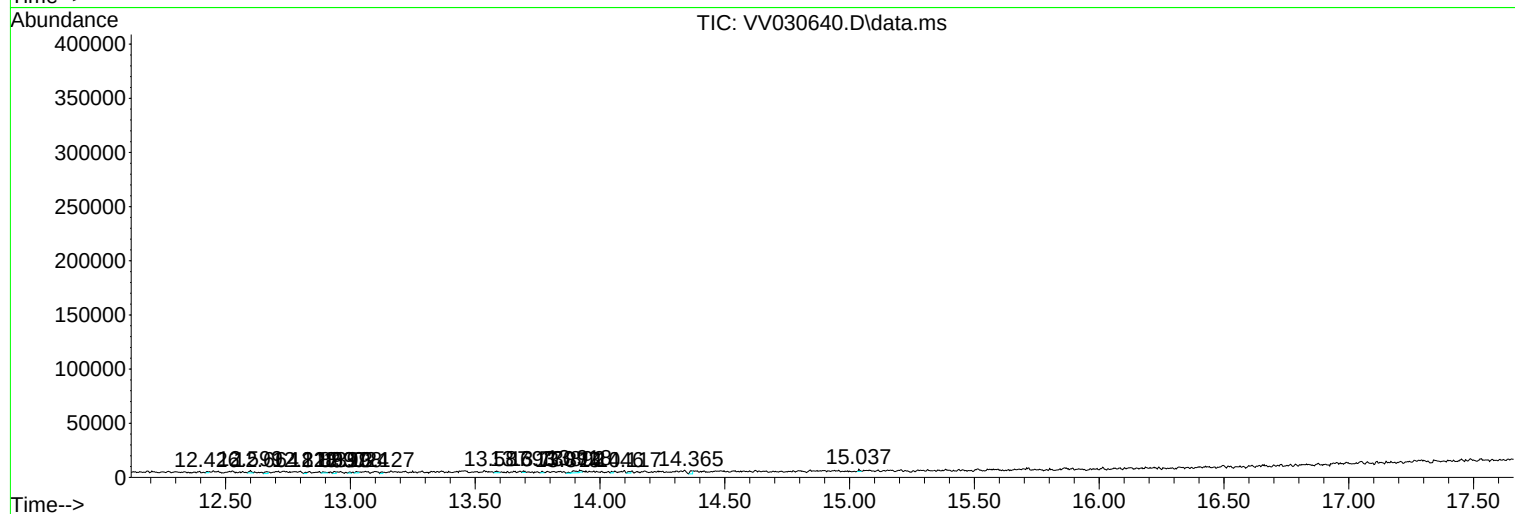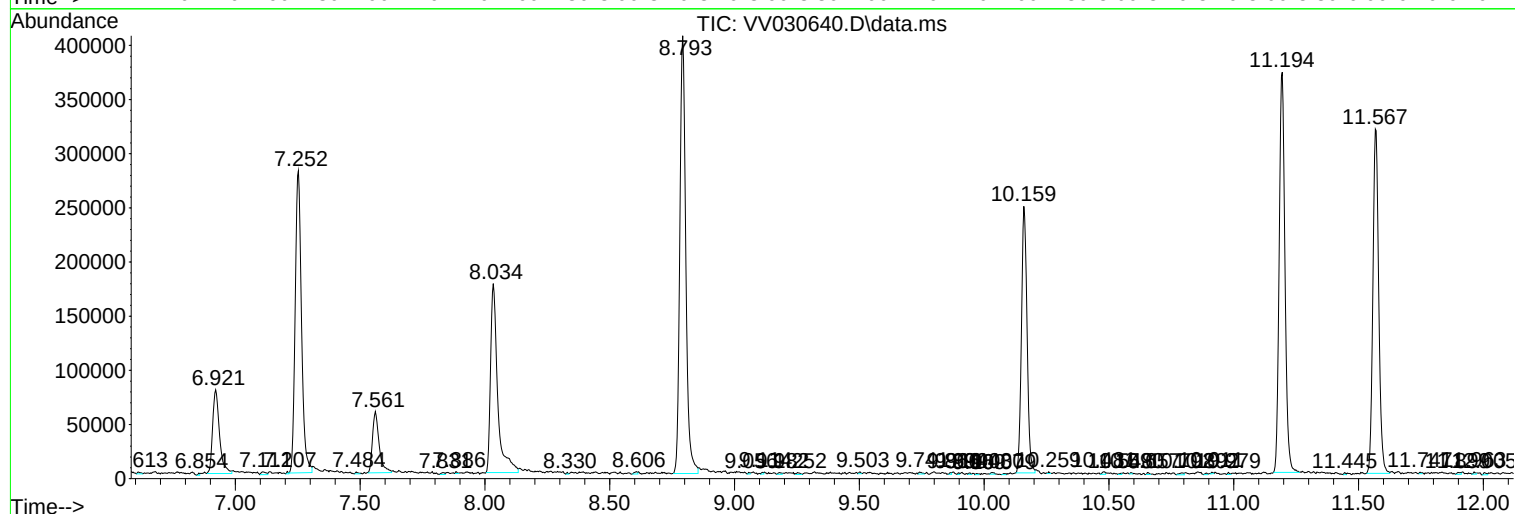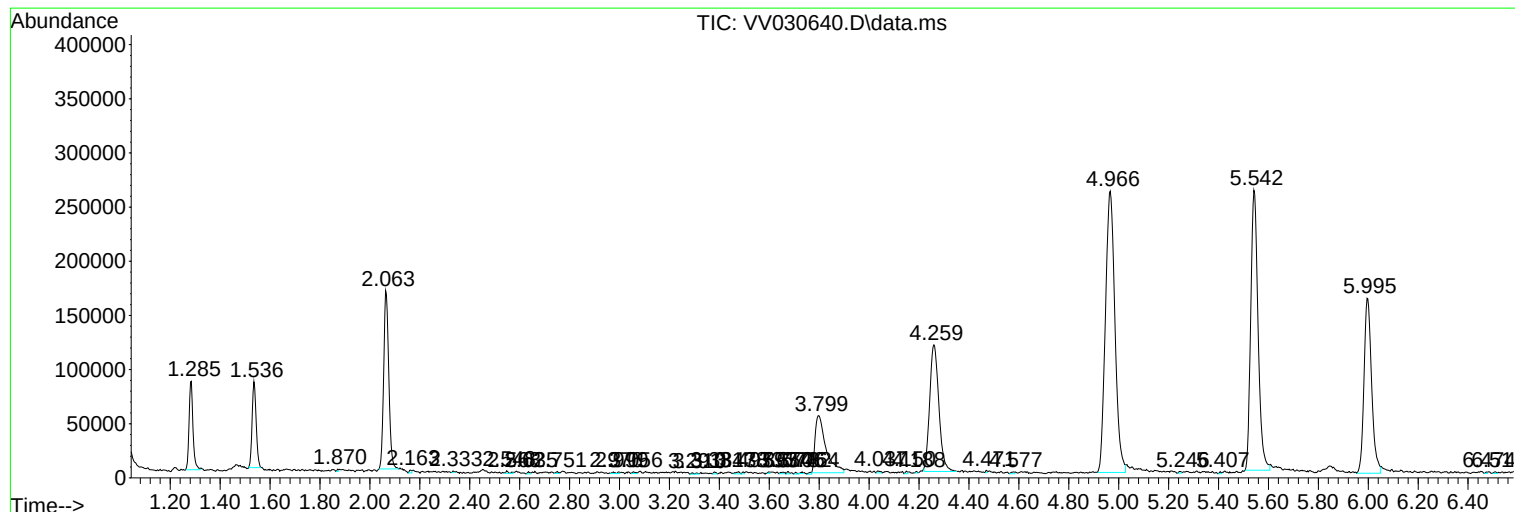

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030640.D
Acq On : 19 Apr 2023 00:40
Operator : SY/MD
Sample : 02333-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030640.D
Acq On : 19 Apr 2023 00:40
Operator : SY/MD
Sample : 02333-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------