

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030647.D
 Acq On : 19 Apr 2023 03:27
 Operator : SY/MD
 Sample : 02398-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	89	rVB	86149	94014	1.88%	0.643%
2	1.536	148	154	167	rVB	88284	101474	2.02%	0.694%
3	2.066	310	319	333	rVB	174314	253310	5.05%	1.733%
4	2.317	393	397	399	rBV5	1780	1222	0.02%	0.008%
5	2.365	410	412	414	rBV3	1546	683	0.01%	0.005%
6	2.677	507	509	511	rBV3	1307	473	0.01%	0.003%
7	2.767	535	537	538	rBV2	1388	455	0.01%	0.003%
8	2.806	548	549	552	rBV3	717	399	0.01%	0.003%
9	2.822	552	554	555	rVV2	1242	446	0.01%	0.003%
10	2.841	559	560	563	rBV3	928	478	0.01%	0.003%
11	2.976	599	602	605	rBV4	1703	1202	0.02%	0.008%
12	3.101	639	641	643	rBV3	1358	800	0.02%	0.005%
13	3.143	652	654	656	rBV3	1701	767	0.02%	0.005%
14	3.188	664	668	671	rBV6	891	888	0.02%	0.006%
15	3.204	671	673	675	rVV3	1235	668	0.01%	0.005%
16	3.246	684	686	688	rBV3	1433	755	0.02%	0.005%
17	3.265	690	692	694	rVB3	1197	341	0.01%	0.002%
18	3.304	702	704	708	rBV5	1529	1027	0.02%	0.007%
19	3.359	719	721	726	rVB6	2300	1616	0.03%	0.011%
20	3.381	726	728	730	rBV3	1401	895	0.02%	0.006%
21	3.420	738	740	742	rBV3	778	346	0.01%	0.002%
22	3.439	742	746	750	rBV5	1468	1295	0.03%	0.009%
23	3.465	752	754	756	rBV3	742	380	0.01%	0.003%
24	3.548	779	780	782	rVB3	860	202	0.00%	0.001%
25	3.568	783	786	788	rBV4	1107	680	0.01%	0.005%
26	3.616	800	801	804	rBV2	1015	513	0.01%	0.004%
27	3.674	816	819	823	rBV6	2400	1612	0.03%	0.011%
28	3.693	823	825	826	rBV3	1130	376	0.01%	0.003%
29	3.725	832	835	837	rBV4	1517	793	0.02%	0.005%
30	3.799	848	858	880	rBV	50105	144367	2.88%	0.988%
31	4.259	989	1001	1025	rVB	120193	308391	6.15%	2.110%
32	4.478	1066	1069	1070	rBV3	1228	548	0.01%	0.004%
33	4.696	1134	1137	1138	rBV2	911	519	0.01%	0.004%
34	4.706	1138	1140	1142	rVV4	1180	470	0.01%	0.003%
35	4.838	1179	1181	1185	rBV5	2305	1257	0.03%	0.009%
36	4.966	1205	1221	1227	rBV2	282987	659658	13.16%	4.514%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030647.D
 Acq On : 19 Apr 2023 03:27
 Operator : SY/MD
 Sample : 02398-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.542	1388	1400	1425	rBV	286825	595087	11.87%	4.072%
38	5.998	1530	1542	1566	rBV2	169636	347456	6.93%	2.377%
39	6.384	1660	1662	1667	rVB6	1805	1205	0.02%	0.008%
40	6.487	1691	1694	1697	rBV4	1707	1319	0.03%	0.009%
41	6.542	1708	1711	1715	rBV6	2025	1670	0.03%	0.011%
42	6.744	1769	1774	1777	rBV5	1762	1683	0.03%	0.012%
43	6.838	1801	1803	1805	rBV3	1611	857	0.02%	0.006%
44	6.921	1817	1829	1845	rBV2	82509	158115	3.15%	1.082%
45	7.117	1888	1890	1891	rBV3	1228	489	0.01%	0.003%
46	7.252	1920	1932	1949	rBV	302318	533941	10.65%	3.653%
47	7.510	2009	2012	2014	rBV4	1425	700	0.01%	0.005%
48	7.561	2019	2028	2041	rVV2	59033	103733	2.07%	0.710%
49	7.902	2132	2134	2137	rBV4	2343	1675	0.03%	0.011%
50	8.034	2166	2175	2206	rBV	162449	314143	6.27%	2.150%
51	8.307	2257	2260	2262	rBV4	1799	1126	0.02%	0.008%
52	8.606	2350	2353	2354	rBV3	2010	909	0.02%	0.006%
53	8.635	2360	2362	2363	rBV2	1640	744	0.01%	0.005%
54	8.821	2400	2420	2452	rBV2	2666415	5013709	100.00%	34.306%
55	9.165	2524	2527	2528	rBV2	1935	1125	0.02%	0.008%
56	9.622	2667	2669	2673	rBV5	1452	888	0.02%	0.006%
57	9.670	2681	2684	2687	rBV4	2382	1822	0.04%	0.012%
58	9.728	2700	2702	2703	rBV2	1043	426	0.01%	0.003%
59	9.882	2745	2750	2752	rBV5	2361	1922	0.04%	0.013%
60	9.915	2758	2760	2762	rBV3	1199	412	0.01%	0.003%
61	9.950	2769	2771	2777	rBV6	1172	872	0.02%	0.006%
62	10.072	2806	2809	2812	rVB5	1191	612	0.01%	0.004%
63	10.159	2826	2836	2854	rVB	236349	374348	7.47%	2.561%
64	10.239	2859	2861	2866	rVB7	1598	1026	0.02%	0.007%
65	10.378	2900	2904	2906	rBV5	1847	1441	0.03%	0.010%
66	10.474	2930	2934	2937	rBV5	2175	2168	0.04%	0.015%
67	10.542	2953	2955	2956	rBV2	982	455	0.01%	0.003%
68	10.571	2961	2964	2967	rBV5	2603	1662	0.03%	0.011%
69	10.596	2970	2972	2974	rBV3	1539	991	0.02%	0.007%
70	10.661	2990	2992	2994	rBV3	1310	506	0.01%	0.003%
71	10.686	2998	3000	3005	rVB6	1186	759	0.02%	0.005%
72	10.709	3005	3007	3008	rBV	2181	733	0.01%	0.005%
73	10.847	3046	3050	3054	rBV5	1562	1387	0.03%	0.009%
74	11.079	3118	3122	3123	rBV5	1479	1135	0.02%	0.008%
75	11.127	3127	3137	3147	rVV	133844	210867	4.21%	1.443%
76	11.217	3148	3165	3186	rVB2	964954	2127607	42.44%	14.558%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030647.D
 Acq On : 19 Apr 2023 03:27
 Operator : SY/MD
 Sample : 02398-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.480	3245	3247	3249	rVB3	1507	590	0.01%	0.004%
78	11.587	3265	3280	3298	rVB2	1186852	2261928	45.11%	15.477%
79	11.760	3332	3334	3340	rVB5	2041	1728	0.03%	0.012%
80	11.866	3365	3367	3371	rVB4	1934	1188	0.02%	0.008%
81	12.011	3410	3412	3415	rBV3	1175	655	0.01%	0.004%
82	12.088	3431	3436	3441	rVB8	1857	2355	0.05%	0.016%
83	12.111	3441	3443	3445	rBV3	1932	1095	0.02%	0.007%
84	12.236	3481	3482	3483	rBV	1510	447	0.01%	0.003%
85	12.590	3588	3592	3603	rVB	4234	6208	0.12%	0.042%
86	12.734	3635	3637	3640	rBV4	1292	890	0.02%	0.006%
87	12.831	3666	3667	3668	rBV	1068	293	0.01%	0.002%
88	12.869	3674	3679	3681	rBV5	2359	1788	0.04%	0.012%
89	12.995	3717	3718	3720	rBV2	1023	534	0.01%	0.004%
90	13.149	3764	3766	3767	rBV2	1280	542	0.01%	0.004%
91	13.207	3773	3784	3797	rBV	472325	721968	14.40%	4.940%
92	13.522	3880	3882	3883	rBV2	1527	516	0.01%	0.004%
93	13.689	3923	3934	3950	rBV2	131110	209022	4.17%	1.430%
94	14.017	4031	4036	4039	rBV8	2027	1915	0.04%	0.013%
95	14.098	4057	4061	4064	rVB5	1829	1292	0.03%	0.009%
96	14.172	4082	4084	4085	rBV2	1931	779	0.02%	0.005%
97	14.236	4102	4104	4107	rBV4	1127	783	0.02%	0.005%
98	14.365	4143	4144	4146	rVB2	1865	532	0.01%	0.004%
99	14.516	4189	4191	4193	rBV3	1541	775	0.02%	0.005%
100	14.725	4253	4256	4257	rBV2	2635	1691	0.03%	0.012%




Sum of corrected areas: 14614559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030647.D
Acq On : 19 Apr 2023 03:27
Operator : SY/MD
Sample : 02398-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMNO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

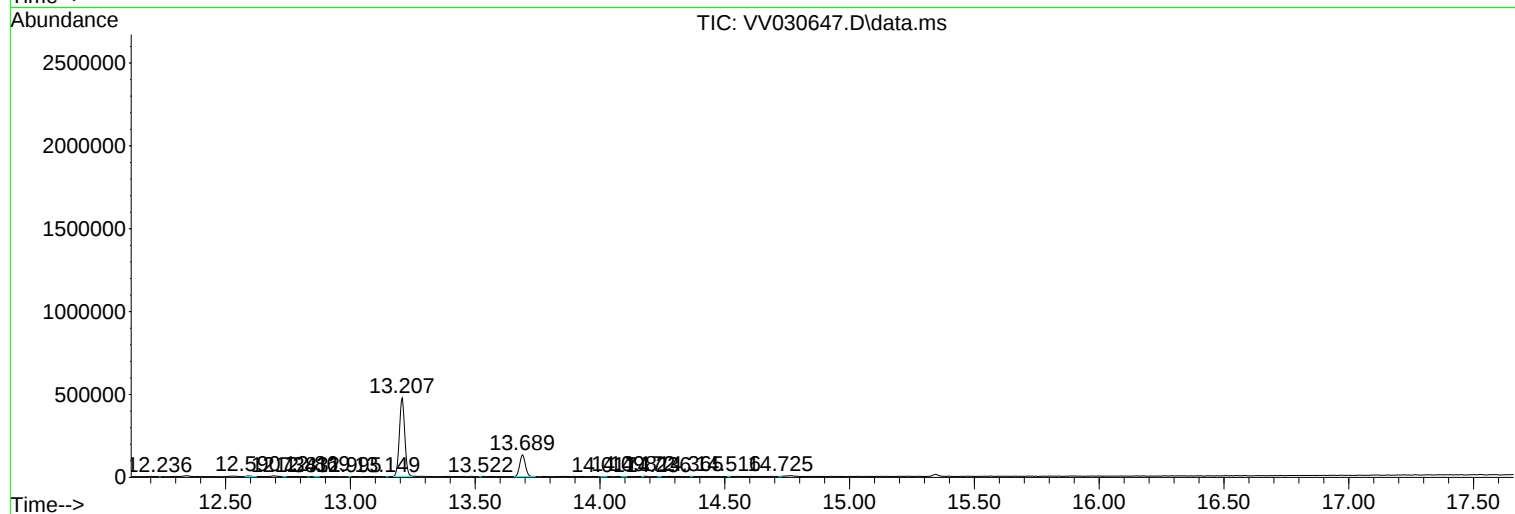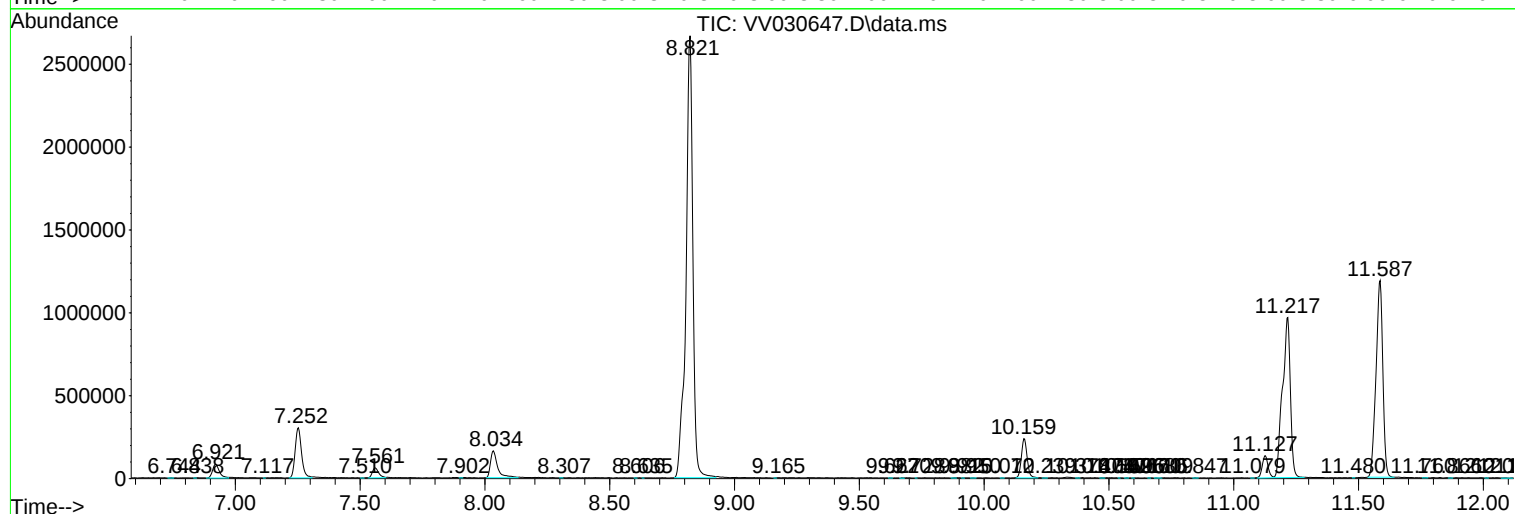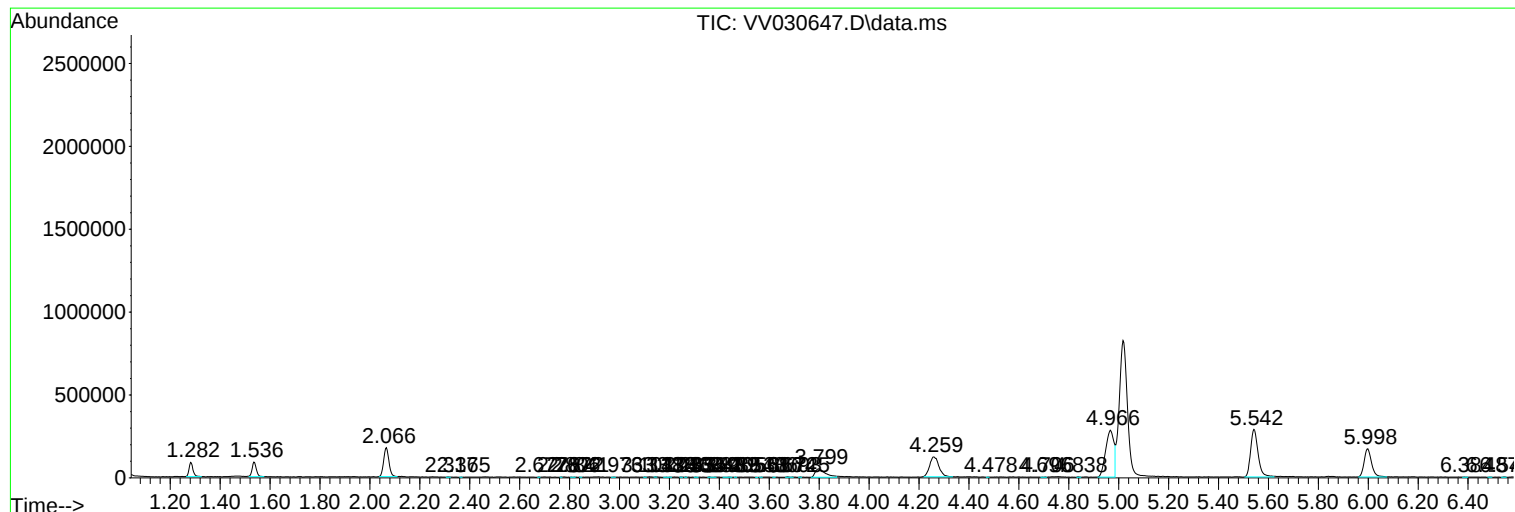

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030647.D
Acq On : 19 Apr 2023 03:27
Operator : SY/MD
Sample : 02398-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030647.D
Acq On : 19 Apr 2023 03:27
Operator : SY/MD
Sample : 02398-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------