

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030648.D
 Acq On : 19 Apr 2023 03:51
 Operator : SY/MD
 Sample : 02398-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	90	rVB	83868	93130	1.91%	0.650%
2	1.536	148	154	167	rVB	83148	98030	2.01%	0.685%
3	2.066	310	319	331	rVB	168739	243789	4.99%	1.703%
4	2.458	439	441	446	rVB6	2151	1844	0.04%	0.013%
5	2.548	467	469	471	rBV3	1342	812	0.02%	0.006%
6	2.593	481	483	486	rBV3	1635	929	0.02%	0.006%
7	2.635	494	496	499	rBV3	1249	730	0.01%	0.005%
8	2.748	529	531	532	rBV2	1192	487	0.01%	0.003%
9	2.809	545	550	551	rBV3	1148	814	0.02%	0.006%
10	2.912	580	582	583	rBV2	1334	446	0.01%	0.003%
11	2.954	592	595	598	rVB3	1700	1204	0.02%	0.008%
12	3.095	636	639	640	rBV3	2133	1221	0.02%	0.009%
13	3.118	645	646	649	rBV3	1732	1027	0.02%	0.007%
14	3.230	679	681	682	rBV2	1033	301	0.01%	0.002%
15	3.314	706	707	708	rBV	1231	383	0.01%	0.003%
16	3.471	753	756	760	rBV6	2242	1728	0.04%	0.012%
17	3.494	760	763	767	rBV6	2031	1976	0.04%	0.014%
18	3.593	789	794	797	rBV6	2549	2631	0.05%	0.018%
19	3.609	797	799	802	rVB4	1208	863	0.02%	0.006%
20	3.661	811	815	817	rBV5	1477	1204	0.02%	0.008%
21	3.796	848	857	881	rBV	50093	138713	2.84%	0.969%
22	4.076	942	944	950	rVB6	1419	1190	0.02%	0.008%
23	4.259	989	1001	1028	rVB	117809	305336	6.25%	2.133%
24	4.532	1083	1086	1089	rBV5	1839	1162	0.02%	0.008%
25	4.629	1114	1116	1117	rBV2	1620	723	0.01%	0.005%
26	4.674	1128	1130	1131	rBV2	1034	464	0.01%	0.003%
27	4.966	1202	1221	1227	rBV2	272298	646823	13.24%	4.518%
28	5.542	1389	1400	1418	rBV	283045	571831	11.70%	3.994%
29	5.998	1530	1542	1559	rBV2	161699	331168	6.78%	2.313%
30	6.240	1614	1617	1620	rBV5	1426	1045	0.02%	0.007%
31	6.478	1688	1691	1694	rBV5	1729	990	0.02%	0.007%
32	6.497	1694	1697	1701	rBV6	1360	1175	0.02%	0.008%
33	6.574	1716	1721	1722	rBV4	1591	1186	0.02%	0.008%
34	6.587	1722	1725	1730	rVV7	1461	1592	0.03%	0.011%
35	6.735	1767	1771	1773	rBV5	1506	1321	0.03%	0.009%
36	6.783	1785	1786	1789	rBV3	1163	593	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041823\
 Data File : VW030648.D
 Acq On : 19 Apr 2023 03:51
 Operator : SY/MD
 Sample : 02398-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1844	rBV2	79823	148016	3.03%	1.034%
38	7.252	1921	1932	1950	rBV	290379	510521	10.45%	3.566%
39	7.561	2016	2028	2042	rBV2	59034	107690	2.20%	0.752%
40	8.034	2165	2175	2202	rBV	159922	313071	6.41%	2.187%
41	8.481	2313	2314	2316	rBV2	1110	494	0.01%	0.003%
42	8.648	2364	2366	2368	rBV3	1454	480	0.01%	0.003%
43	8.722	2386	2389	2391	rBV4	2031	1204	0.02%	0.008%
44	8.821	2400	2420	2447	rBV2	2602302	4886138	100.00%	34.127%
45	9.175	2526	2530	2534	rBV6	2109	2186	0.04%	0.015%
46	9.268	2556	2559	2560	rBV3	2011	1247	0.03%	0.009%
47	9.593	2656	2660	2661	rBV3	2345	1356	0.03%	0.009%
48	9.690	2687	2690	2693	rBV4	1572	1336	0.03%	0.009%
49	10.159	2825	2836	2851	rBV	223290	363205	7.43%	2.537%
50	10.256	2863	2866	2868	rBV4	1467	540	0.01%	0.004%
51	10.378	2902	2904	2907	rBV4	1496	872	0.02%	0.006%
52	10.410	2913	2914	2917	rBV3	1377	590	0.01%	0.004%
53	10.458	2927	2929	2932	rBV4	1512	744	0.02%	0.005%
54	10.651	2986	2989	2990	rBV3	814	444	0.01%	0.003%
55	10.673	2994	2996	2999	rVB4	2176	1045	0.02%	0.007%
56	10.702	3003	3005	3009	rBV5	1352	776	0.02%	0.005%
57	10.725	3010	3012	3015	rBV3	1330	828	0.02%	0.006%
58	10.809	3036	3038	3041	rVB3	1527	882	0.02%	0.006%
59	10.825	3041	3043	3044	rBV2	970	338	0.01%	0.002%
60	10.921	3071	3073	3076	rBV4	1248	853	0.02%	0.006%
61	10.950	3080	3082	3083	rBV2	1194	589	0.01%	0.004%
62	10.995	3092	3096	3100	rBV6	2268	2302	0.05%	0.016%
63	11.053	3112	3114	3115	rBV2	1639	749	0.02%	0.005%
64	11.124	3126	3136	3147	rBV	131072	209811	4.29%	1.465%
65	11.217	3148	3165	3184	rVB2	948933	2097991	42.94%	14.653%
66	11.448	3235	3237	3238	rBV2	1415	484	0.01%	0.003%
67	11.587	3264	3280	3295	rBV2	1176806	2230756	45.65%	15.581%
68	11.915	3380	3382	3384	rBV3	1124	493	0.01%	0.003%
69	12.014	3409	3413	3415	rBV4	1430	1251	0.03%	0.009%
70	12.111	3441	3443	3445	rBV3	2062	1201	0.02%	0.008%
71	12.278	3493	3495	3496	rVB2	1105	318	0.01%	0.002%
72	12.394	3529	3531	3534	rVB3	2010	895	0.02%	0.006%
73	12.458	3549	3551	3552	rBV2	1122	456	0.01%	0.003%
74	12.490	3559	3561	3563	rBV3	1494	572	0.01%	0.004%
75	12.699	3619	3626	3630	rBV7	4220	5384	0.11%	0.038%
76	12.783	3648	3652	3654	rBV5	1982	1488	0.03%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030648.D
 Acq On : 19 Apr 2023 03:51
 Operator : SY/MD
 Sample : 02398-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.821	3662	3664	3667	rBV4	1712	863	0.02%	0.006%
78	12.908	3688	3691	3692	rBV2	1670	733	0.02%	0.005%
79	12.944	3699	3702	3704	rBV4	1814	1351	0.03%	0.009%
80	13.085	3742	3746	3749	rBV5	1358	973	0.02%	0.007%
81	13.207	3772	3784	3800	rBV	479835	729305	14.93%	5.094%
82	13.689	3921	3934	3946	rBV	138614	222339	4.55%	1.553%
83	13.844	3980	3982	3986	rBV6	1386	786	0.02%	0.005%
84	13.950	4011	4015	4018	rBV6	1688	1756	0.04%	0.012%
85	14.162	4079	4081	4083	rVB3	1059	337	0.01%	0.002%
86	14.181	4085	4087	4088	rBV	1545	565	0.01%	0.004%




Sum of corrected areas: 14317465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030648.D
Acq On : 19 Apr 2023 03:51
Operator : SY/MD
Sample : 02398-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

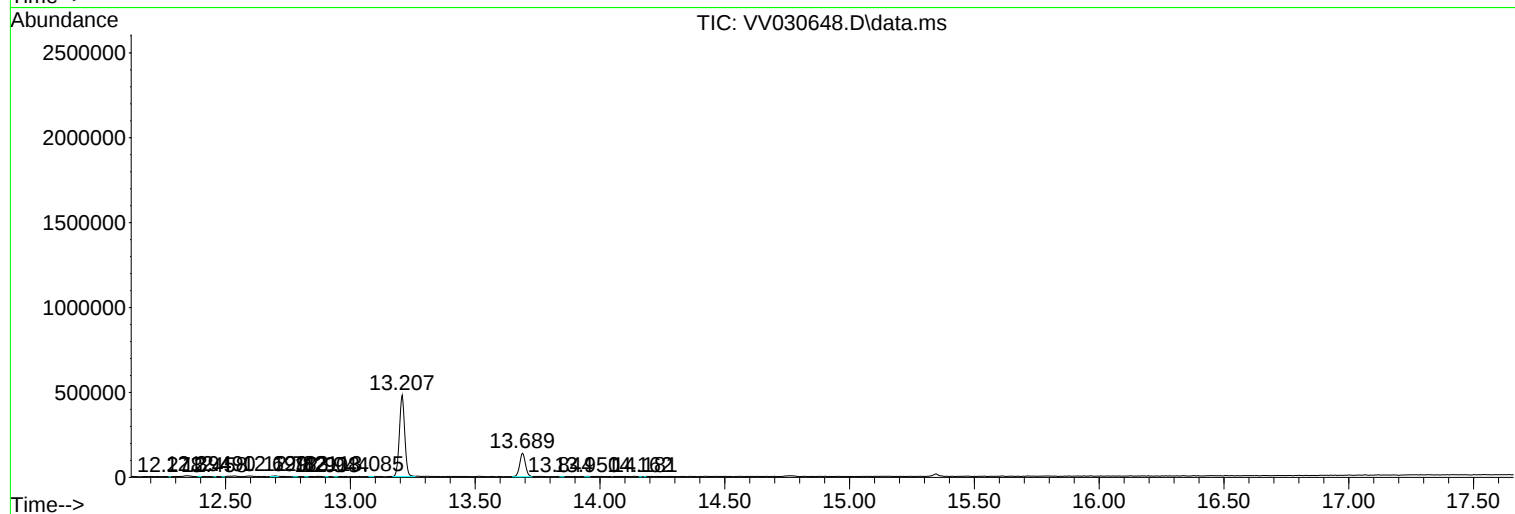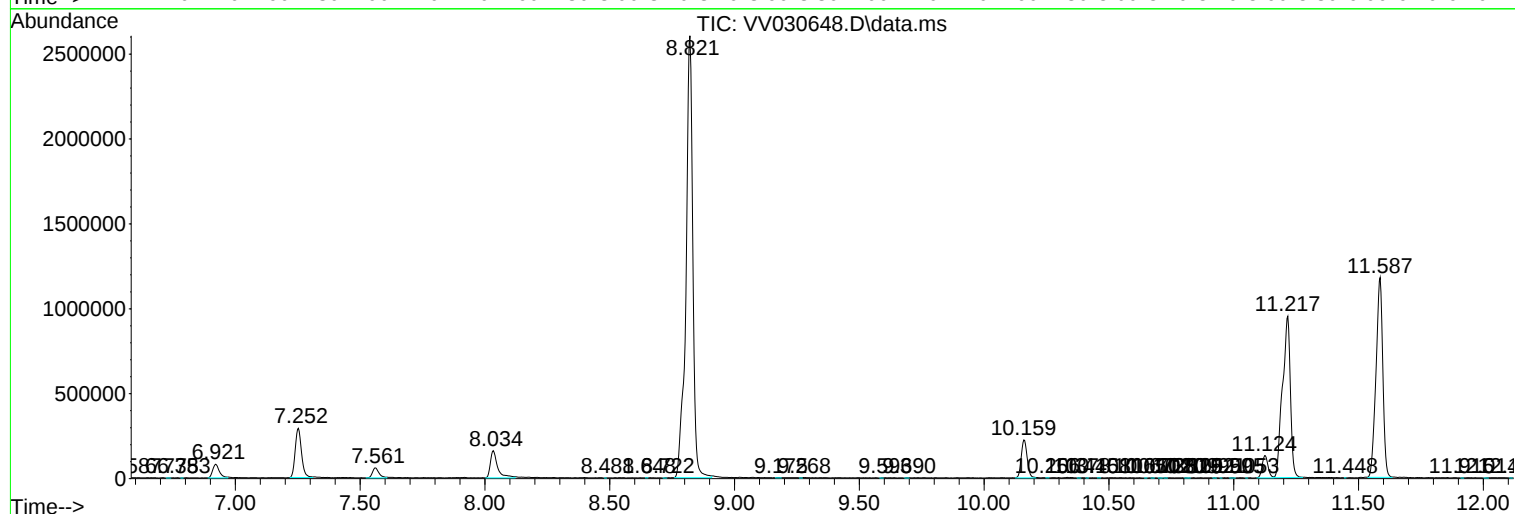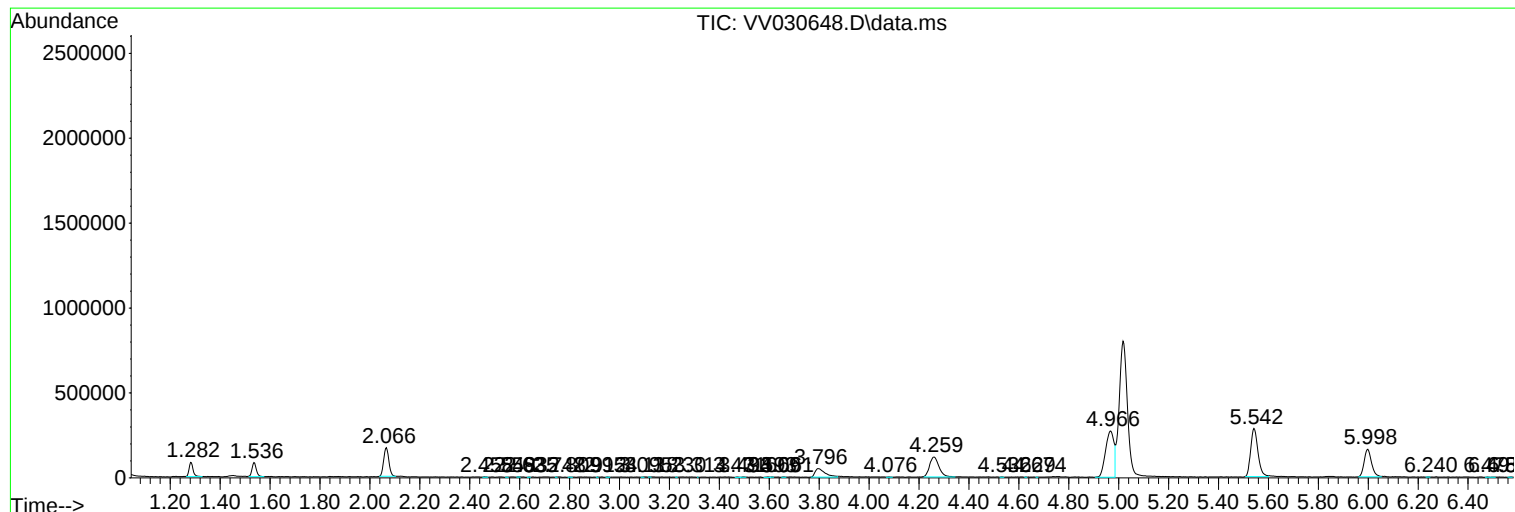

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030648.D
Acq On : 19 Apr 2023 03:51
Operator : SY/MD
Sample : 02398-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
Data File : VV030648.D
Acq On : 19 Apr 2023 03:51
Operator : SY/MD
Sample : 02398-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------