


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041823\
 Data File : VV030610.D
 Acq On : 18 Apr 2023 11:55
 Operator : SY/MD
 Sample : BFB367
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB367

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 18 02:45:56 2023

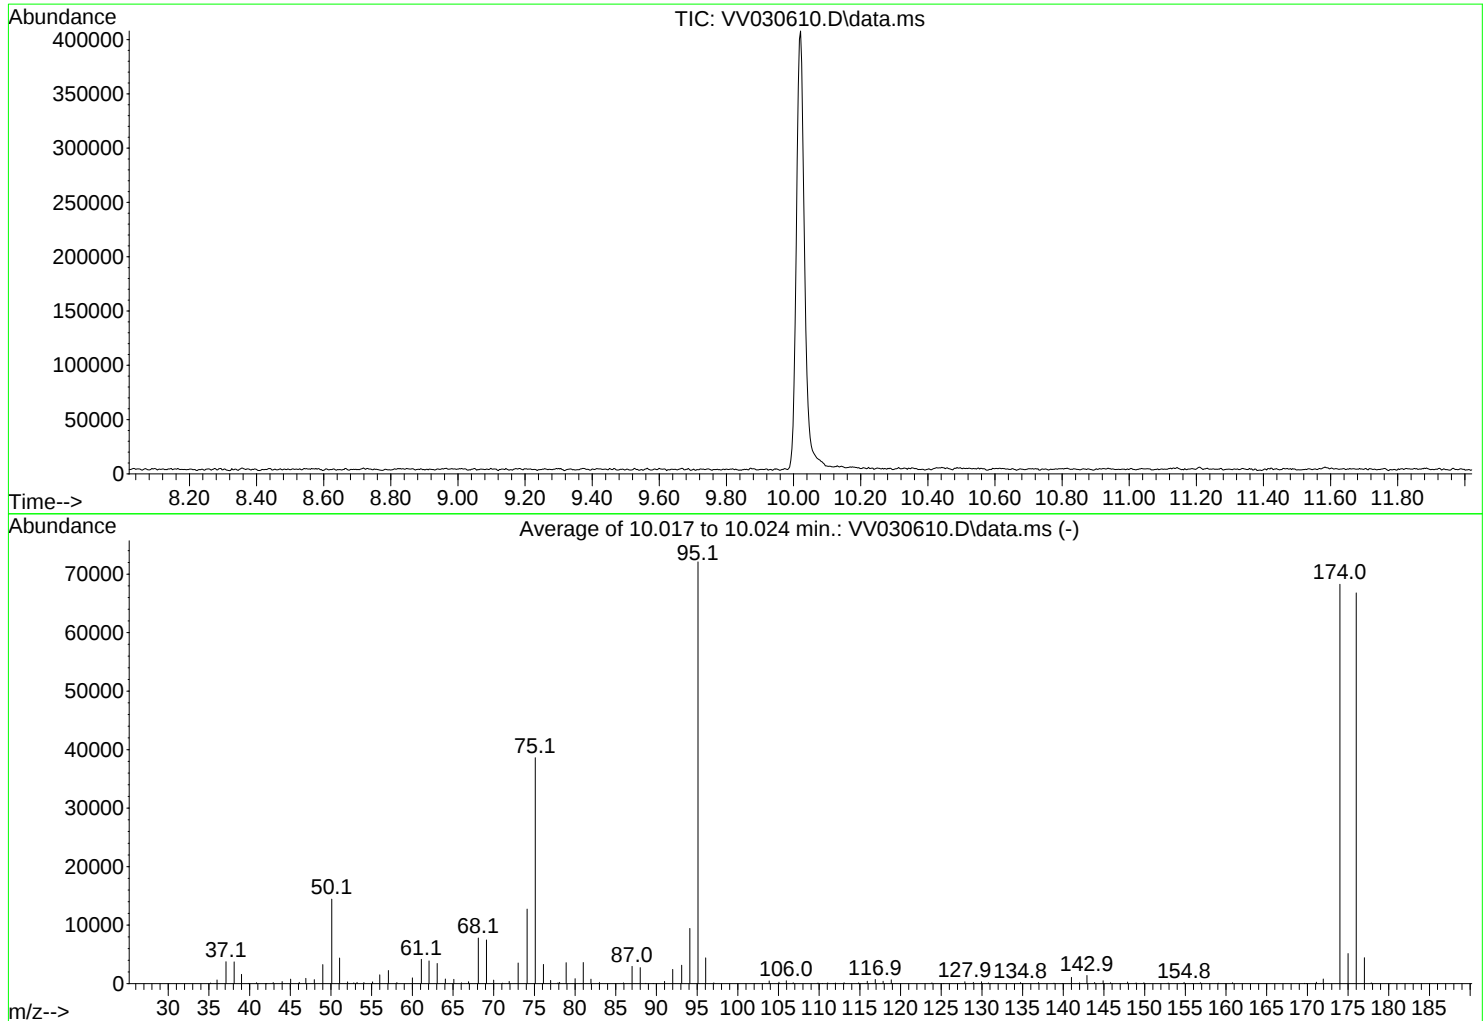

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	14455	PASS
75	95	30	80	53.6	38613	PASS
95	95	100	100	100.0	72104	PASS
96	95	5	9	6.1	4401	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.7	68283	PASS
175	174	5	9	7.5	5137	PASS
176	174	95	105	97.8	66792	PASS
177	176	5	10	6.7	4444	PASS

m/z	Abundance
35.50	106.0
36.00	150.0
36.70	167.0
37.70	105.0
38.60	141.0
39.30	139.0
39.90	235.0
41.50	110.0
42.00	123.0
42.60	138.0
43.20	160.0
44.00	297.0
44.60	183.0
46.40	128.0
47.40	188.0
48.20	132.0
48.60	149.0
49.20	111.0
49.70	110.0
51.00	133.0
52.40	119.0
54.80	118.0
55.40	127.0
57.60	146.0
58.70	149.0
65.80	105.0
69.90	135.0
71.90	145.0
73.00	134.0
121.30	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
35.20	154.0
36.00	783.0
37.10	3966.0
38.10	3771.0
39.00	1580.0
39.90	295.0
40.80	192.0
42.10	134.0
42.90	176.0
44.10	686.0
45.00	789.0
46.10	176.0
46.90	1027.0
47.90	660.0
49.00	3518.0
50.10	14831.0
51.10	4589.0
52.10	334.0
52.80	203.0
53.20	204.0
54.10	211.0
55.10	284.0
56.00	1444.0
57.00	2340.0
58.00	174.0
60.00	1054.0
61.10	4207.0
62.00	4035.0
63.10	3391.0
64.10	828.0
65.10	771.0
66.10	138.0
66.90	371.0
68.10	7977.0
69.10	7586.0
70.00	699.0
71.90	537.0
73.00	3881.0
74.10	13214.0
75.10	39064.0
76.10	3284.0
77.00	515.0
77.90	384.0
78.90	3596.0
80.00	787.0
81.00	3703.0
81.90	749.0
83.10	183.0
85.90	133.0
87.00	3084.0
88.00	2904.0
91.10	394.0
92.00	2549.0
93.10	3093.0
94.10	9537.0
95.10	73000.0
96.10	4625.0
97.00	152.0
103.80	450.0
105.00	243.0
105.90	471.0
106.80	159.0
109.80	113.0
110.40	104.0
111.00	133.0
111.80	107.0
113.10	170.0
114.80	126.0
115.90	405.0
116.90	659.0
117.80	483.0
118.80	685.0
123.90	135.0
125.30	116.0
127.90	368.0
129.00	236.0
129.90	337.0
130.80	134.0
134.70	160.0
136.90	188.0
141.00	1109.0
142.00	126.0
142.90	1445.0
143.80	178.0
144.90	428.0
145.80	164.0
147.90	321.0
149.00	101.0
149.90	154.0
152.90	107.0
154.90	221.0
156.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

159.00	151.0
160.80	171.0
169.90	100.0
171.20	286.0
172.00	675.0
174.00	68664.0
175.00	5033.0
176.00	67016.0
177.00	4471.0
177.90	155.0
180.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
35.20	163.0
36.00	786.0
37.10	3853.0
38.10	3861.0
39.00	1653.0
39.90	277.0
40.90	165.0
42.10	133.0
42.90	201.0
44.10	666.0
45.10	816.0
46.10	232.0
46.90	927.0
48.00	699.0
49.00	3509.0
50.10	15001.0
51.10	4610.0
52.10	283.0
52.80	178.0
53.20	230.0
54.10	182.0
55.10	316.0
56.00	1564.0
57.10	2306.0
58.10	167.0
60.00	987.0
61.10	4299.0
62.00	3987.0
63.00	3533.0
64.00	800.0
65.10	765.0
66.10	155.0
66.90	332.0
68.10	8023.0
69.10	7657.0
70.10	750.0
71.10	106.0
71.90	547.0
73.00	3811.0
74.10	13133.0
75.10	39936.0
76.10	3409.0
77.00	571.0
78.10	324.0
78.90	3688.0
80.00	914.0
81.00	3741.0
82.00	788.0
83.00	217.0
85.90	154.0
87.00	2941.0
88.00	2801.0
91.00	395.0
92.00	2477.0
93.10	3230.0
94.10	9791.0
95.10	74712.0
96.00	4481.0
97.00	134.0
103.90	491.0
105.10	279.0
105.90	487.0
106.80	174.0
109.80	130.0
111.00	139.0
112.00	157.0
113.00	169.0
114.80	123.0
115.90	432.0
116.90	739.0
117.90	412.0
118.80	664.0
123.90	126.0
127.90	345.0
128.90	230.0
130.00	321.0
130.80	136.0
131.10	127.0
134.70	200.0
137.00	177.0
138.80	105.0
141.00	1097.0
142.00	150.0
142.90	1425.0
143.90	198.0
144.90	510.0
145.80	177.0
147.90	291.0
148.90	130.0
149.90	157.0
152.90	114.0
154.80	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

156.80	154.0
159.10	119.0
160.80	185.0
169.60	103.0
171.10	257.0
171.90	811.0
174.00	70216.0
175.00	5286.0
176.00	69040.0
177.00	4593.0
177.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
36.00	785.0
37.10	3471.0
38.10	3568.0
39.00	1509.0
39.90	267.0
40.90	142.0
42.00	115.0
42.90	199.0
44.00	614.0
45.10	719.0
46.10	267.0
46.90	770.0
48.00	712.0
49.00	3107.0
50.10	13534.0
51.10	4291.0
51.90	294.0
53.20	196.0
54.00	177.0
55.10	305.0
56.00	1511.0
57.00	2054.0
58.20	204.0
60.00	875.0
61.10	3940.0
62.10	3651.0
63.00	3394.0
64.00	737.0
65.10	694.0
66.00	161.0
66.90	251.0
68.10	7417.0
69.10	7163.0
70.10	733.0
71.10	110.0
71.90	498.0
73.00	3318.0
74.10	11878.0
75.10	36840.0
76.10	3196.0
77.00	538.0
78.10	301.0
78.90	3454.0
80.00	859.0
81.00	3359.0
82.00	776.0
82.90	220.0
86.00	159.0
87.00	2813.0
88.00	2515.0
88.70	208.0
89.60	100.0
90.90	380.0
92.00	2328.0
93.10	3099.0
94.10	8996.0
95.10	68600.0
96.00	4097.0
97.10	128.0
102.00	104.0
103.90	426.0
105.10	256.0
106.00	520.0
106.80	158.0
109.90	120.0
111.10	131.0
112.00	176.0
113.00	146.0
114.90	143.0
115.90	413.0
116.90	709.0
117.90	362.0
118.90	598.0
123.80	110.0
127.90	304.0
128.90	237.0
130.00	316.0
130.80	120.0
134.80	240.0
137.00	204.0
138.90	115.0
139.90	114.0
141.00	999.0
142.00	157.0
142.90	1286.0
143.90	181.0
144.90	557.0
145.80	178.0
147.00	116.0
147.90	207.0
148.90	143.0
149.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

152.90	114.0
154.80	221.0
155.90	103.0
156.90	164.0
160.80	182.0
169.70	107.0
171.00	228.0
171.90	880.0
174.00	65968.0
175.00	5091.0
176.00	64320.0
177.00	4268.0
177.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367