

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021052.D
 Acq On : 19 Apr 2021 13:49
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	99	rVB	153707	170261	12.93%	1.899%
2	2.346	404	406	410	rBV	227	164	0.01%	0.002%
3	2.458	439	441	444	rBB2	356	176	0.01%	0.002%
4	2.481	445	448	450	rBV	357	218	0.02%	0.002%
5	2.510	450	457	458	rBV4	3145	3056	0.23%	0.034%
6	2.597	481	484	486	rBB	281	171	0.01%	0.002%
7	2.625	489	493	496	rBV	347	216	0.02%	0.002%
8	2.706	515	518	521	rBB	287	182	0.01%	0.002%
9	2.770	535	538	539	rBV	444	227	0.02%	0.003%
10	2.818	551	553	557	rBB2	312	230	0.02%	0.003%
11	2.851	558	563	564	rBB	347	198	0.02%	0.002%
12	2.870	565	569	573	rBB2	280	230	0.02%	0.003%
13	2.950	590	594	599	rBB	454	346	0.03%	0.004%
14	2.982	600	604	608	rBB2	444	383	0.03%	0.004%
15	3.117	643	646	649	rBB2	343	219	0.02%	0.002%
16	3.867	877	879	881	rBV	274	163	0.01%	0.002%
17	4.539	1085	1088	1090	rBV	427	266	0.02%	0.003%
18	4.703	1137	1139	1142	rBB	285	157	0.01%	0.002%
19	4.764	1156	1158	1161	rVB3	443	306	0.02%	0.003%
20	4.834	1178	1180	1184	rBB	260	184	0.01%	0.002%
21	4.873	1190	1192	1193	rBV	423	181	0.01%	0.002%
22	4.924	1206	1208	1212	rBB	266	180	0.01%	0.002%
23	4.960	1217	1219	1222	rBB	349	157	0.01%	0.002%
24	5.050	1230	1247	1277	rBV4	505561	1316676	100.00%	14.687%
25	5.423	1358	1363	1366	rBV3	553	433	0.03%	0.005%
26	5.516	1388	1392	1393	rBV	302	167	0.01%	0.002%
27	5.526	1393	1395	1398	rBV	307	165	0.01%	0.002%
28	5.555	1401	1404	1406	rBV2	464	293	0.02%	0.003%
29	5.619	1412	1424	1445	rBV	439916	879235	66.78%	9.807%
30	5.915	1507	1516	1521	rBV6	3080	4859	0.37%	0.054%
31	6.014	1543	1547	1550	rBV	415	269	0.02%	0.003%
32	6.072	1551	1565	1584	rBV	280669	560324	42.56%	6.250%
33	6.204	1604	1606	1608	rBV3	589	180	0.01%	0.002%
34	6.284	1629	1631	1634	rBB2	401	218	0.02%	0.002%
35	6.342	1646	1649	1651	rBB2	606	262	0.02%	0.003%
36	6.381	1659	1661	1662	rBV	399	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021052.D
 Acq On : 19 Apr 2021 13:49
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.416	1670	1672	1676	rBB	273	172	0.01%	0.002%
38	6.529	1704	1707	1709	rBV	396	188	0.01%	0.002%
39	6.551	1712	1714	1718	rBV2	330	280	0.02%	0.003%
40	6.802	1789	1792	1795	rBB2	383	220	0.02%	0.002%
41	6.854	1806	1808	1810	rBB	315	165	0.01%	0.002%
42	6.908	1821	1825	1827	rBB	321	178	0.01%	0.002%
43	6.989	1838	1850	1874	rBV	168487	314292	23.87%	3.506%
44	7.207	1916	1918	1922	rVB3	457	218	0.02%	0.002%
45	7.317	1940	1952	1970	rBV	638891	1109763	84.29%	12.379%
46	7.625	2038	2048	2069	rBV	122734	216384	16.43%	2.414%
47	7.847	2115	2117	2120	rVB	454	225	0.02%	0.003%
48	7.985	2150	2160	2164	rBV2	1312	1731	0.13%	0.019%
49	8.050	2177	2180	2183	rBV2	637	385	0.03%	0.004%
50	8.091	2183	2193	2223	rBV	258698	477133	36.24%	5.322%
51	8.378	2278	2282	2288	rBB3	685	655	0.05%	0.007%
52	8.407	2289	2291	2293	rBV	335	180	0.01%	0.002%
53	8.442	2300	2302	2304	rBB	385	163	0.01%	0.002%
54	8.458	2304	2307	2311	rBV2	405	331	0.03%	0.004%
55	8.587	2344	2347	2349	rBV2	485	278	0.02%	0.003%
56	8.603	2350	2352	2355	rVV3	384	252	0.02%	0.003%
57	8.651	2364	2367	2370	rBV	414	290	0.02%	0.003%
58	8.712	2384	2386	2389	rBB	278	165	0.01%	0.002%
59	8.757	2397	2400	2404	rBB	252	227	0.02%	0.003%
60	8.857	2419	2431	2457	rBV	655517	1075490	81.68%	11.997%
61	9.024	2480	2483	2486	rBV2	566	436	0.03%	0.005%
62	9.101	2505	2507	2508	rBV2	403	199	0.02%	0.002%
63	9.127	2514	2515	2518	rBV	425	177	0.01%	0.002%
64	9.149	2518	2522	2525	rBV2	848	701	0.05%	0.008%
65	9.304	2565	2570	2573	rBB	531	383	0.03%	0.004%
66	9.368	2587	2590	2593	rBV	244	217	0.02%	0.002%
67	9.403	2598	2601	2604	rBV	297	258	0.02%	0.003%
68	9.554	2645	2648	2650	rBV	427	323	0.02%	0.004%
69	9.728	2697	2702	2707	rBB	335	279	0.02%	0.003%
70	9.763	2709	2713	2715	rBV2	455	328	0.02%	0.004%
71	9.808	2724	2727	2729	rBV	292	197	0.01%	0.002%
72	10.175	2836	2841	2844	rBB2	362	330	0.03%	0.004%
73	10.220	2844	2855	2875	rBV	420089	657708	49.95%	7.336%
74	10.419	2914	2917	2921	rBV2	255	168	0.01%	0.002%
75	10.468	2930	2932	2935	rVB	348	189	0.01%	0.002%
76	10.497	2935	2941	2943	rBV	410	372	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021052.D
 Acq On : 19 Apr 2021 13:49
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.754	3018	3021	3024	rBV	253	207	0.02%	0.002%
78	10.812	3037	3039	3041	rBV	365	168	0.01%	0.002%
79	10.889	3059	3063	3065	rBV	566	416	0.03%	0.005%
80	10.998	3094	3097	3099	rBV	335	235	0.02%	0.003%
81	11.082	3117	3123	3127	rBB	518	528	0.04%	0.006%
82	11.104	3127	3130	3132	rBV	311	205	0.02%	0.002%
83	11.255	3165	3177	3197	rBV	679549	1065874	80.95%	11.889%
84	11.500	3250	3253	3256	rBV	345	197	0.01%	0.002%
85	11.532	3258	3263	3268	rBB2	514	428	0.03%	0.005%
86	11.583	3274	3279	3280	rBV	472	402	0.03%	0.004%
87	11.632	3282	3294	3313	rBV	688102	1085431	82.44%	12.107%
88	11.908	3377	3380	3382	rBV2	256	170	0.01%	0.002%
89	12.101	3435	3440	3442	rBV3	693	638	0.05%	0.007%
90	12.168	3456	3461	3464	rBV	380	368	0.03%	0.004%
91	12.230	3478	3480	3482	rBV	569	377	0.03%	0.004%
92	12.455	3549	3550	3553	rBV	532	304	0.02%	0.003%
93	12.532	3571	3574	3575	rBV	467	243	0.02%	0.003%
94	12.593	3590	3593	3595	rBV	497	240	0.02%	0.003%
95	12.757	3642	3644	3648	rBV	497	295	0.02%	0.003%
96	12.857	3673	3675	3677	rBV	429	207	0.02%	0.002%
97	13.130	3758	3760	3762	rBV2	569	284	0.02%	0.003%
98	13.271	3799	3804	3815	rBV5	3019	4240	0.32%	0.047%
99	13.390	3838	3841	3842	rBV	464	214	0.02%	0.002%
100	13.815	3969	3973	3976	rBV2	535	549	0.04%	0.006%




Sum of corrected areas: 8964993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021052.D
Acq On : 19 Apr 2021 13:49
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

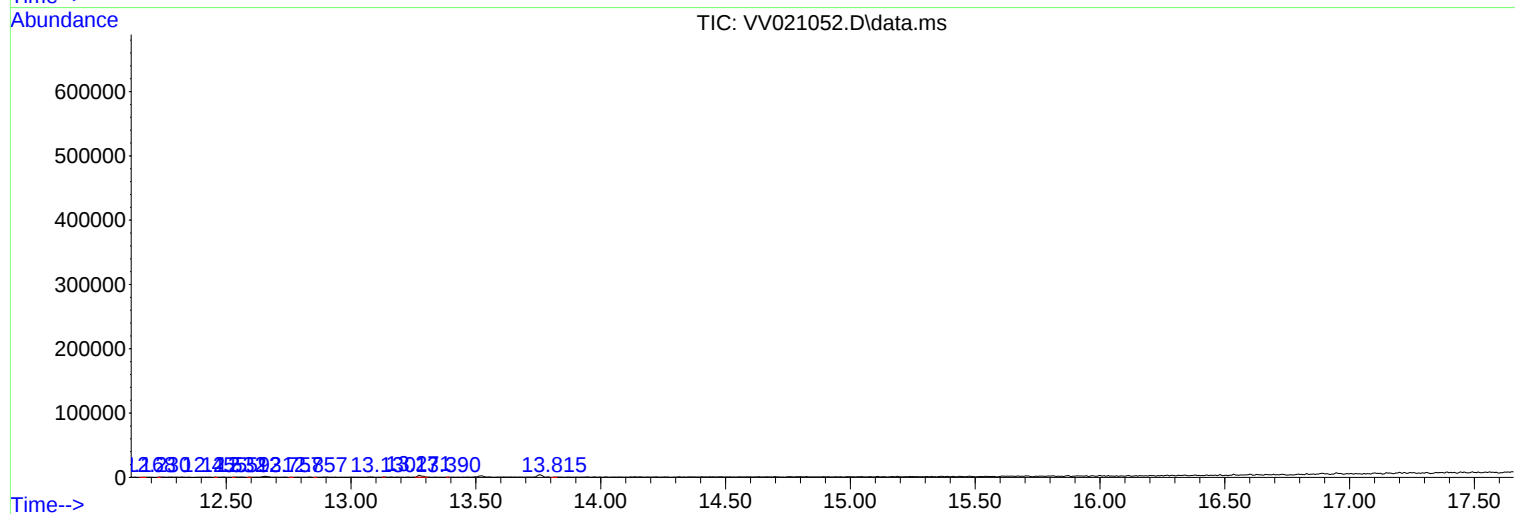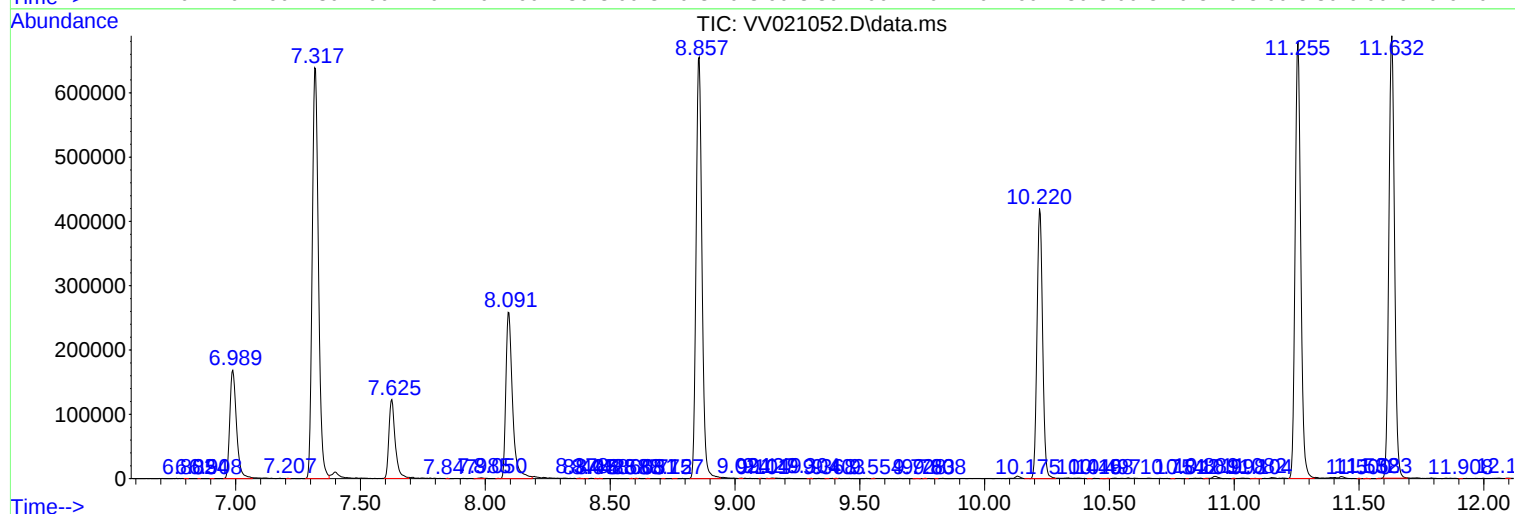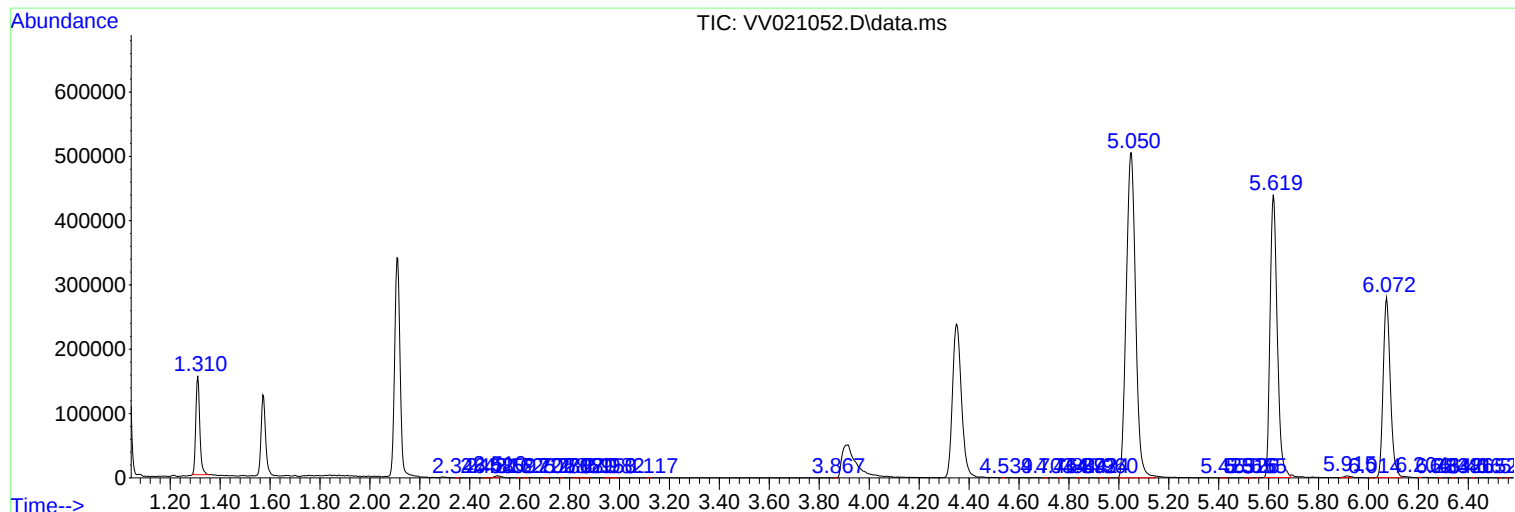

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021052.D
Acq On : 19 Apr 2021 13:49
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021052.D
Acq On : 19 Apr 2021 13:49
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
