

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021053.D
 Acq On : 19 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2031-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	98	rVB	170741	181933	13.05%	1.840%
2	2.111	324	333	347	rBV	357633	508404	36.48%	5.143%
3	2.298	386	391	395	rBV2	974	1004	0.07%	0.010%
4	2.404	420	424	427	rBB	162	156	0.01%	0.002%
5	2.481	442	448	451	rBV2	463	518	0.04%	0.005%
6	2.696	513	515	517	rBB	528	228	0.02%	0.002%
7	2.722	520	523	524	rBV	326	157	0.01%	0.002%
8	2.796	541	546	549	rBB2	278	288	0.02%	0.003%
9	2.883	570	573	576	rBB	253	182	0.01%	0.002%
10	3.124	644	648	650	rBV2	305	239	0.02%	0.002%
11	3.343	714	716	719	rBV	286	196	0.01%	0.002%
12	3.413	734	738	742	rBB3	271	274	0.02%	0.003%
13	3.580	787	790	793	rBB2	290	191	0.01%	0.002%
14	3.908	881	892	930	rBV	51873	202130	14.50%	2.045%
15	4.600	1105	1107	1110	rBV	481	218	0.02%	0.002%
16	4.635	1114	1118	1121	rBV	269	281	0.02%	0.003%
17	4.664	1125	1127	1129	rBV2	643	366	0.03%	0.004%
18	4.696	1135	1137	1141	rBV2	346	253	0.02%	0.003%
19	4.812	1171	1173	1175	rBV	340	169	0.01%	0.002%
20	5.050	1229	1247	1284	rBV2	533458	1393757	100.00%	14.099%
21	5.339	1335	1337	1341	rBV2	471	316	0.02%	0.003%
22	5.426	1361	1364	1368	rBV3	461	384	0.03%	0.004%
23	5.551	1400	1403	1404	rBB3	323	169	0.01%	0.002%
24	5.622	1412	1425	1462	rBV	412040	839326	60.22%	8.490%
25	6.072	1553	1565	1592	rVV	285198	590648	42.38%	5.975%
26	6.301	1632	1636	1641	rBB2	420	366	0.03%	0.004%
27	6.323	1641	1643	1645	rBB	346	173	0.01%	0.002%
28	6.381	1659	1661	1663	rVB	501	170	0.01%	0.002%
29	6.471	1685	1689	1694	rBB	270	226	0.02%	0.002%
30	6.497	1694	1697	1699	rBB2	415	255	0.02%	0.003%
31	6.526	1702	1706	1707	rBV	210	151	0.01%	0.002%
32	6.587	1721	1725	1727	rBV	218	190	0.01%	0.002%
33	6.751	1774	1776	1781	rBB	236	212	0.02%	0.002%
34	6.844	1801	1805	1809	rBV2	389	367	0.03%	0.004%
35	6.989	1838	1850	1881	rBV	181963	334880	24.03%	3.388%
36	7.217	1919	1921	1922	rBV	494	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041921\
 Data File : VW021053.D
 Acq On : 19 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2031-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	7.249	1929	1931	1933	rBV	427	214	0.02%	0.002%
38	7.320	1936	1953	1970	rBV	677430	1171502	84.05%	11.851%
39	7.625	2038	2048	2070	rBV2	130863	229260	16.45%	2.319%
40	7.860	2119	2121	2122	rBV	435	155	0.01%	0.002%
41	7.902	2132	2134	2137	rBV2	303	192	0.01%	0.002%
42	8.030	2171	2174	2176	rBB	269	157	0.01%	0.002%
43	8.050	2177	2180	2182	rBV2	538	343	0.02%	0.003%
44	8.095	2184	2194	2226	rVV	277655	513844	36.87%	5.198%
45	8.439	2297	2301	2303	rBV3	561	419	0.03%	0.004%
46	8.487	2313	2316	2319	rBV2	613	488	0.04%	0.005%
47	8.548	2333	2335	2338	rBV	485	267	0.02%	0.003%
48	8.580	2343	2345	2352	rVB2	444	300	0.02%	0.003%
49	8.673	2367	2374	2376	rBV2	455	392	0.03%	0.004%
50	8.706	2383	2384	2388	rBB	468	218	0.02%	0.002%
51	8.747	2394	2397	2400	rBB	249	161	0.01%	0.002%
52	8.857	2419	2431	2455	rBV	634493	1017191	72.98%	10.290%
53	9.243	2548	2551	2553	rBV	192	151	0.01%	0.002%
54	9.252	2553	2554	2559	rVB2	366	249	0.02%	0.003%
55	9.394	2595	2598	2600	rBB2	296	160	0.01%	0.002%
56	9.407	2600	2602	2604	rBV	232	154	0.01%	0.002%
57	9.468	2616	2621	2625	rBB2	304	247	0.02%	0.002%
58	9.522	2635	2638	2641	rBV2	358	279	0.02%	0.003%
59	9.545	2642	2645	2648	rVB2	514	250	0.02%	0.003%
60	9.564	2648	2651	2654	rBB	357	190	0.01%	0.002%
61	9.583	2654	2657	2660	rBB	399	296	0.02%	0.003%
62	9.628	2666	2671	2674	rBB2	540	407	0.03%	0.004%
63	9.657	2678	2680	2682	rBV	300	172	0.01%	0.002%
64	9.686	2686	2689	2691	rBV2	428	207	0.01%	0.002%
65	9.731	2701	2703	2705	rBV	297	154	0.01%	0.002%
66	9.747	2705	2708	2711	rVV	350	184	0.01%	0.002%
67	9.786	2718	2720	2722	rBV	416	166	0.01%	0.002%
68	9.940	2765	2768	2770	rBB	349	211	0.02%	0.002%
69	9.956	2771	2773	2776	rBV	235	176	0.01%	0.002%
70	10.001	2785	2787	2792	rVB2	292	205	0.01%	0.002%
71	10.050	2798	2802	2803	rBV	335	171	0.01%	0.002%
72	10.095	2814	2816	2820	rBB2	495	294	0.02%	0.003%
73	10.133	2821	2828	2836	rBV6	3812	5530	0.40%	0.056%
74	10.220	2844	2855	2869	rBV	447916	700052	50.23%	7.082%
75	10.313	2879	2884	2886	rBV3	1121	888	0.06%	0.009%
76	10.362	2895	2899	2902	rBV4	669	605	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021053.D
 Acq On : 19 Apr 2021 14:15
 Operator : SY/MD
 Sample : M2031-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.419	2911	2917	2919	rBB	457	306	0.02%	0.003%
78	10.435	2919	2922	2926	rBV2	459	406	0.03%	0.004%
79	10.468	2930	2932	2936	rVB	274	201	0.01%	0.002%
80	10.493	2937	2940	2941	rBV	309	164	0.01%	0.002%
81	10.554	2955	2959	2961	rBV	563	403	0.03%	0.004%
82	10.677	2994	2997	2999	rBV2	695	407	0.03%	0.004%
83	10.702	3002	3005	3008	rVV	255	191	0.01%	0.002%
84	10.783	3028	3030	3031	rBV	412	194	0.01%	0.002%
85	10.831	3043	3045	3047	rVB2	484	205	0.01%	0.002%
86	10.844	3047	3049	3050	rBV2	524	193	0.01%	0.002%
87	11.127	3130	3137	3139	rBV2	636	601	0.04%	0.006%
88	11.181	3151	3154	3159	rBV	434	394	0.03%	0.004%
89	11.255	3164	3177	3201	rBV	653408	1012618	72.65%	10.243%
90	11.551	3265	3269	3270	rBV	307	239	0.02%	0.002%
91	11.632	3280	3294	3318	rBV	749924	1160468	83.26%	11.739%
92	11.860	3361	3365	3367	rBV2	327	198	0.01%	0.002%
93	11.908	3376	3380	3383	rBB	272	177	0.01%	0.002%
94	11.927	3383	3386	3389	rBV	431	328	0.02%	0.003%
95	12.217	3472	3476	3479	rBV	519	452	0.03%	0.005%
96	12.821	3659	3664	3666	rBV	441	451	0.03%	0.005%
97	12.956	3704	3706	3708	rBV	524	295	0.02%	0.003%
98	13.059	3736	3738	3740	rBV2	412	254	0.02%	0.003%
99	13.249	3795	3797	3799	rBV2	681	332	0.02%	0.003%
100	13.818	3968	3974	3979	rBV3	464	552	0.04%	0.006%




Sum of corrected areas: 9885502

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021053.D
Acq On : 19 Apr 2021 14:15
Operator : SY/MD
Sample : M2031-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

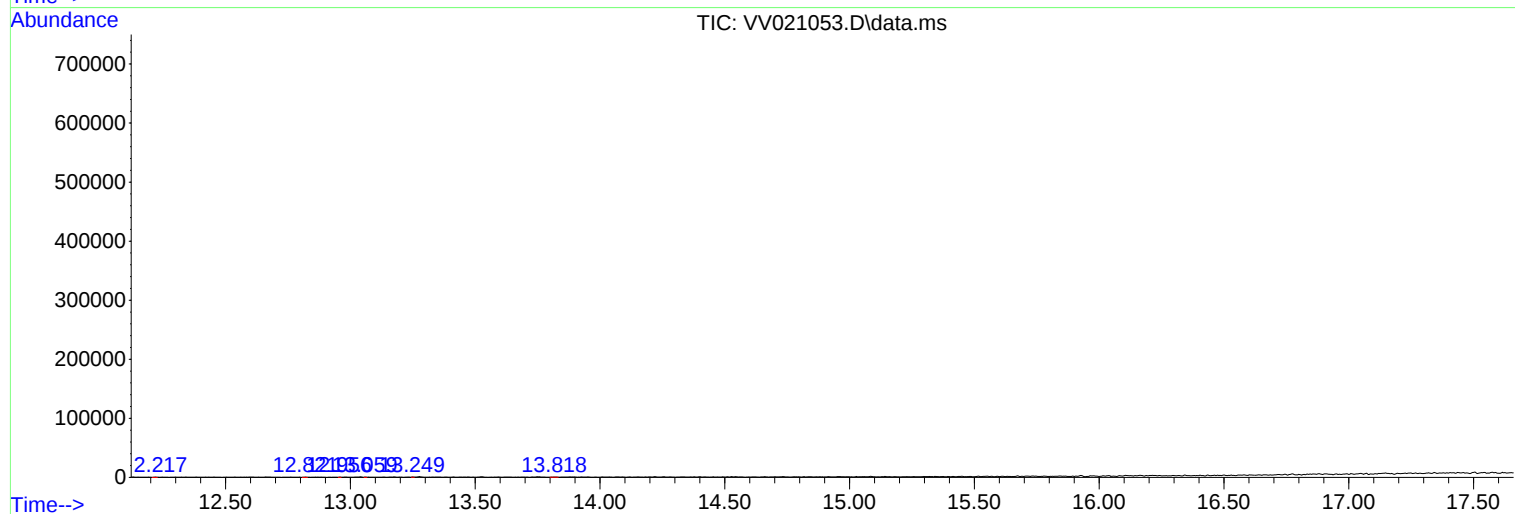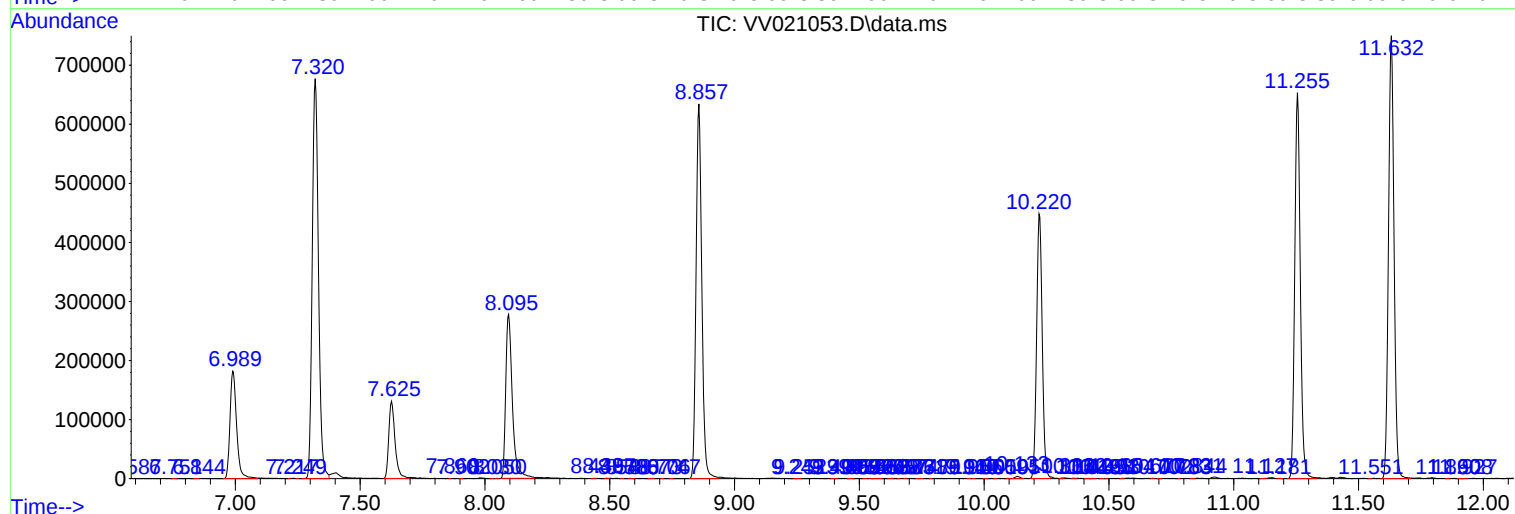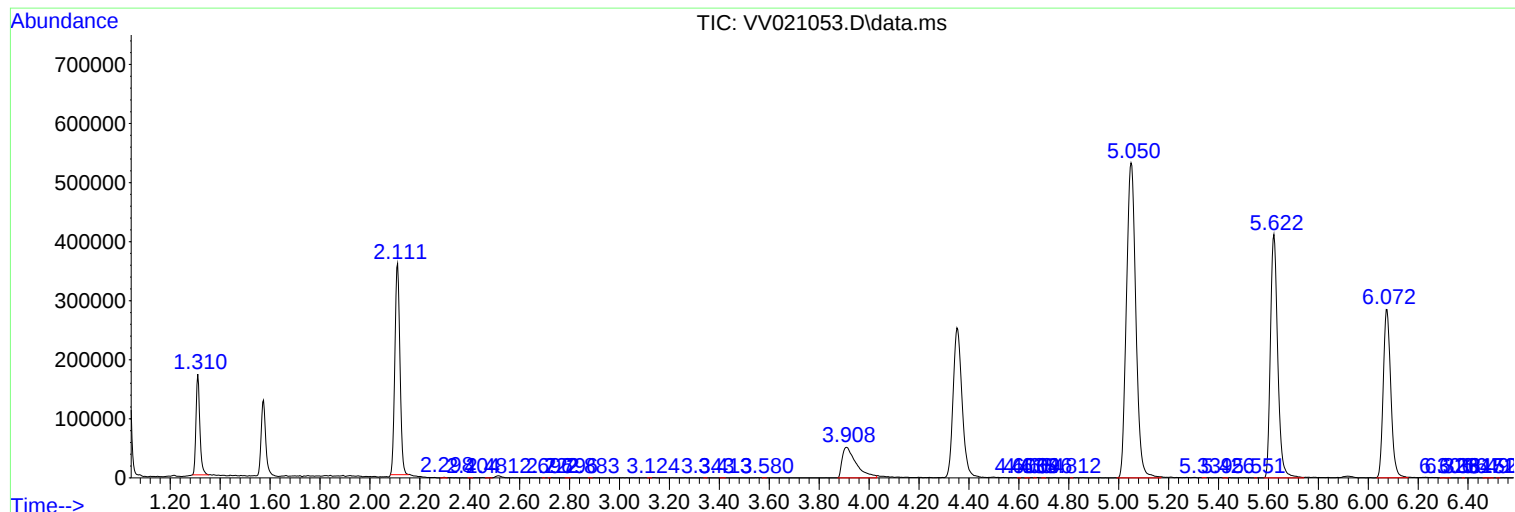

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021053.D
Acq On : 19 Apr 2021 14:15
Operator : SY/MD
Sample : M2031-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021053.D
Acq On : 19 Apr 2021 14:15
Operator : SY/MD
Sample : M2031-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
