

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021054.D
 Acq On : 19 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2067-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.372	413	414	421	rVB2	317	241	0.02%	0.003%
2	2.446	432	437	441	rBV2	366	368	0.03%	0.004%
3	2.474	444	446	449	rBV	360	248	0.02%	0.003%
4	2.513	453	458	459	rBV	876	775	0.07%	0.009%
5	2.552	466	470	473	rBB2	509	395	0.03%	0.004%
6	2.616	487	490	492	rBV2	572	438	0.04%	0.005%
7	2.671	504	507	509	rBB	342	169	0.01%	0.002%
8	2.703	512	517	519	rBV	443	371	0.03%	0.004%
9	2.812	550	551	555	rBV	225	150	0.01%	0.002%
10	2.886	572	574	578	rBB	264	184	0.02%	0.002%
11	2.944	589	592	594	rBV2	422	267	0.02%	0.003%
12	3.227	678	680	682	rBB	378	140	0.01%	0.002%
13	3.375	724	726	729	rBB	323	160	0.01%	0.002%
14	3.645	808	810	812	rBV	304	155	0.01%	0.002%
15	3.751	839	843	845	rBV	515	452	0.04%	0.005%
16	3.905	881	891	916	rBV	55123	186285	16.01%	2.100%
17	4.355	1015	1031	1062	rBV	210842	535835	46.06%	6.040%
18	4.558	1091	1094	1097	rBV	377	332	0.03%	0.004%
19	4.593	1103	1105	1106	rBV	386	173	0.01%	0.002%
20	4.638	1117	1119	1123	rVB2	527	238	0.02%	0.003%
21	4.764	1153	1158	1160	rBB2	334	266	0.02%	0.003%
22	4.777	1160	1162	1164	rBB	337	132	0.01%	0.001%
23	4.835	1178	1180	1182	rBB	300	148	0.01%	0.002%
24	4.957	1214	1218	1223	rBB	319	282	0.02%	0.003%
25	5.053	1230	1248	1274	rBV3	446990	1163247	100.00%	13.113%
26	5.336	1332	1336	1337	rBV	442	323	0.03%	0.004%
27	5.400	1350	1356	1358	rBV2	512	399	0.03%	0.004%
28	5.410	1358	1359	1361	rBV2	331	129	0.01%	0.001%
29	5.474	1374	1379	1380	rBV	317	175	0.02%	0.002%
30	5.519	1387	1393	1395	rBV2	539	492	0.04%	0.006%
31	5.555	1400	1404	1406	rBB	285	186	0.02%	0.002%
32	5.622	1412	1425	1457	rBV	426947	857723	73.74%	9.669%
33	5.918	1509	1517	1530	rVV9	2577	5319	0.46%	0.060%
34	5.970	1530	1533	1537	rVB2	523	278	0.02%	0.003%
35	6.076	1552	1566	1587	rBV	256610	515558	44.32%	5.812%
36	6.388	1661	1663	1664	rBV	318	156	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041921\
 Data File : VW021054.D
 Acq On : 19 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2067-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.484	1689	1693	1697	rBB	282	246	0.02%	0.003%
38	6.539	1705	1710	1713	rBB2	509	415	0.04%	0.005%
39	6.580	1721	1723	1728	rBV	288	226	0.02%	0.003%
40	6.725	1765	1768	1771	rBB	387	233	0.02%	0.003%
41	6.857	1806	1809	1814	rVB	397	323	0.03%	0.004%
42	6.937	1831	1834	1835	rBB	343	137	0.01%	0.002%
43	6.989	1840	1850	1875	rBV	150330	282313	24.27%	3.182%
44	7.162	1903	1904	1913	rVB3	635	613	0.05%	0.007%
45	7.201	1913	1916	1920	rBB	677	398	0.03%	0.004%
46	7.227	1921	1924	1926	rBV	411	250	0.02%	0.003%
47	7.320	1942	1953	1974	rBV	543452	943019	81.07%	10.630%
48	7.625	2037	2048	2074	rBV	110420	200041	17.20%	2.255%
49	7.815	2102	2107	2111	rBV3	497	396	0.03%	0.004%
50	7.847	2114	2117	2122	rBV2	270	233	0.02%	0.003%
51	7.899	2131	2133	2134	rBB2	460	162	0.01%	0.002%
52	7.941	2138	2146	2147	rBV3	2944	3070	0.26%	0.035%
53	8.095	2184	2194	2217	rBV	270345	484906	41.69%	5.466%
54	8.346	2270	2272	2274	rBV	265	142	0.01%	0.002%
55	8.368	2276	2279	2280	rBV	401	236	0.02%	0.003%
56	8.587	2342	2347	2352	rBV2	358	394	0.03%	0.004%
57	8.674	2369	2374	2377	rBV	478	416	0.04%	0.005%
58	8.773	2402	2405	2406	rBV	427	218	0.02%	0.002%
59	8.815	2416	2418	2419	rBV	471	209	0.02%	0.002%
60	8.857	2420	2431	2461	rVV	652116	1052974	90.52%	11.870%
61	9.149	2519	2522	2524	rBV2	791	616	0.05%	0.007%
62	9.243	2549	2551	2555	rBB	516	208	0.02%	0.002%
63	9.265	2555	2558	2562	rBB	570	349	0.03%	0.004%
64	9.291	2563	2566	2568	rBV	279	133	0.01%	0.001%
65	9.368	2588	2590	2593	rBV2	580	403	0.03%	0.005%
66	9.416	2599	2605	2610	rBV3	435	525	0.05%	0.006%
67	9.461	2614	2619	2621	rBV	287	324	0.03%	0.004%
68	9.493	2626	2629	2630	rBV	300	190	0.02%	0.002%
69	9.555	2644	2648	2653	rBB3	434	475	0.04%	0.005%
70	9.593	2656	2660	2661	rBV3	224	162	0.01%	0.002%
71	9.725	2698	2701	2702	rBV	303	178	0.02%	0.002%
72	9.809	2724	2727	2730	rBV2	413	328	0.03%	0.004%
73	9.895	2751	2754	2758	rBB	366	236	0.02%	0.003%
74	9.934	2759	2766	2769	rBV3	492	554	0.05%	0.006%
75	10.011	2788	2790	2792	rBV	356	162	0.01%	0.002%
76	10.072	2803	2809	2813	rBB	188	265	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021054.D
 Acq On : 19 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2067-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.108	2816	2820	2822	rBV	590	355	0.03%	0.004%
78	10.220	2844	2855	2876	rBV	409766	648346	55.74%	7.308%
79	10.307	2880	2882	2885	rBV2	364	178	0.02%	0.002%
80	10.465	2930	2931	2939	rVB2	558	443	0.04%	0.005%
81	10.513	2944	2946	2948	rBV	372	226	0.02%	0.003%
82	10.548	2956	2957	2959	rBV	467	154	0.01%	0.002%
83	10.635	2981	2984	2987	rBV2	487	333	0.03%	0.004%
84	10.818	3036	3041	3045	rBV	404	430	0.04%	0.005%
85	10.921	3069	3073	3077	rBV5	2270	2398	0.21%	0.027%
86	11.008	3097	3100	3101	rBV	508	279	0.02%	0.003%
87	11.104	3125	3130	3133	rBV	365	356	0.03%	0.004%
88	11.182	3152	3154	3156	rVB	422	128	0.01%	0.001%
89	11.201	3156	3160	3162	rBV2	801	522	0.04%	0.006%
90	11.255	3165	3177	3195	rBV	638630	980338	84.28%	11.051%
91	11.632	3282	3294	3316	rBV	625528	984519	84.64%	11.098%
92	11.789	3337	3343	3345	rBV3	767	655	0.06%	0.007%
93	11.873	3365	3369	3376	rVB2	424	525	0.05%	0.006%
94	11.927	3382	3386	3392	rBV	646	545	0.05%	0.006%
95	12.140	3449	3452	3455	rBV	306	226	0.02%	0.003%
96	12.654	3610	3612	3613	rBV	377	165	0.01%	0.002%
97	12.918	3691	3694	3697	rBV	358	316	0.03%	0.004%
98	12.976	3710	3712	3716	rVB2	364	221	0.02%	0.002%
99	12.998	3716	3719	3723	rVB2	527	382	0.03%	0.004%
100	13.024	3724	3727	3728	rBV	361	221	0.02%	0.002%




Sum of corrected areas: 8871128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021054.D
Acq On : 19 Apr 2021 14:38
Operator : SY/MD
Sample : M2067-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG592

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

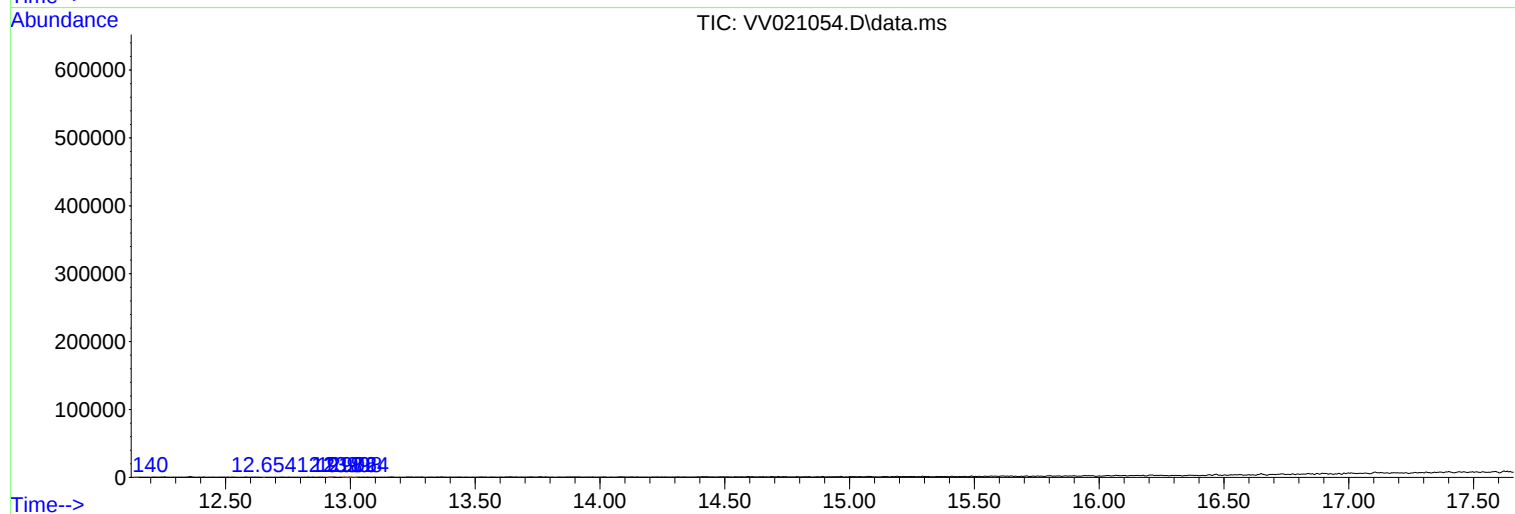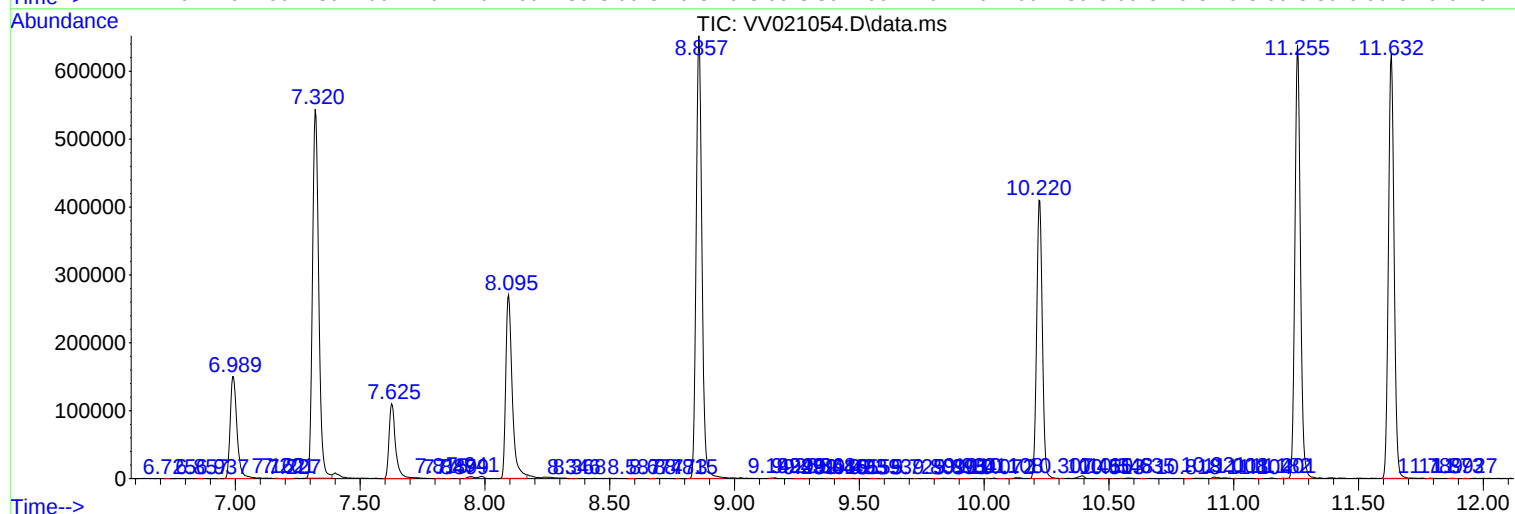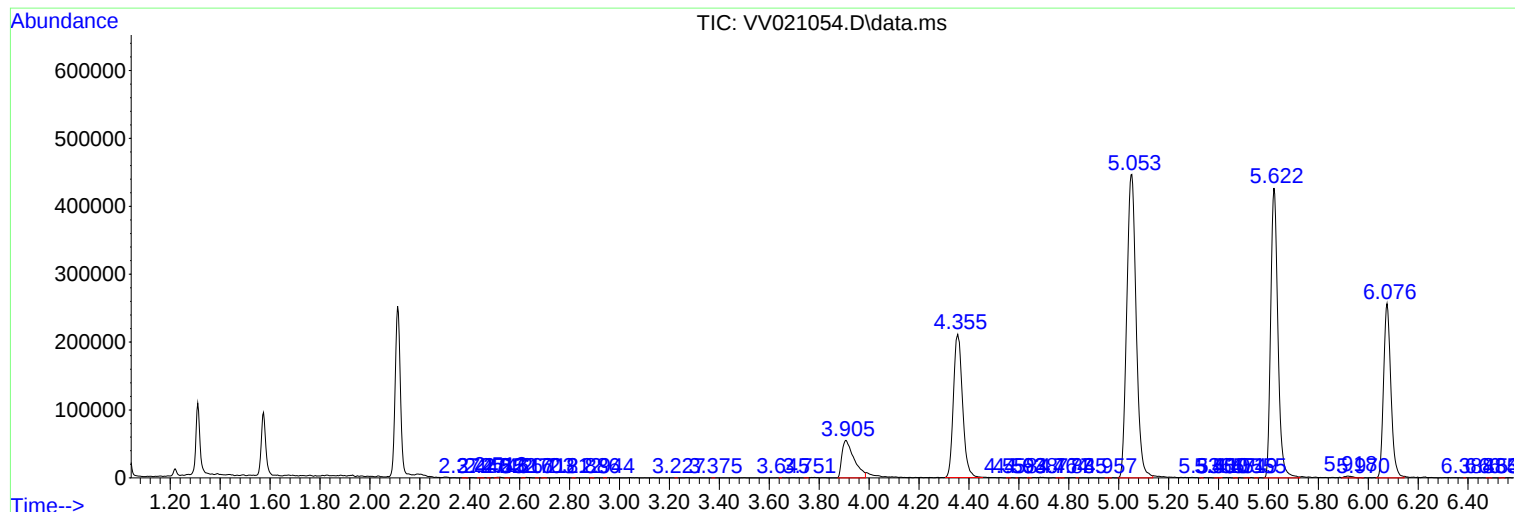

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021054.D
Acq On : 19 Apr 2021 14:38
Operator : SY/MD
Sample : M2067-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG592

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021054.D
Acq On : 19 Apr 2021 14:38
Operator : SY/MD
Sample : M2067-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG592

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
