

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021055.D
 Acq On : 19 Apr 2021 15:01
 Operator : SY/MD
 Sample : M2067-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.391	417	420	426	rBV2	453	401	0.03%	0.005%
2	2.452	435	439	443	rBB	667	534	0.05%	0.006%
3	2.516	452	459	471	rVV4	1706	2862	0.24%	0.032%
4	2.635	492	496	500	rVV4	617	673	0.06%	0.008%
5	2.777	528	540	554	rBV3	5664	12353	1.05%	0.139%
6	2.876	568	571	574	rBV2	258	173	0.01%	0.002%
7	2.992	605	607	611	rBV	283	209	0.02%	0.002%
8	3.050	619	625	631	rBV3	500	657	0.06%	0.007%
9	3.076	632	633	638	rVB	261	185	0.02%	0.002%
10	3.150	653	656	660	rBB	328	252	0.02%	0.003%
11	3.339	709	715	718	rBB	156	207	0.02%	0.002%
12	3.449	745	749	752	rBB2	224	189	0.02%	0.002%
13	3.548	775	780	782	rBB	388	248	0.02%	0.003%
14	3.587	790	792	795	rBV	386	187	0.02%	0.002%
15	3.696	824	826	829	rBB	290	175	0.01%	0.002%
16	3.860	873	877	880	rBB2	372	215	0.02%	0.002%
17	3.908	880	892	924	rBV2	55639	197257	16.78%	2.219%
18	4.355	1014	1031	1057	rBV2	219062	546772	46.52%	6.151%
19	4.584	1100	1102	1104	rBV2	310	214	0.02%	0.002%
20	4.670	1126	1129	1131	rBV	336	273	0.02%	0.003%
21	4.793	1165	1167	1171	rBB2	527	366	0.03%	0.004%
22	4.831	1176	1179	1181	rBV2	372	188	0.02%	0.002%
23	4.979	1219	1225	1228	rBV2	252	286	0.02%	0.003%
24	5.050	1231	1247	1281	rBV2	450967	1175315	100.00%	13.221%
25	5.326	1331	1333	1335	rBV	324	193	0.02%	0.002%
26	5.404	1352	1357	1363	rBB4	563	679	0.06%	0.008%
27	5.449	1370	1371	1375	rBV	369	259	0.02%	0.003%
28	5.551	1399	1403	1405	rBB2	446	254	0.02%	0.003%
29	5.622	1412	1425	1450	rBV	420255	839435	71.42%	9.443%
30	5.863	1497	1500	1508	rVB	4059	2713	0.23%	0.031%
31	6.027	1547	1551	1552	rBV	356	240	0.02%	0.003%
32	6.076	1552	1566	1592	rBV2	251457	511212	43.50%	5.751%
33	6.259	1620	1623	1624	rBV2	431	237	0.02%	0.003%
34	6.394	1661	1665	1668	rBV	325	327	0.03%	0.004%
35	6.442	1677	1680	1682	rBV2	483	279	0.02%	0.003%
36	6.571	1716	1720	1725	rBB2	501	417	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021055.D
 Acq On : 19 Apr 2021 15:01
 Operator : SY/MD
 Sample : M2067-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.622	1732	1736	1737	rBV2	259	166	0.01%	0.002%
38	6.703	1759	1761	1764	rVB2	401	202	0.02%	0.002%
39	6.793	1786	1789	1791	rBV2	318	199	0.02%	0.002%
40	6.857	1806	1809	1811	rBB	361	198	0.02%	0.002%
41	6.883	1814	1817	1821	rBB	261	192	0.02%	0.002%
42	6.992	1840	1851	1877	rBV	157471	283504	24.12%	3.189%
43	7.278	1937	1940	1942	rBB	456	268	0.02%	0.003%
44	7.320	1942	1953	1971	rBV	552710	955136	81.27%	10.744%
45	7.574	2031	2032	2037	rVB	527	327	0.03%	0.004%
46	7.625	2037	2048	2065	rBV	116697	198393	16.88%	2.232%
47	7.793	2097	2100	2101	rBV	566	359	0.03%	0.004%
48	7.828	2107	2111	2113	rBB	403	284	0.02%	0.003%
49	7.850	2116	2118	2122	rVB2	293	212	0.02%	0.002%
50	7.895	2130	2132	2134	rVB	447	180	0.02%	0.002%
51	7.931	2137	2143	2145	rBV2	541	536	0.05%	0.006%
52	7.982	2151	2159	2172	rVB4	10832	19241	1.64%	0.216%
53	8.095	2184	2194	2214	rBV	271143	478856	40.74%	5.387%
54	8.432	2296	2299	2304	rVB3	552	352	0.03%	0.004%
55	8.519	2321	2326	2328	rBV2	845	626	0.05%	0.007%
56	8.667	2370	2372	2374	rBV2	452	222	0.02%	0.002%
57	8.693	2379	2380	2385	rVB	353	199	0.02%	0.002%
58	8.748	2394	2397	2398	rBV	308	202	0.02%	0.002%
59	8.857	2418	2431	2464	rBV	631972	1023680	87.10%	11.515%
60	9.082	2499	2501	2503	rBV2	538	277	0.02%	0.003%
61	9.262	2554	2557	2558	rBV2	441	211	0.02%	0.002%
62	9.307	2569	2571	2575	rBV2	566	407	0.03%	0.005%
63	9.384	2591	2595	2599	rBV2	470	425	0.04%	0.005%
64	9.426	2606	2608	2614	rVB	370	255	0.02%	0.003%
65	9.548	2642	2646	2651	rBV2	487	528	0.04%	0.006%
66	9.593	2658	2660	2666	rBV	370	365	0.03%	0.004%
67	9.625	2666	2670	2675	rVB2	318	363	0.03%	0.004%
68	9.657	2676	2680	2682	rBV	280	225	0.02%	0.003%
69	9.921	2760	2762	2765	rBV	310	221	0.02%	0.002%
70	9.937	2765	2767	2769	rVV	511	224	0.02%	0.003%
71	9.953	2770	2772	2777	rVB	556	375	0.03%	0.004%
72	10.050	2800	2802	2806	rVB	265	185	0.02%	0.002%
73	10.069	2806	2808	2812	rBB2	383	270	0.02%	0.003%
74	10.104	2813	2819	2821	rBV2	619	469	0.04%	0.005%
75	10.223	2844	2856	2872	rBV	425382	659480	56.11%	7.418%
76	10.346	2891	2894	2895	rBV	355	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021055.D
 Acq On : 19 Apr 2021 15:01
 Operator : SY/MD
 Sample : M2067-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.362	2897	2899	2902	rBV2	343	169	0.01%	0.002%
78	10.391	2902	2908	2911	rBV4	928	1001	0.09%	0.011%
79	10.452	2925	2927	2929	rBV	343	199	0.02%	0.002%
80	10.612	2976	2977	2980	rVB	400	185	0.02%	0.002%
81	10.635	2981	2984	2986	rBV	245	180	0.02%	0.002%
82	10.664	2990	2993	2994	rBV	392	223	0.02%	0.003%
83	10.754	3017	3021	3023	rBV2	479	288	0.02%	0.003%
84	10.834	3039	3046	3048	rBV2	489	507	0.04%	0.006%
85	10.915	3064	3071	3072	rBV2	1365	1041	0.09%	0.012%
86	10.963	3084	3086	3091	rBV	311	290	0.02%	0.003%
87	10.989	3091	3094	3095	rVV	435	208	0.02%	0.002%
88	11.024	3102	3105	3107	rBV	216	176	0.01%	0.002%
89	11.072	3116	3120	3122	rBV2	477	296	0.03%	0.003%
90	11.153	3139	3145	3149	rVV3	979	843	0.07%	0.009%
91	11.255	3166	3177	3194	rBV	619923	957415	81.46%	10.770%
92	11.632	3282	3294	3314	rBV	635423	998498	84.96%	11.232%
93	11.908	3378	3380	3384	rVB	471	307	0.03%	0.003%
94	11.944	3388	3391	3394	rBV	641	494	0.04%	0.006%
95	12.259	3482	3489	3494	rBV2	1074	1428	0.12%	0.016%
96	12.603	3591	3596	3600	rBV2	573	552	0.05%	0.006%
97	12.882	3681	3683	3686	rVB2	372	187	0.02%	0.002%
98	12.905	3686	3690	3694	rBV2	359	381	0.03%	0.004%
99	13.410	3845	3847	3851	rVB2	484	285	0.02%	0.003%
100	13.599	3904	3906	3907	rBV	441	232	0.02%	0.003%




Sum of corrected areas: 8889821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021055.D
Acq On : 19 Apr 2021 15:01
Operator : SY/MD
Sample : M2067-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

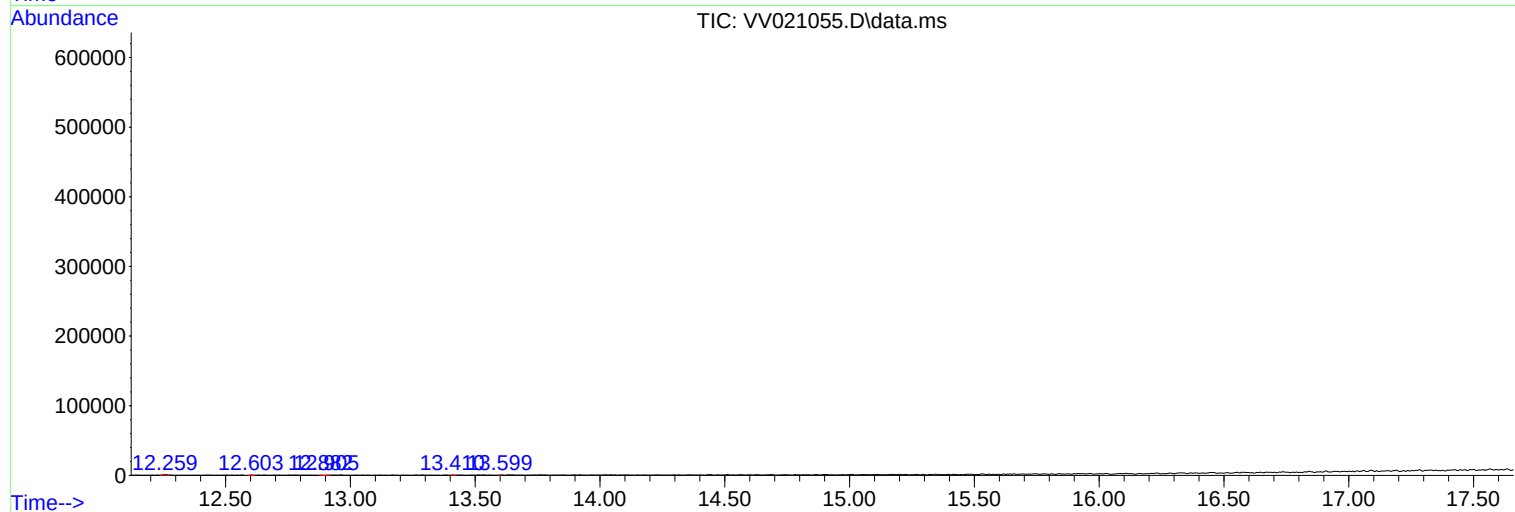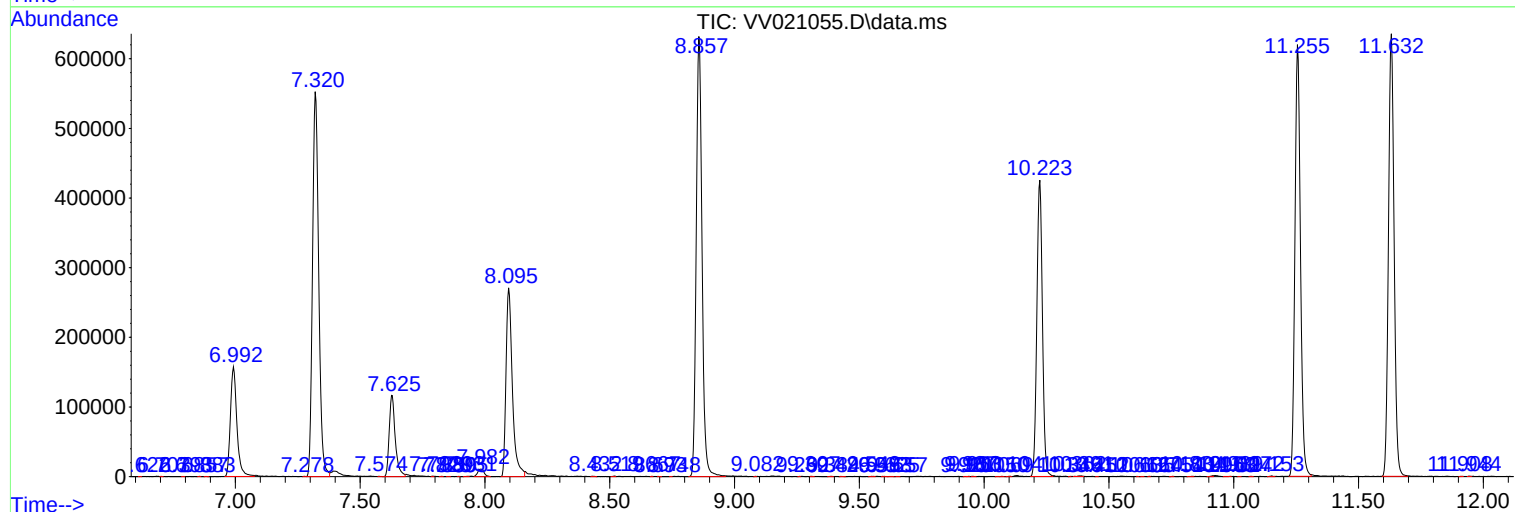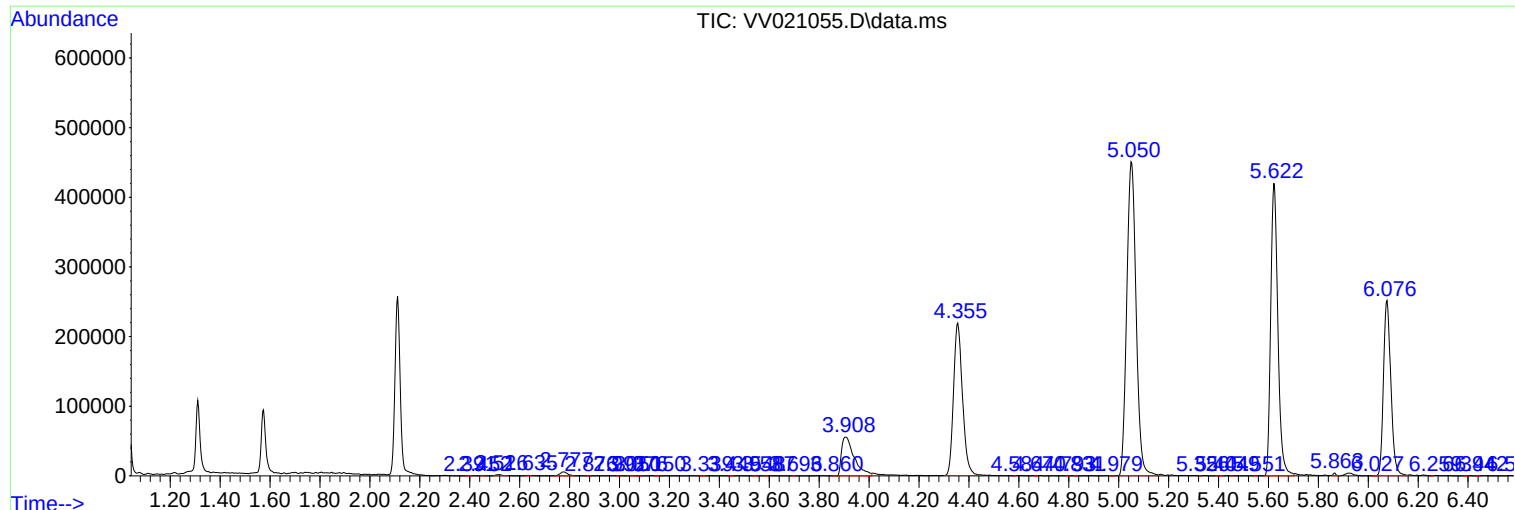

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021055.D
Acq On : 19 Apr 2021 15:01
Operator : SY/MD
Sample : M2067-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021055.D
Acq On : 19 Apr 2021 15:01
Operator : SY/MD
Sample : M2067-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
