

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021058.D
 Acq On : 19 Apr 2021 16:38
 Operator : SY/MD
 Sample : M2067-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.420	426	429	433	rBB	287	229	0.02%	0.002%
2	2.462	434	442	446	rBV3	933	1363	0.10%	0.014%
3	2.574	474	477	479	rBV2	334	257	0.02%	0.003%
4	2.773	525	539	572	rVB2	623554	1318764	100.00%	13.360%
5	2.966	596	599	601	rBV4	912	459	0.03%	0.005%
6	3.008	609	612	615	rBV2	330	230	0.02%	0.002%
7	3.053	615	626	634	rVB3	3586	6381	0.48%	0.065%
8	3.198	668	671	676	rBB2	272	206	0.02%	0.002%
9	3.224	677	679	683	rBB	628	277	0.02%	0.003%
10	3.249	684	687	688	rBV	417	218	0.02%	0.002%
11	3.298	693	702	706	rBV5	2011	3533	0.27%	0.036%
12	3.423	739	741	744	rBB	338	218	0.02%	0.002%
13	3.490	759	762	765	rBB	355	197	0.01%	0.002%
14	3.741	837	840	841	rBV	466	295	0.02%	0.003%
15	3.828	865	867	871	rVV2	239	170	0.01%	0.002%
16	3.905	881	891	923	rBV2	56325	193952	14.71%	1.965%
17	4.571	1095	1098	1100	rBV2	636	356	0.03%	0.004%
18	4.654	1119	1124	1125	rBB	553	305	0.02%	0.003%
19	4.715	1141	1143	1147	rVB2	334	214	0.02%	0.002%
20	4.780	1161	1163	1165	rVB	390	179	0.01%	0.002%
21	4.809	1170	1172	1174	rBB	418	179	0.01%	0.002%
22	4.966	1218	1221	1223	rBV	229	179	0.01%	0.002%
23	5.053	1230	1248	1273	rBV3	459163	1195926	90.69%	12.115%
24	5.314	1328	1329	1332	rBV3	729	316	0.02%	0.003%
25	5.381	1347	1350	1352	rBB2	389	211	0.02%	0.002%
26	5.397	1353	1355	1358	rBB	640	271	0.02%	0.003%
27	5.413	1359	1360	1364	rBB	270	168	0.01%	0.002%
28	5.455	1369	1373	1374	rBV	321	221	0.02%	0.002%
29	5.622	1412	1425	1449	rBV	416980	837078	63.47%	8.480%
30	5.924	1507	1519	1536	rBV5	26452	56063	4.25%	0.568%
31	6.076	1550	1566	1587	rBV2	254817	519856	39.42%	5.266%
32	6.211	1606	1608	1609	rBV2	497	257	0.02%	0.003%
33	6.339	1646	1648	1652	rVV	401	207	0.02%	0.002%
34	6.378	1657	1660	1665	rBB2	557	408	0.03%	0.004%
35	6.429	1673	1676	1678	rBV	446	217	0.02%	0.002%
36	6.564	1716	1718	1720	rBV	272	183	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021058.D
 Acq On : 19 Apr 2021 16:38
 Operator : SY/MD
 Sample : M2067-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.596	1725	1728	1731	rVB2	452	244	0.02%	0.002%
38	6.677	1750	1753	1756	rBB2	275	205	0.02%	0.002%
39	6.703	1756	1761	1764	rBB	284	216	0.02%	0.002%
40	6.751	1773	1776	1777	rBV	366	172	0.01%	0.002%
41	6.799	1787	1791	1794	rBV	468	303	0.02%	0.003%
42	6.818	1794	1797	1800	rVB2	354	252	0.02%	0.003%
43	6.992	1839	1851	1871	rBV	126009	228530	17.33%	2.315%
44	7.162	1901	1904	1910	rVB3	865	749	0.06%	0.008%
45	7.194	1911	1914	1918	rBV3	723	623	0.05%	0.006%
46	7.262	1930	1935	1939	rBV3	509	496	0.04%	0.005%
47	7.320	1942	1953	1971	rBV	563084	972953	73.78%	9.857%
48	7.625	2039	2048	2070	rBV	91177	163130	12.37%	1.653%
49	7.876	2123	2126	2133	rBV3	439	462	0.04%	0.005%
50	7.979	2148	2158	2175	rVB	203761	337243	25.57%	3.416%
51	8.095	2184	2194	2218	rBV	270422	483579	36.67%	4.899%
52	8.394	2283	2287	2289	rBV	272	177	0.01%	0.002%
53	8.423	2293	2296	2297	rBV	436	262	0.02%	0.003%
54	8.458	2303	2307	2308	rBV	325	231	0.02%	0.002%
55	8.490	2314	2317	2319	rBV2	443	273	0.02%	0.003%
56	8.632	2359	2361	2364	rBV	360	298	0.02%	0.003%
57	8.702	2382	2383	2385	rBV	376	204	0.02%	0.002%
58	8.767	2400	2403	2405	rBV	241	166	0.01%	0.002%
59	8.857	2419	2431	2450	rBV	629780	1013210	76.83%	10.264%
60	9.075	2497	2499	2501	rBV	436	205	0.02%	0.002%
61	9.095	2503	2505	2506	rBV	467	213	0.02%	0.002%
62	9.185	2531	2533	2535	rBV2	382	222	0.02%	0.002%
63	9.345	2580	2583	2585	rBV3	337	218	0.02%	0.002%
64	9.403	2597	2601	2605	rVV2	317	308	0.02%	0.003%
65	9.474	2619	2623	2625	rBV	300	259	0.02%	0.003%
66	9.693	2689	2691	2695	rBV	314	198	0.02%	0.002%
67	10.050	2799	2802	2806	rVB3	330	223	0.02%	0.002%
68	10.124	2823	2825	2828	rVB	510	276	0.02%	0.003%
69	10.140	2828	2830	2836	rBB	440	308	0.02%	0.003%
70	10.169	2836	2839	2841	rBV	283	225	0.02%	0.002%
71	10.220	2844	2855	2874	rBV	417148	655735	49.72%	6.643%
72	10.374	2901	2903	2905	rBV	571	302	0.02%	0.003%
73	10.616	2974	2978	2980	rBV2	487	366	0.03%	0.004%
74	10.670	2991	2995	2999	rBV	338	329	0.02%	0.003%
75	10.744	3016	3018	3021	rBV	274	191	0.01%	0.002%
76	10.805	3034	3037	3040	rBB	292	173	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021058.D
 Acq On : 19 Apr 2021 16:38
 Operator : SY/MD
 Sample : M2067-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.898	3063	3066	3068	rBV2	418	280	0.02%	0.003%
78	10.995	3091	3096	3098	rBV2	336	346	0.03%	0.004%
79	11.021	3102	3104	3106	rBV	325	195	0.01%	0.002%
80	11.056	3110	3115	3118	rBB2	410	306	0.02%	0.003%
81	11.075	3118	3121	3123	rBV2	408	306	0.02%	0.003%
82	11.159	3145	3147	3149	rBV	751	289	0.02%	0.003%
83	11.255	3165	3177	3199	rBV	570324	901331	68.35%	9.131%
84	11.464	3239	3242	3244	rBV	255	179	0.01%	0.002%
85	11.506	3253	3255	3260	rVB	540	419	0.03%	0.004%
86	11.538	3261	3265	3266	rBV2	543	334	0.03%	0.003%
87	11.632	3282	3294	3311	rBV	612509	959168	72.73%	9.717%
88	11.873	3365	3369	3372	rBV3	725	630	0.05%	0.006%
89	11.969	3394	3399	3401	rBV	238	221	0.02%	0.002%
90	12.066	3427	3429	3433	rVB	459	213	0.02%	0.002%
91	12.130	3446	3449	3452	rBV2	437	342	0.03%	0.003%
92	12.175	3459	3463	3466	rBV2	423	443	0.03%	0.004%
93	12.394	3528	3531	3533	rBV2	409	252	0.02%	0.003%
94	12.464	3550	3553	3556	rBV	529	319	0.02%	0.003%
95	12.741	3636	3639	3640	rBV	293	191	0.01%	0.002%
96	13.143	3760	3764	3767	rBV	380	366	0.03%	0.004%
97	13.246	3794	3796	3799	rBV2	640	389	0.03%	0.004%
98	13.619	3906	3912	3915	rBV2	702	829	0.06%	0.008%
99	13.786	3962	3964	3968	rBV	334	249	0.02%	0.003%
100	13.818	3972	3974	3977	rBV	595	279	0.02%	0.003%




Sum of corrected areas: 9871148

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021058.D
Acq On : 19 Apr 2021 16:38
Operator : SY/MD
Sample : M2067-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

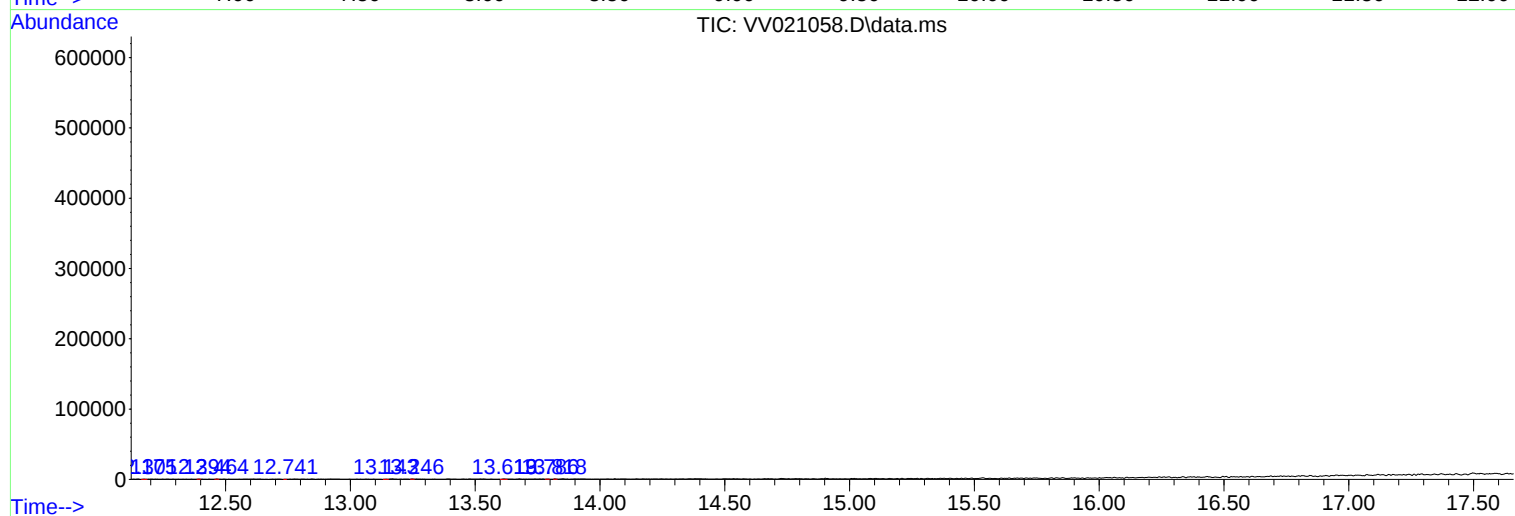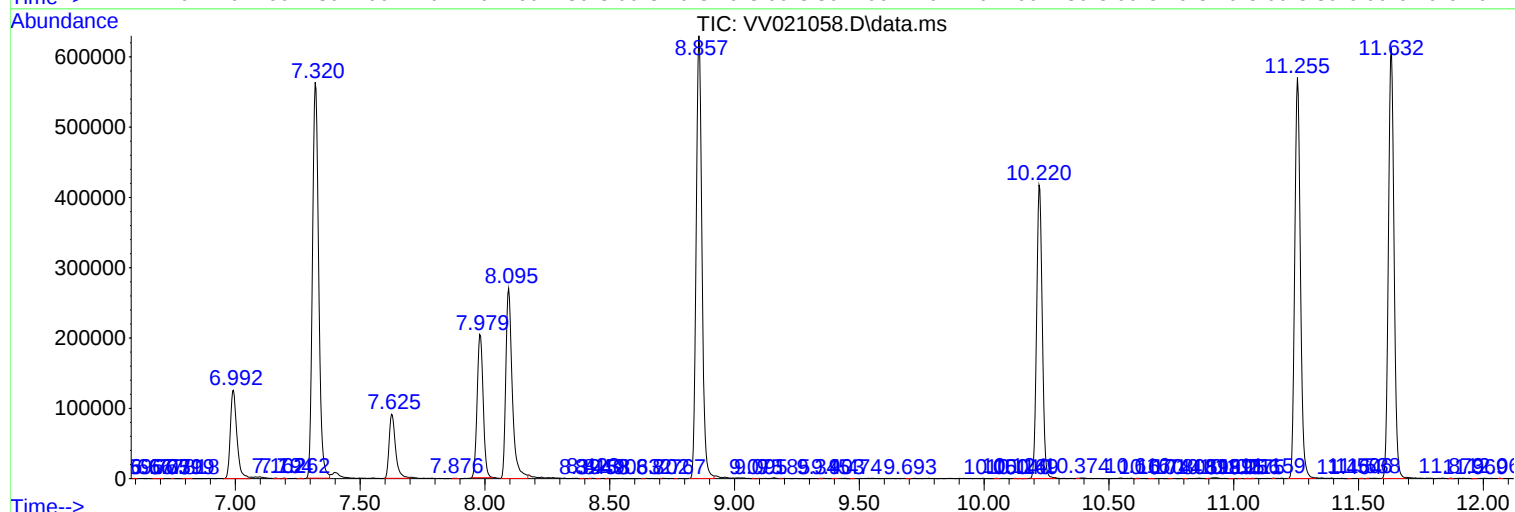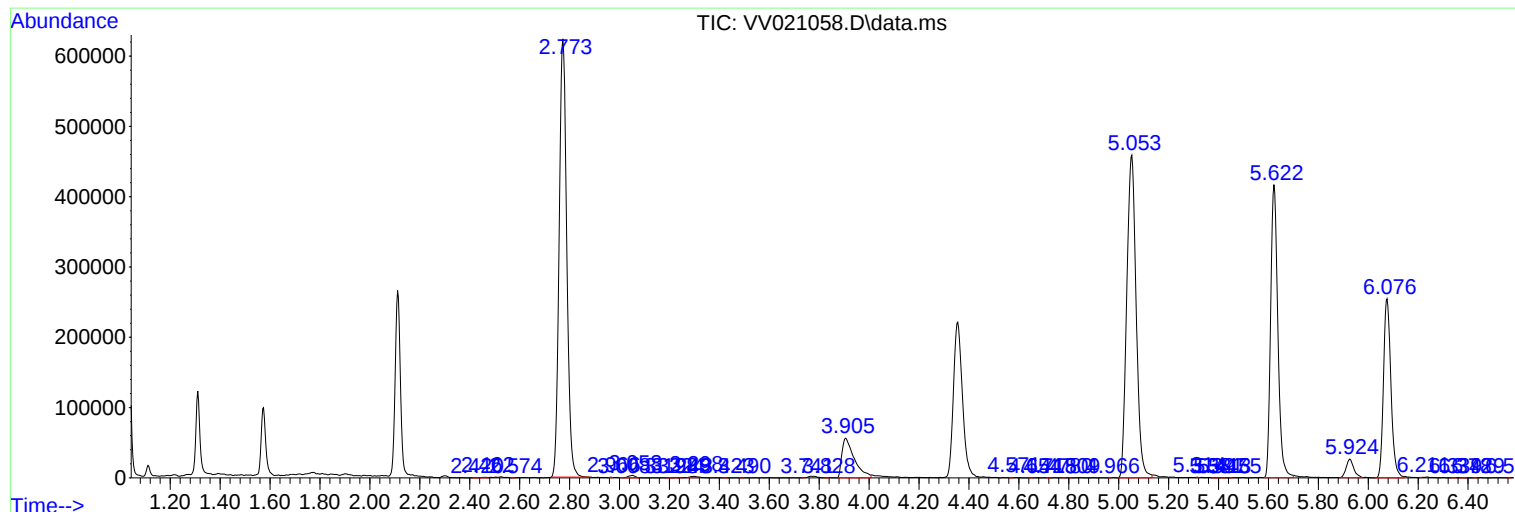

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021058.D
Acq On : 19 Apr 2021 16:38
Operator : SY/MD
Sample : M2067-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021058.D
Acq On : 19 Apr 2021 16:38
Operator : SY/MD
Sample : M2067-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
