

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021062.D
 Acq On : 19 Apr 2021 18:12
 Operator : SY/MD
 Sample : M2067-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.285	384	387	388	rBV3	548	293	0.02%	0.003%
2	2.410	422	426	428	rBV	321	253	0.02%	0.003%
3	2.426	429	431	433	rVB	437	162	0.01%	0.002%
4	2.513	450	458	469	rVB6	3321	5175	0.44%	0.062%
5	2.606	482	487	488	rBV6	798	433	0.04%	0.005%
6	2.709	515	519	522	rBB	336	205	0.02%	0.002%
7	2.728	522	525	527	rBV	256	169	0.01%	0.002%
8	2.806	547	549	552	rBV	418	318	0.03%	0.004%
9	2.841	558	560	562	rBV	304	182	0.02%	0.002%
10	2.966	597	599	603	rVB	397	206	0.02%	0.002%
11	3.095	636	639	641	rBV	285	177	0.02%	0.002%
12	3.204	669	673	675	rBV2	437	300	0.03%	0.004%
13	3.281	695	697	699	rBV3	425	253	0.02%	0.003%
14	3.400	732	734	737	rBV	397	296	0.03%	0.004%
15	3.603	794	797	800	rBV2	484	255	0.02%	0.003%
16	3.622	800	803	806	rVB2	406	242	0.02%	0.003%
17	3.699	825	827	831	rBB2	273	188	0.02%	0.002%
18	3.912	882	893	930	rBV2	48180	196404	16.66%	2.339%
19	4.606	1106	1109	1112	rBV	283	266	0.02%	0.003%
20	4.680	1130	1132	1134	rBV	396	216	0.02%	0.003%
21	4.693	1134	1136	1139	rVB2	385	209	0.02%	0.002%
22	4.732	1144	1148	1150	rBB	307	211	0.02%	0.003%
23	4.748	1150	1153	1154	rBV	470	296	0.03%	0.004%
24	4.831	1175	1179	1183	rBB2	375	295	0.03%	0.004%
25	4.854	1184	1186	1188	rBV2	280	152	0.01%	0.002%
26	5.050	1231	1247	1277	rBV3	451406	1179029	100.00%	14.043%
27	5.291	1320	1322	1326	rBV3	737	487	0.04%	0.006%
28	5.358	1340	1343	1346	rBV	270	206	0.02%	0.002%
29	5.429	1363	1365	1368	rVB	323	152	0.01%	0.002%
30	5.487	1381	1383	1386	rBV	433	208	0.02%	0.002%
31	5.500	1386	1387	1390	rBV2	410	253	0.02%	0.003%
32	5.622	1411	1425	1454	rBV	432331	869922	73.78%	10.361%
33	5.815	1482	1485	1488	rVB2	740	474	0.04%	0.006%
34	6.005	1542	1544	1548	rVB	395	216	0.02%	0.003%
35	6.024	1548	1550	1552	rBV	509	237	0.02%	0.003%
36	6.075	1552	1566	1587	rBV	248676	511747	43.40%	6.095%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021062.D
 Acq On : 19 Apr 2021 18:12
 Operator : SY/MD
 Sample : M2067-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1645	rBV	386	227	0.02%	0.003%
38	6.362	1653	1655	1660	rBB	323	276	0.02%	0.003%
39	6.394	1663	1665	1668	rBB	376	155	0.01%	0.002%
40	6.439	1674	1679	1684	rBB2	540	467	0.04%	0.006%
41	6.474	1687	1690	1692	rBB2	602	281	0.02%	0.003%
42	6.532	1705	1708	1710	rBB	259	181	0.02%	0.002%
43	6.551	1711	1714	1717	rBV	141	148	0.01%	0.002%
44	6.657	1744	1747	1748	rBV	296	154	0.01%	0.002%
45	6.776	1782	1784	1786	rBV	465	257	0.02%	0.003%
46	6.924	1826	1830	1832	rVB2	387	259	0.02%	0.003%
47	6.992	1837	1851	1882	rBV	154572	282959	24.00%	3.370%
48	7.236	1925	1927	1929	rBV	488	247	0.02%	0.003%
49	7.320	1941	1953	1971	rBV	543826	947704	80.38%	11.287%
50	7.625	2036	2048	2076	rBV2	112427	200496	17.01%	2.388%
51	7.789	2097	2099	2104	rVB2	657	368	0.03%	0.004%
52	7.841	2111	2115	2118	rBV2	651	584	0.05%	0.007%
53	7.870	2122	2124	2127	rBB	692	425	0.04%	0.005%
54	7.895	2130	2132	2134	rBB	339	171	0.01%	0.002%
55	7.985	2153	2160	2170	rBV7	2996	4389	0.37%	0.052%
56	8.098	2184	2195	2226	rBV	266292	499019	42.32%	5.943%
57	8.432	2293	2299	2300	rBV2	424	346	0.03%	0.004%
58	8.493	2315	2318	2320	rBV	392	245	0.02%	0.003%
59	8.587	2343	2347	2350	rBB2	296	254	0.02%	0.003%
60	8.616	2354	2356	2361	rBB2	418	310	0.03%	0.004%
61	8.638	2361	2363	2365	rBV2	378	200	0.02%	0.002%
62	8.735	2390	2393	2396	rBB	254	152	0.01%	0.002%
63	8.767	2401	2403	2405	rBB	331	148	0.01%	0.002%
64	8.792	2409	2411	2414	rBV	286	210	0.02%	0.003%
65	8.857	2420	2431	2448	rBV	644900	1047321	88.83%	12.474%
66	9.140	2516	2519	2520	rBV	378	164	0.01%	0.002%
67	9.394	2591	2598	2600	rBV2	257	353	0.03%	0.004%
68	9.410	2600	2603	2606	rVV2	249	149	0.01%	0.002%
69	9.474	2620	2623	2626	rBV	224	209	0.02%	0.002%
70	9.554	2644	2648	2650	rBV2	313	284	0.02%	0.003%
71	9.706	2693	2695	2698	rBV	285	204	0.02%	0.002%
72	9.751	2705	2709	2713	rBB2	323	294	0.02%	0.004%
73	9.998	2782	2786	2787	rBV2	285	176	0.01%	0.002%
74	10.021	2792	2793	2797	rBB	312	178	0.02%	0.002%
75	10.043	2797	2800	2801	rBV	493	270	0.02%	0.003%
76	10.133	2818	2828	2835	rBV3	1665	2330	0.20%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021062.D
 Acq On : 19 Apr 2021 18:12
 Operator : SY/MD
 Sample : M2067-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.223	2844	2856	2873	rBV	427130	664381	56.35%	7.913%
78	10.362	2896	2899	2900	rBV	573	335	0.03%	0.004%
79	10.429	2916	2920	2922	rBV	238	155	0.01%	0.002%
80	10.464	2928	2931	2933	rBV2	332	163	0.01%	0.002%
81	10.519	2945	2948	2954	rBB	403	309	0.03%	0.004%
82	10.558	2955	2960	2962	rBV2	691	650	0.06%	0.008%
83	10.644	2985	2987	2991	rBB	278	181	0.02%	0.002%
84	10.754	3017	3021	3022	rBV	338	257	0.02%	0.003%
85	10.860	3051	3054	3058	rBV3	702	596	0.05%	0.007%
86	10.976	3089	3090	3093	rBV3	312	180	0.02%	0.002%
87	11.011	3099	3101	3105	rVB	393	246	0.02%	0.003%
88	11.034	3105	3108	3110	rBV	445	343	0.03%	0.004%
89	11.149	3140	3144	3150	rBV4	944	1146	0.10%	0.014%
90	11.255	3165	3177	3203	rBV	630255	979711	83.09%	11.669%
91	11.480	3245	3247	3255	rVB	712	515	0.04%	0.006%
92	11.529	3255	3262	3265	rBV2	601	654	0.06%	0.008%
93	11.632	3283	3294	3316	rBV	638520	980672	83.18%	11.680%
94	12.111	3441	3443	3446	rBV	668	323	0.03%	0.004%
95	12.249	3482	3486	3488	rBV2	731	594	0.05%	0.007%
96	12.307	3500	3504	3508	rVB2	809	547	0.05%	0.007%
97	12.487	3558	3560	3563	rVB	438	230	0.02%	0.003%
98	12.786	3651	3653	3657	rBV	395	302	0.03%	0.004%
99	13.249	3793	3797	3801	rBV2	688	710	0.06%	0.008%
100	13.722	3942	3944	3947	rBV2	393	228	0.02%	0.003%




Sum of corrected areas: 8396079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021062.D
Acq On : 19 Apr 2021 18:12
Operator : SY/MD
Sample : M2067-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

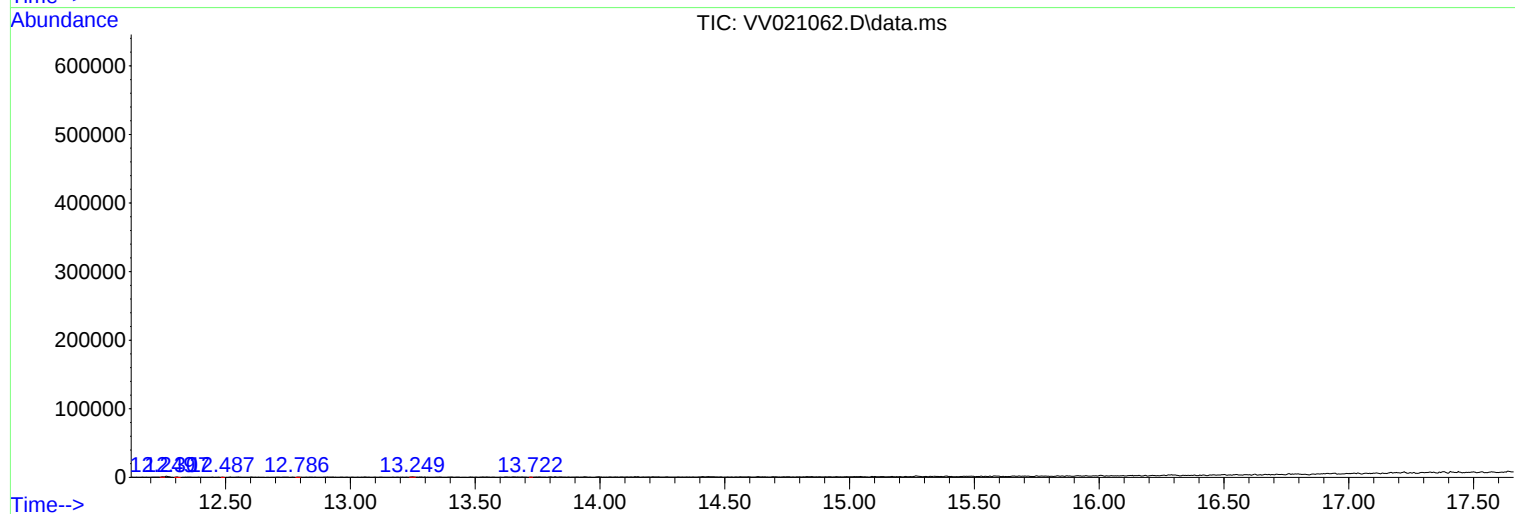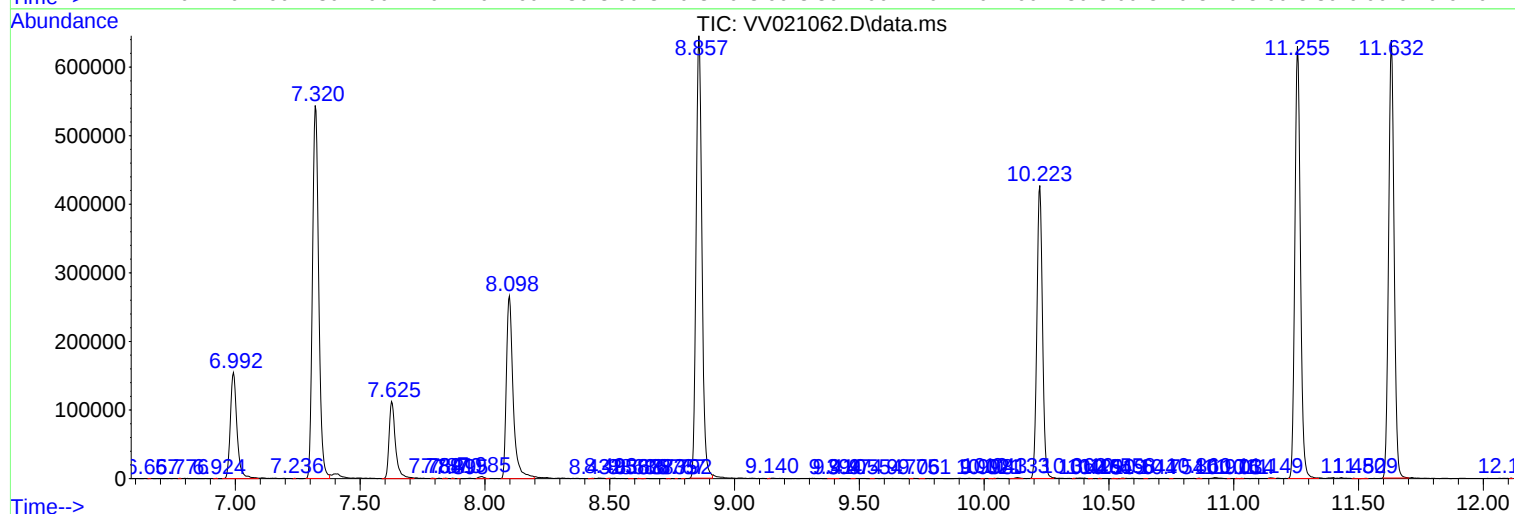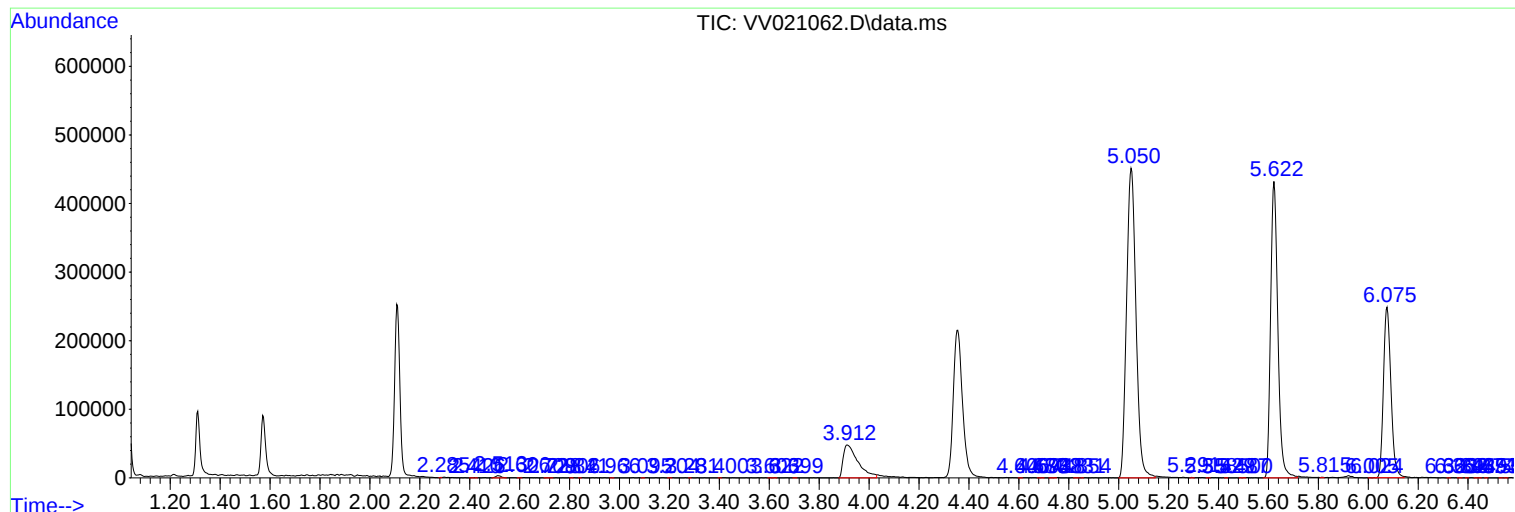

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021062.D
Acq On : 19 Apr 2021 18:12
Operator : SY/MD
Sample : M2067-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021062.D
Acq On : 19 Apr 2021 18:12
Operator : SY/MD
Sample : M2067-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
