

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021063.D
 Acq On : 19 Apr 2021 18:36
 Operator : SY/MD
 Sample : M2067-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG799DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	79	84	103	rVB	166054	181802	13.27%	1.790%
2	2.330	399	401	404	rBB	364	184	0.01%	0.002%
3	2.455	437	440	441	rBV	296	148	0.01%	0.001%
4	2.510	453	457	466	rBV5	1423	2023	0.15%	0.020%
5	2.587	477	481	484	rBV	254	202	0.01%	0.002%
6	2.760	533	535	539	rBB	375	187	0.01%	0.002%
7	2.805	544	549	556	rBV2	330	543	0.04%	0.005%
8	2.895	574	577	579	rBV	282	187	0.01%	0.002%
9	2.924	584	586	589	rBB	293	179	0.01%	0.002%
10	3.558	781	783	788	rBB	255	224	0.02%	0.002%
11	3.645	807	810	813	rBV2	307	243	0.02%	0.002%
12	3.690	820	824	827	rBB2	458	282	0.02%	0.003%
13	3.754	842	844	850	rBB	218	165	0.01%	0.002%
14	3.915	882	894	924	rBV2	51933	197776	14.44%	1.947%
15	4.587	1099	1103	1108	rVB3	461	376	0.03%	0.004%
16	4.616	1109	1112	1114	rBV3	374	247	0.02%	0.002%
17	4.754	1153	1155	1159	rVB	488	252	0.02%	0.002%
18	4.799	1166	1169	1171	rBV	282	174	0.01%	0.002%
19	4.911	1203	1204	1207	rBB	389	170	0.01%	0.002%
20	4.947	1213	1215	1217	rVV2	352	164	0.01%	0.002%
21	4.979	1222	1225	1228	rBB	344	186	0.01%	0.002%
22	5.050	1230	1247	1276	rBV2	531331	1369967	100.00%	13.486%
23	5.426	1362	1364	1367	rBV	445	368	0.03%	0.004%
24	5.484	1379	1382	1383	rBV	335	199	0.01%	0.002%
25	5.561	1401	1406	1407	rBV	219	166	0.01%	0.002%
26	5.622	1413	1425	1451	rBV	427548	857289	62.58%	8.439%
27	6.014	1545	1547	1549	rBV	269	150	0.01%	0.001%
28	6.075	1553	1566	1594	rVV2	287748	586242	42.79%	5.771%
29	6.323	1640	1643	1644	rBV	395	188	0.01%	0.002%
30	6.355	1649	1653	1656	rBV2	382	295	0.02%	0.003%
31	6.384	1660	1662	1663	rBV2	513	227	0.02%	0.002%
32	6.474	1687	1690	1694	rBB	270	171	0.01%	0.002%
33	6.522	1700	1705	1707	rBV3	525	449	0.03%	0.004%
34	6.712	1760	1764	1768	rBB	349	272	0.02%	0.003%
35	6.786	1784	1787	1789	rBB	454	200	0.01%	0.002%
36	6.802	1789	1792	1795	rBB2	389	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021063.D
 Acq On : 19 Apr 2021 18:36
 Operator : SY/MD
 Sample : M2067-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG799DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.821	1796	1798	1802	rBB	325	226	0.02%	0.002%
38	6.857	1806	1809	1810	rBV	438	254	0.02%	0.003%
39	6.992	1840	1851	1875	rVV	174798	318162	23.22%	3.132%
40	7.181	1906	1910	1914	rBV	539	556	0.04%	0.005%
41	7.320	1939	1953	1973	rBV	662479	1137678	83.04%	11.199%
42	7.571	2028	2031	2035	rBB2	711	466	0.03%	0.005%
43	7.625	2035	2048	2064	rBV	131587	225450	16.46%	2.219%
44	7.857	2118	2120	2122	rBV	299	180	0.01%	0.002%
45	7.979	2143	2158	2181	rBV	534483	898138	65.56%	8.841%
46	8.095	2185	2194	2227	rVV	283999	511169	37.31%	5.032%
47	8.426	2295	2297	2299	rBV	473	262	0.02%	0.003%
48	8.554	2334	2337	2340	rBV2	385	243	0.02%	0.002%
49	8.577	2340	2344	2348	rVV2	488	434	0.03%	0.004%
50	8.596	2348	2350	2353	rVB	486	289	0.02%	0.003%
51	8.619	2353	2357	2359	rBV	408	294	0.02%	0.003%
52	8.648	2364	2366	2368	rBV	371	168	0.01%	0.002%
53	8.693	2377	2380	2382	rBV2	427	306	0.02%	0.003%
54	8.744	2395	2396	2399	rVB	371	162	0.01%	0.002%
55	8.783	2402	2408	2410	rBV	339	306	0.02%	0.003%
56	8.857	2419	2431	2453	rBV	644016	1047602	76.47%	10.312%
57	9.046	2488	2490	2492	rBV2	555	257	0.02%	0.003%
58	9.162	2519	2526	2530	rBV4	831	1076	0.08%	0.011%
59	9.207	2539	2540	2543	rVB	395	171	0.01%	0.002%
60	9.313	2572	2573	2576	rBV	251	166	0.01%	0.002%
61	9.413	2601	2604	2606	rBV3	673	320	0.02%	0.003%
62	9.435	2609	2611	2615	rBV	354	264	0.02%	0.003%
63	9.500	2626	2631	2633	rBB	349	264	0.02%	0.003%
64	9.516	2633	2636	2638	rBB	455	261	0.02%	0.003%
65	9.587	2653	2658	2659	rBB	235	179	0.01%	0.002%
66	9.599	2659	2662	2663	rBV	271	147	0.01%	0.001%
67	9.660	2676	2681	2682	rBV	343	223	0.02%	0.002%
68	9.693	2688	2691	2693	rBB	369	214	0.02%	0.002%
69	9.722	2696	2700	2702	rBB	376	210	0.02%	0.002%
70	9.757	2709	2711	2714	rBV	441	215	0.02%	0.002%
71	9.863	2738	2744	2747	rBV	345	376	0.03%	0.004%
72	10.027	2789	2795	2796	rBV2	425	371	0.03%	0.004%
73	10.069	2806	2808	2812	rBV	246	192	0.01%	0.002%
74	10.088	2812	2814	2817	rVV2	315	188	0.01%	0.002%
75	10.223	2843	2856	2871	rBV	433731	688348	50.25%	6.776%
76	10.410	2911	2914	2916	rBV	717	378	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021063.D
 Acq On : 19 Apr 2021 18:36
 Operator : SY/MD
 Sample : M2067-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG799DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.506	2942	2944	2948	rBV2	372	265	0.02%	0.003%
78	10.625	2979	2981	2985	rVB	375	258	0.02%	0.003%
79	10.654	2988	2990	2994	rBB2	398	232	0.02%	0.002%
80	10.741	3015	3017	3020	rBV	351	199	0.01%	0.002%
81	10.857	3049	3053	3060	rVB4	677	827	0.06%	0.008%
82	10.886	3060	3062	3065	rBB	465	222	0.02%	0.002%
83	10.921	3065	3073	3078	rBV5	2404	3228	0.24%	0.032%
84	11.033	3104	3108	3110	rBV2	611	529	0.04%	0.005%
85	11.107	3125	3131	3132	rBV	284	241	0.02%	0.002%
86	11.255	3165	3177	3195	rBV	659979	1011684	73.85%	9.959%
87	11.484	3246	3248	3250	rBV2	558	368	0.03%	0.004%
88	11.545	3262	3267	3271	rVB3	901	780	0.06%	0.008%
89	11.567	3271	3274	3275	rBV3	415	252	0.02%	0.002%
90	11.631	3283	3294	3315	rBV	715115	1097952	80.14%	10.808%
91	11.882	3369	3372	3375	rBV	362	253	0.02%	0.002%
92	12.011	3410	3412	3417	rVB2	533	259	0.02%	0.003%
93	12.223	3476	3478	3481	rVB	386	153	0.01%	0.002%
94	12.799	3652	3657	3661	rBV	508	518	0.04%	0.005%
95	12.905	3687	3690	3693	rBV	394	243	0.02%	0.002%
96	13.165	3766	3771	3774	rBV2	582	512	0.04%	0.005%
97	13.400	3842	3844	3847	rVB	497	243	0.02%	0.002%
98	13.490	3871	3872	3879	rVB	620	426	0.03%	0.004%
99	13.535	3884	3886	3890	rBV2	556	412	0.03%	0.004%
100	14.053	4044	4047	4049	rBV	358	250	0.02%	0.002%




Sum of corrected areas: 10158571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021063.D
Acq On : 19 Apr 2021 18:36
Operator : SY/MD
Sample : M2067-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG799DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

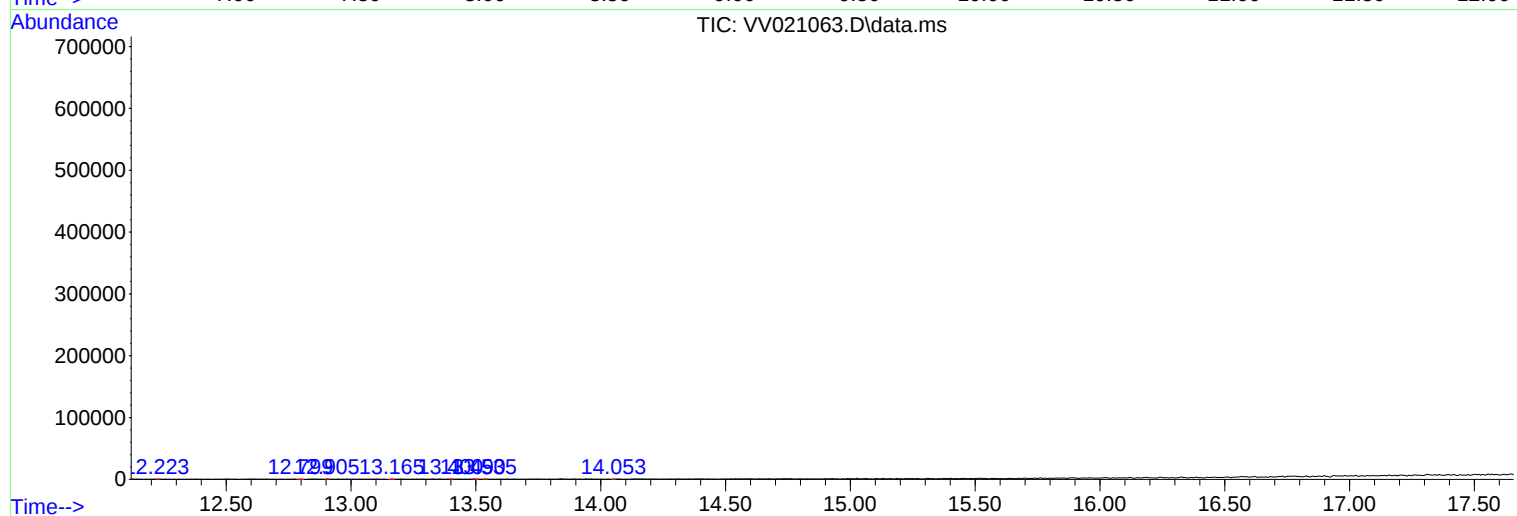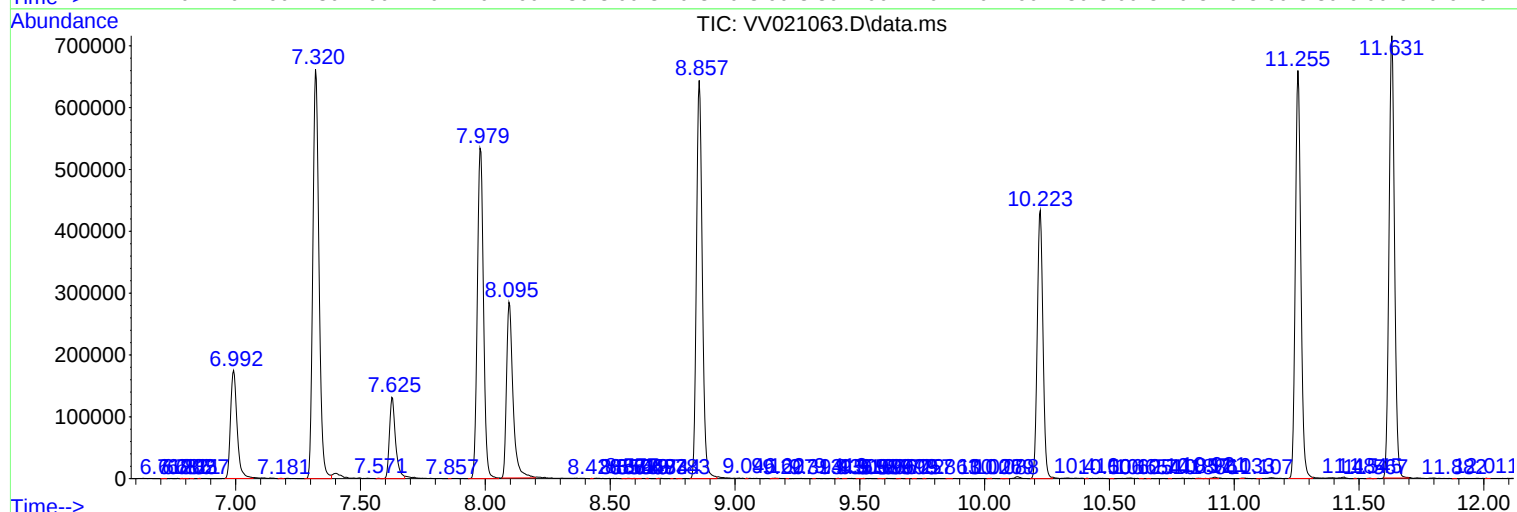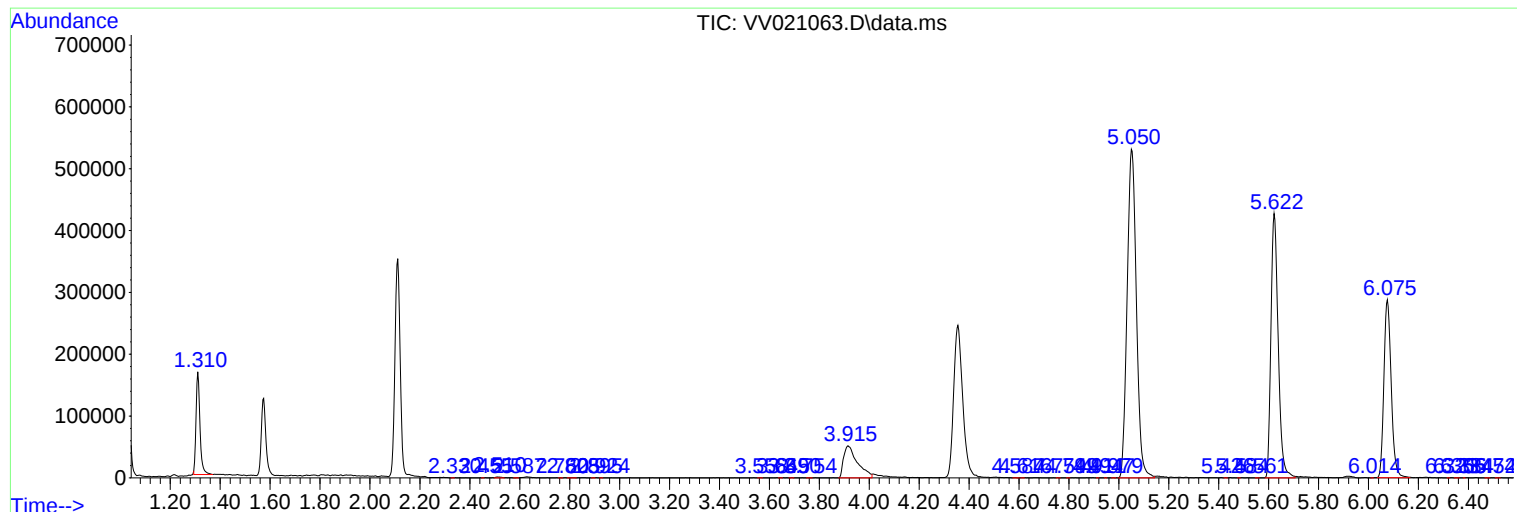

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021063.D
Acq On : 19 Apr 2021 18:36
Operator : SY/MD
Sample : M2067-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG799DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021063.D
Acq On : 19 Apr 2021 18:36
Operator : SY/MD
Sample : M2067-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG799DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
