

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021064.D
 Acq On : 19 Apr 2021 18:59
 Operator : SY/MD
 Sample : M2067-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.259	376	379	381	rBV	441	269	0.01%	0.002%
2	2.362	408	411	412	rVV	484	231	0.01%	0.002%
3	2.413	424	427	428	rBV	328	153	0.01%	0.001%
4	2.513	450	458	473	rBB8	2403	4705	0.16%	0.038%
5	2.600	481	485	486	rBV8	368	230	0.01%	0.002%
6	2.696	511	515	519	rBB2	288	275	0.01%	0.002%
7	2.754	529	533	536	rBV	717	651	0.02%	0.005%
8	2.783	540	542	546	rBV	632	392	0.01%	0.003%
9	2.828	551	556	559	rBB2	293	179	0.01%	0.001%
10	3.047	617	624	633	rBB6	2199	3881	0.13%	0.031%
11	3.313	703	707	709	rBB	292	191	0.01%	0.002%
12	3.365	721	723	725	rBB	280	130	0.00%	0.001%
13	3.455	748	751	752	rBV	258	131	0.00%	0.001%
14	3.548	779	780	783	rBV	223	129	0.00%	0.001%
15	3.590	790	793	797	rBB	391	243	0.01%	0.002%
16	3.754	840	844	845	rBV	385	207	0.01%	0.002%
17	3.834	866	869	871	rBV	207	159	0.01%	0.001%
18	3.866	876	879	882	rBB	318	149	0.01%	0.001%
19	3.918	883	895	926	rBV2	52125	200475	6.90%	1.606%
20	4.574	1094	1099	1104	rVB3	268	270	0.01%	0.002%
21	4.603	1104	1108	1112	rBV3	632	510	0.02%	0.004%
22	4.866	1187	1190	1193	rBV	240	141	0.00%	0.001%
23	4.947	1214	1215	1218	rBV	366	165	0.01%	0.001%
24	4.985	1224	1227	1230	rBB2	365	257	0.01%	0.002%
25	5.050	1230	1247	1277	rBV2	542539	1403986	48.29%	11.248%
26	5.407	1357	1358	1360	rBV	563	245	0.01%	0.002%
27	5.468	1374	1377	1379	rBB	267	153	0.01%	0.001%
28	5.487	1379	1383	1387	rBV2	582	467	0.02%	0.004%
29	5.510	1387	1390	1392	rVB	1014	486	0.02%	0.004%
30	5.526	1392	1395	1398	rBV2	466	289	0.01%	0.002%
31	5.622	1413	1425	1450	rBV	431322	876805	30.16%	7.024%
32	5.918	1504	1517	1548	rBV	491836	975211	33.55%	7.813%
33	6.297	1632	1635	1637	rBV2	691	405	0.01%	0.003%
34	6.484	1690	1693	1695	rBB2	375	186	0.01%	0.001%
35	6.564	1714	1718	1721	rBV2	276	264	0.01%	0.002%
36	6.599	1726	1729	1731	rBV	370	252	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021064.D
 Acq On : 19 Apr 2021 18:59
 Operator : SY/MD
 Sample : M2067-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.657	1745	1747	1751	rVV	457	286	0.01%	0.002%
38	6.673	1751	1752	1759	rVB2	531	441	0.02%	0.004%
39	6.847	1800	1806	1807	rBV2	285	249	0.01%	0.002%
40	6.879	1814	1816	1820	rBB	359	226	0.01%	0.002%
41	6.915	1821	1827	1828	rBV	353	233	0.01%	0.002%
42	6.950	1835	1838	1840	rBV	423	237	0.01%	0.002%
43	6.992	1840	1851	1877	rBV	176538	324180	11.15%	2.597%
44	7.185	1908	1911	1915	rVB3	482	377	0.01%	0.003%
45	7.214	1916	1920	1924	rBV4	564	535	0.02%	0.004%
46	7.278	1938	1940	1942	rBV	305	186	0.01%	0.001%
47	7.320	1942	1953	1972	rBV	657179	1146312	39.43%	9.183%
48	7.625	2038	2048	2072	rBV	131509	228631	7.86%	1.832%
49	7.837	2111	2114	2115	rBV	373	172	0.01%	0.001%
50	7.927	2140	2142	2144	rBV2	436	285	0.01%	0.002%
51	7.979	2145	2158	2185	rVV	1770623	2907148	100.00%	23.290%
52	8.098	2186	2195	2226	rVB2	270057	503149	17.31%	4.031%
53	8.426	2293	2297	2299	rBV3	436	330	0.01%	0.003%
54	8.468	2308	2310	2311	rBV3	365	148	0.01%	0.001%
55	8.545	2330	2334	2340	rBV2	418	603	0.02%	0.005%
56	8.570	2340	2342	2346	rVB	337	177	0.01%	0.001%
57	8.593	2347	2349	2354	rBV	530	367	0.01%	0.003%
58	8.616	2354	2356	2360	rVB	297	158	0.01%	0.001%
59	8.641	2360	2364	2365	rBV	275	194	0.01%	0.002%
60	8.677	2370	2375	2378	rBV3	445	373	0.01%	0.003%
61	8.715	2386	2387	2391	rBB2	384	229	0.01%	0.002%
62	8.763	2398	2402	2407	rBB2	550	424	0.01%	0.003%
63	8.792	2407	2411	2414	rBV2	396	367	0.01%	0.003%
64	8.857	2419	2431	2459	rBV	660059	1067702	36.73%	8.554%
65	9.152	2518	2523	2526	rBV2	931	858	0.03%	0.007%
66	9.326	2575	2577	2579	rVV	352	161	0.01%	0.001%
67	9.352	2582	2585	2587	rBB2	290	162	0.01%	0.001%
68	9.361	2587	2588	2590	rBB2	476	144	0.00%	0.001%
69	9.490	2625	2628	2630	rBV2	281	199	0.01%	0.002%
70	9.509	2633	2634	2638	rBB	269	162	0.01%	0.001%
71	9.535	2639	2642	2644	rBV	232	167	0.01%	0.001%
72	9.596	2658	2661	2664	rBB	279	177	0.01%	0.001%
73	9.622	2665	2669	2672	rBB2	527	367	0.01%	0.003%
74	9.641	2672	2675	2677	rBV	412	257	0.01%	0.002%
75	9.776	2714	2717	2719	rBV	289	175	0.01%	0.001%
76	9.831	2733	2734	2738	rVB	327	177	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021064.D
 Acq On : 19 Apr 2021 18:59
 Operator : SY/MD
 Sample : M2067-05DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	9.860	2738	2743	2748	rBV2	317	391	0.01%	0.003%
78	9.918	2758	2761	2762	rBV	256	166	0.01%	0.001%
79	9.979	2777	2780	2784	rBV2	266	231	0.01%	0.002%
80	10.024	2791	2794	2797	rBB	257	148	0.01%	0.001%
81	10.046	2797	2801	2803	rBV	230	199	0.01%	0.002%
82	10.223	2844	2856	2876	rBV	445864	695411	23.92%	5.571%
83	10.477	2933	2935	2938	rBB	413	201	0.01%	0.002%
84	10.493	2938	2940	2942	rBV	383	175	0.01%	0.001%
85	10.541	2950	2955	2957	rBV	220	219	0.01%	0.002%
86	10.641	2982	2986	2988	rBV	365	261	0.01%	0.002%
87	10.677	2992	2997	2999	rBV	494	350	0.01%	0.003%
88	10.747	3017	3019	3023	rBV	358	227	0.01%	0.002%
89	10.808	3034	3038	3044	rBV2	507	520	0.02%	0.004%
90	11.037	3104	3109	3112	rBV6	714	722	0.02%	0.006%
91	11.255	3165	3177	3197	rBV	663000	1021877	35.15%	8.187%
92	11.631	3283	3294	3311	rBV	715237	1098021	37.77%	8.797%
93	11.795	3341	3345	3353	rVB6	842	1250	0.04%	0.010%
94	11.831	3353	3356	3359	rBV3	589	428	0.01%	0.003%
95	12.194	3465	3469	3474	rVB2	428	345	0.01%	0.003%
96	12.300	3498	3502	3503	rBV2	433	273	0.01%	0.002%
97	12.432	3540	3543	3544	rBV	276	152	0.01%	0.001%
98	13.075	3740	3743	3746	rVB2	738	421	0.01%	0.003%
99	13.098	3746	3750	3752	rBV	471	346	0.01%	0.003%
100	13.284	3805	3808	3811	rBV2	568	424	0.01%	0.003%




Sum of corrected areas: 12482355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021064.D
Acq On : 19 Apr 2021 18:59
Operator : SY/MD
Sample : M2067-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

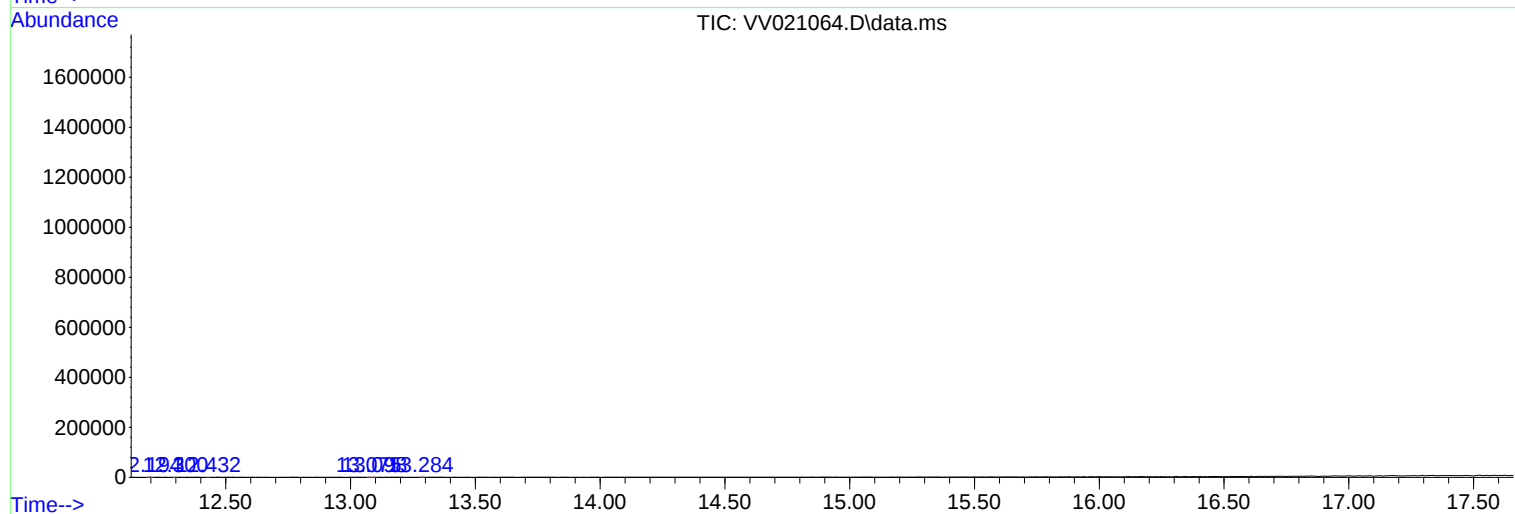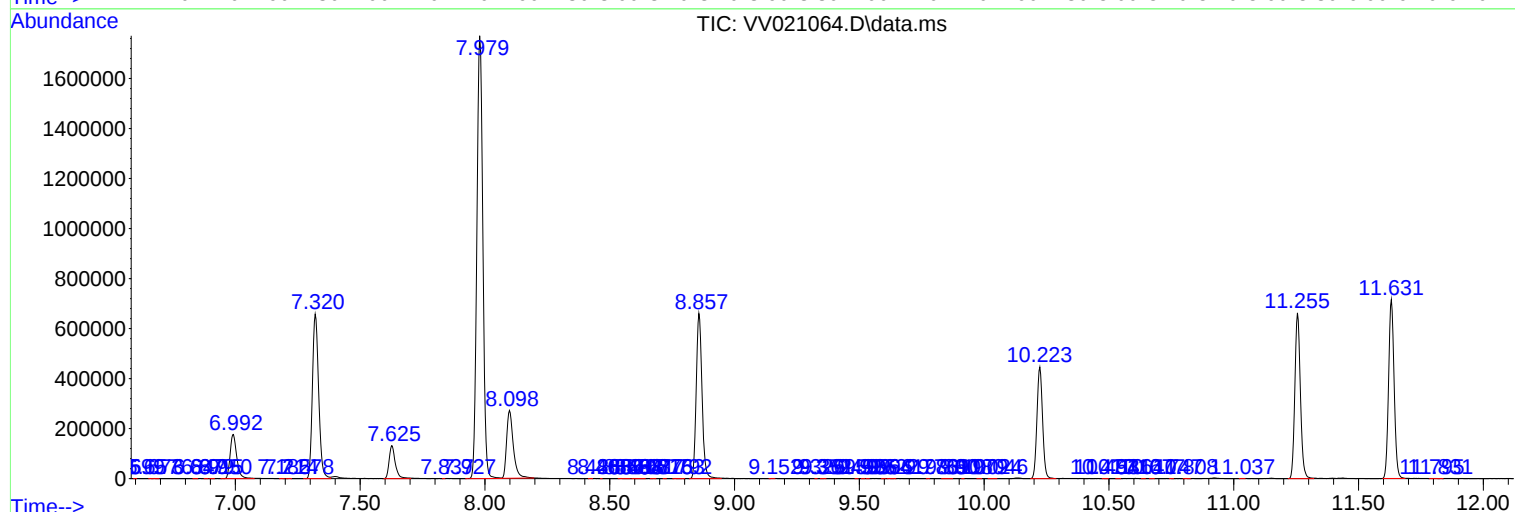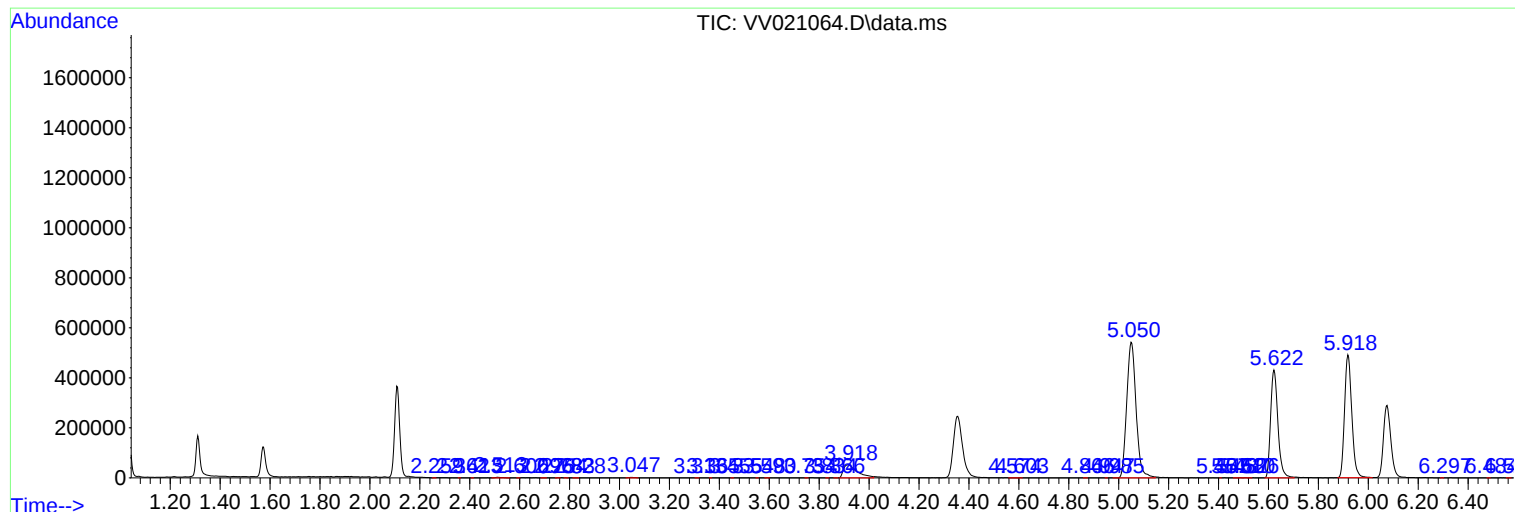

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021064.D
Acq On : 19 Apr 2021 18:59
Operator : SY/MD
Sample : M2067-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
Data File : VV021064.D
Acq On : 19 Apr 2021 18:59
Operator : SY/MD
Sample : M2067-05DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
