


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041921\
 Data File : VV021050.D
 Acq On : 19 Apr 2021 12:46
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB185

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 20 01:39:15 2021

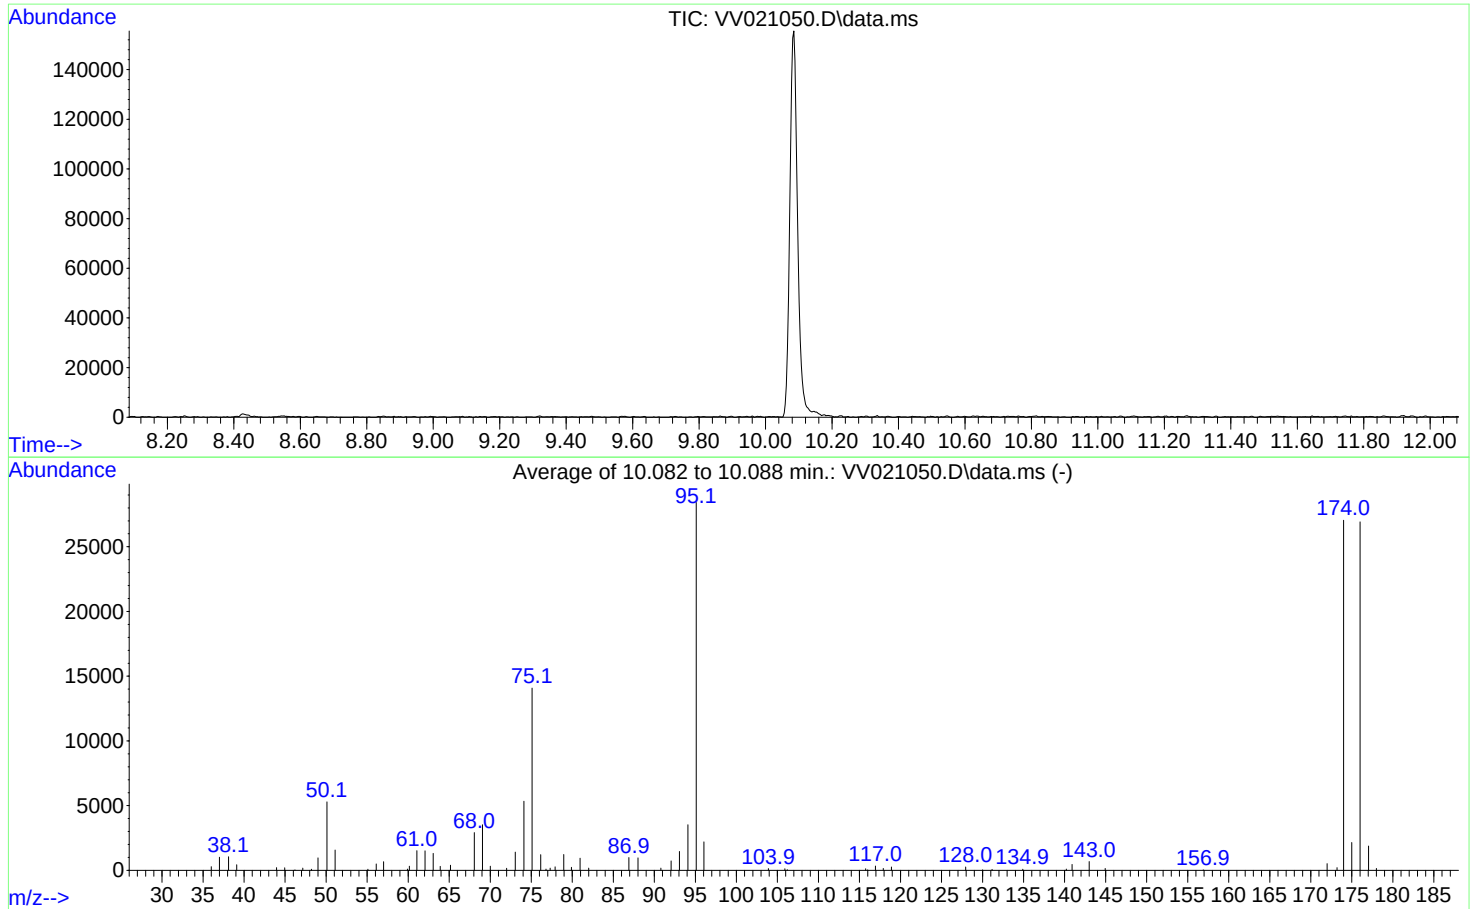

AutoFind: Scans 2812, 2813, 2814; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	5285	PASS
75	95	30	80	49.6	14082	PASS
95	95	100	100	100.0	28416	PASS
96	95	5	9	7.7	2199	PASS
173	174	0.00	2	0.8	207	PASS
174	95	50	120	95.2	27048	PASS
175	174	5	9	7.9	2146	PASS
176	174	95	101	99.5	26915	PASS
177	176	5	9	7.0	1883	PASS

m/z	Abundance
36.00	278.0
37.00	942.0
38.10	998.0
39.00	316.0
44.00	314.0
44.90	199.0
46.20	128.0
47.20	113.0
48.20	160.0
49.00	759.0
50.10	5499.0
51.10	1540.0
55.10	147.0
56.10	421.0
57.00	646.0
60.10	362.0
61.10	1378.0
62.00	1435.0
63.10	1402.0
63.90	223.0
65.20	421.0
68.10	2969.0
69.00	2968.0
70.00	230.0
72.10	186.0
73.10	1446.0
74.10	5149.0
75.10	13182.0
76.10	1143.0
76.80	155.0
77.90	144.0
79.00	1188.0
79.90	235.0
81.00	1019.0
82.00	173.0
86.90	981.0
88.00	821.0
90.80	178.0
92.00	641.0
93.00	1217.0
94.10	3275.0
95.10	27608.0
96.00	2050.0
103.90	139.0
106.20	141.0
115.70	121.0
116.00	112.0
116.90	356.0
117.90	149.0
119.00	247.0
127.90	229.0
131.20	106.0
140.20	177.0
140.90	415.0
143.00	709.0
144.90	145.0
172.00	508.0
174.00	26008.0
175.00	1893.0
176.00	25624.0
177.10	1720.0
178.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB185

m/z	Abundance
43.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB185

m/z	Abundance
36.00	283.0
37.00	1054.0
38.10	1055.0
39.10	455.0
44.00	362.0
44.90	232.0
47.20	198.0
48.20	119.0
49.00	1010.0
50.10	5482.0
51.10	1637.0
55.10	112.0
56.10	537.0
57.00	643.0
60.20	322.0
61.00	1579.0
62.00	1596.0
63.10	1315.0
63.90	322.0
65.20	418.0
68.10	2990.0
69.10	3670.0
70.00	346.0
72.00	141.0
73.10	1420.0
74.10	5604.0
75.10	14498.0
76.10	1265.0
76.80	140.0
77.30	195.0
77.90	305.0
79.00	1249.0
79.90	238.0
80.90	962.0
82.00	175.0
86.90	1023.0
88.00	1018.0
90.80	183.0
92.00	752.0
93.10	1434.0
94.10	3621.0
95.10	29536.0
96.00	2235.0
103.90	138.0
105.90	158.0
115.80	140.0
116.90	318.0
117.90	172.0
118.90	251.0
128.00	281.0
131.10	102.0
134.90	107.0
140.20	132.0
140.90	479.0
143.00	686.0
145.00	161.0
172.00	574.0
174.00	27752.0
175.00	2221.0
176.00	28000.0
177.00	1986.0
178.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB185

m/z	Abundance
36.00	287.0
37.00	1027.0
38.10	1113.0
39.10	537.0
44.00	313.0
45.00	169.0
47.10	200.0
49.00	1132.0
50.10	4874.0
51.10	1532.0
56.10	527.0
57.00	699.0
59.90	294.0
60.10	287.0
61.00	1607.0
62.10	1505.0
63.00	1209.0
63.90	370.0
65.10	345.0
68.00	2803.0
69.10	3925.0
70.00	372.0
71.90	168.0
73.00	1350.0
74.10	5263.0
75.10	14566.0
76.20	1229.0
77.30	309.0
77.90	383.0
78.90	1217.0
79.90	250.0
81.00	850.0
82.00	168.0
86.90	981.0
88.00	1046.0
90.80	146.0
92.10	793.0
93.10	1742.0
94.10	3658.0
95.10	28104.0
96.10	2311.0
103.90	141.0
105.90	219.0
115.80	120.0
117.10	336.0
117.90	136.0
118.80	294.0
128.00	255.0
130.00	110.0
134.90	147.0
140.90	494.0
143.00	649.0
145.00	151.0
156.90	104.0
172.00	480.0
173.20	621.0
174.00	27384.0
175.00	2325.0
176.00	27120.0
177.00	1944.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB185