

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041923\
 Data File : VW030671.D
 Acq On : 19 Apr 2023 17:42
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 20 01:30:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 01:26:42 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	230221	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	220250	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	102285	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	87530	51.863	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 103.720%	
7) Chloroethane-d5	1.539	69	75642	53.484	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery		

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030671.D
Acq On : 19 Apr 2023 17:42
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 20 01:30:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 01:26:42 2023
Response via : Initial Calibration

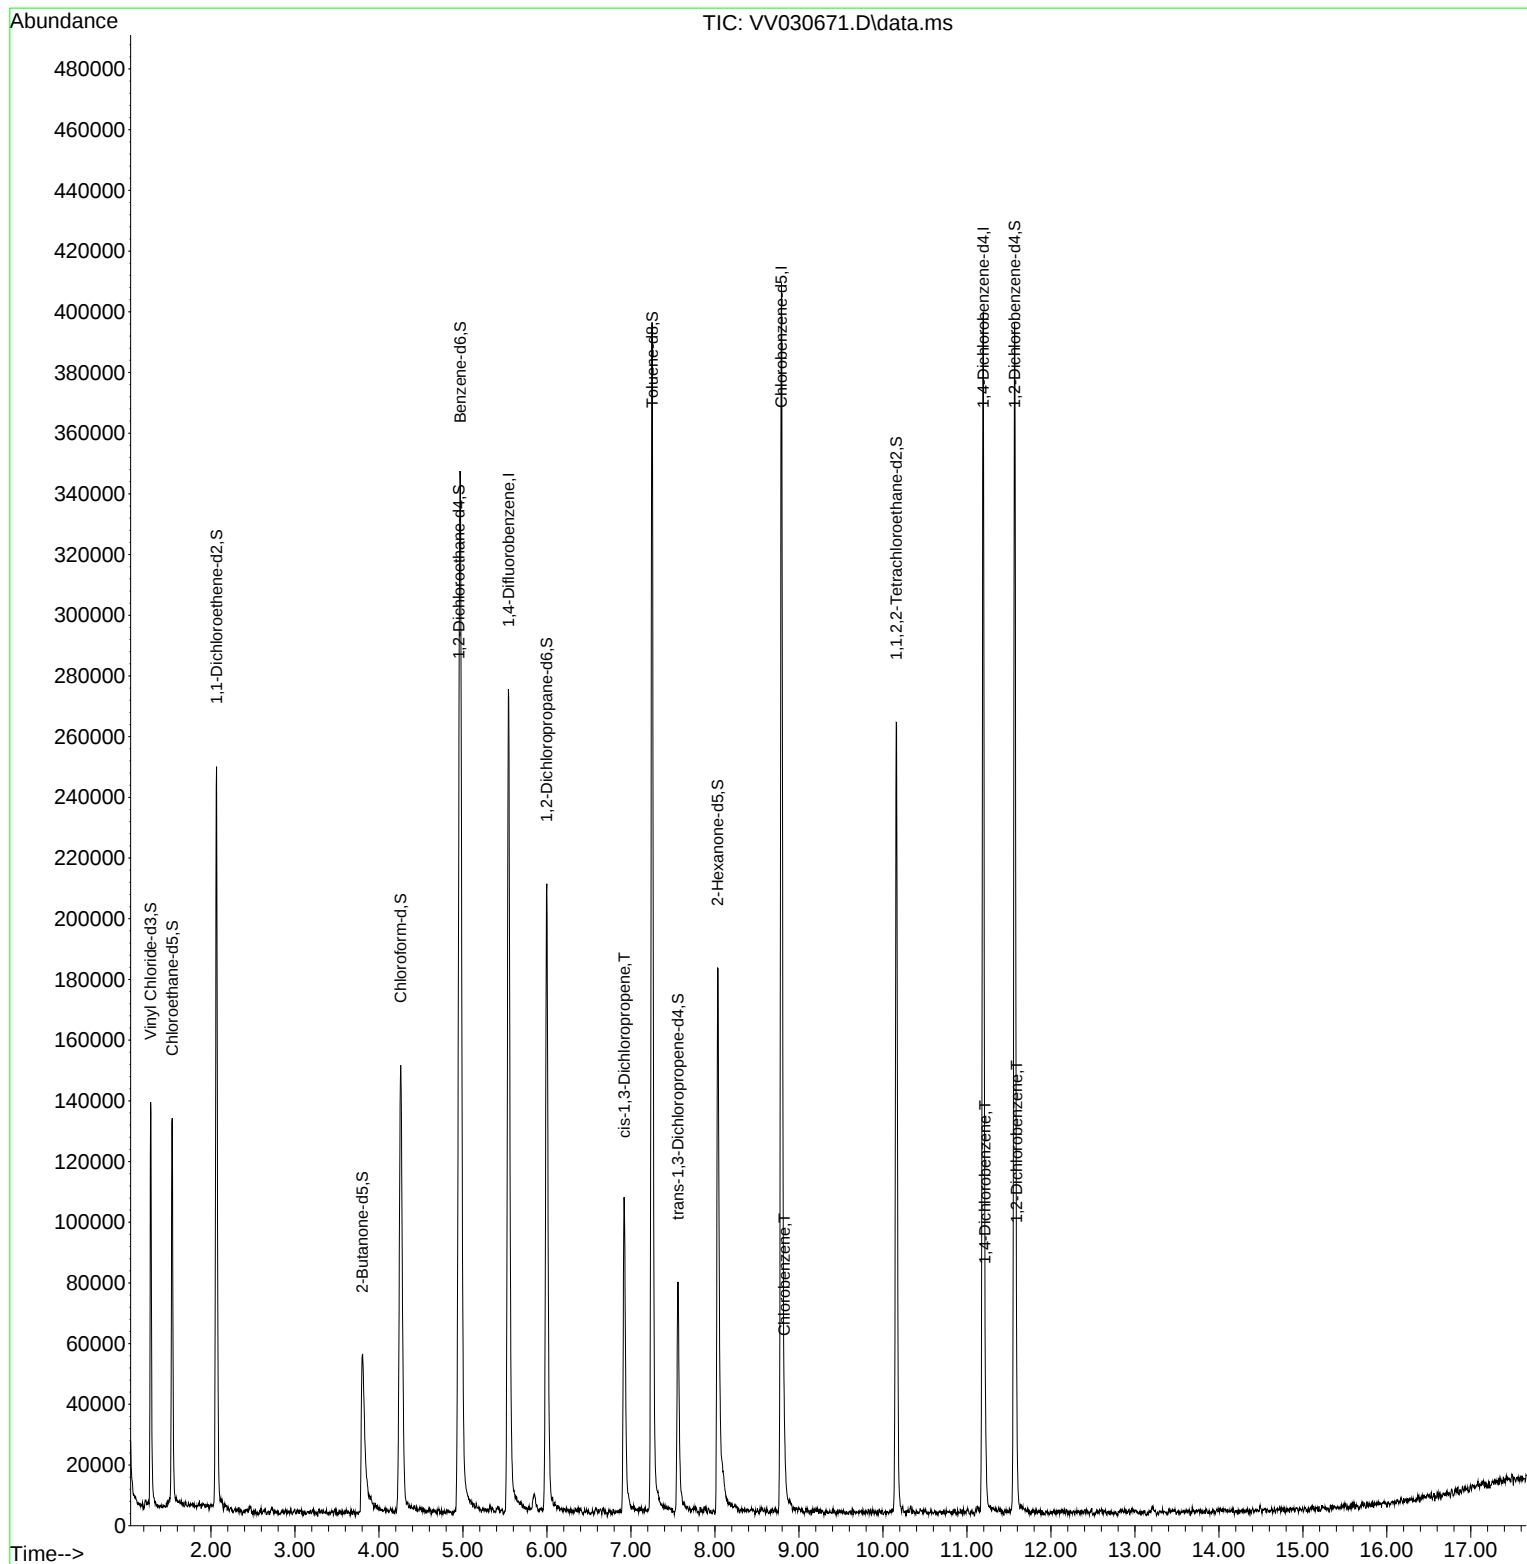

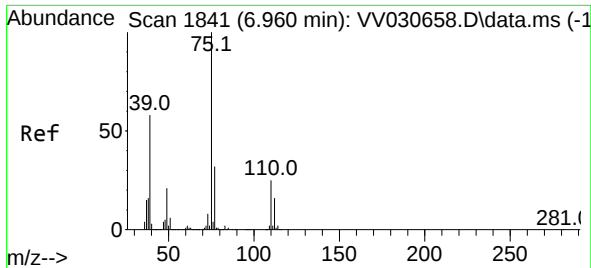

#39

cis-1,3-Dichloropropene

Concen: 1.175 ug/L

RT: 6.921 min Scan# 1829

Delta R.T. -0.039 min

Lab File: VV030671.D

Acq: 19 Apr 2023 17:42

Instrument :

MSVOA_V





ClientSampleId :


Tgt Ion: 75 Resp: 3174

Ion Ratio Lower Upper

75 100

77 54.1 22.0 40.8#

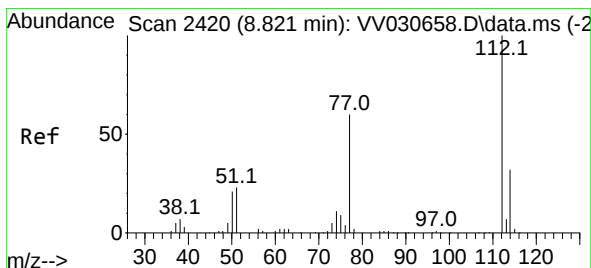
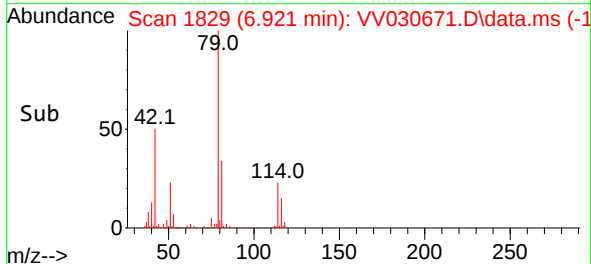
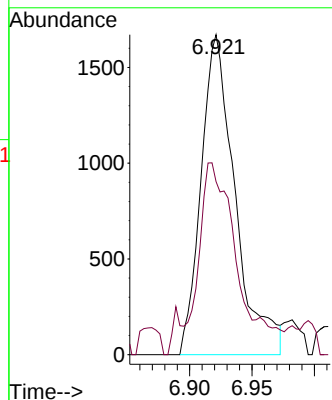
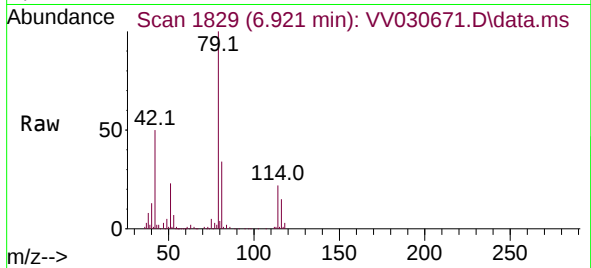


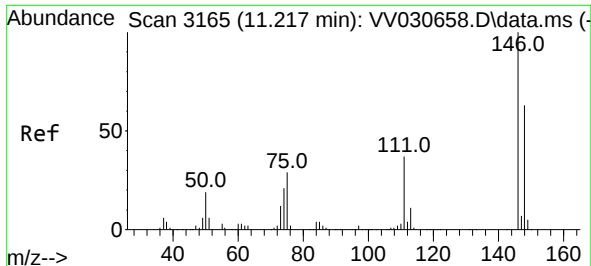

#65
1,4-Dichlorobenzene
Concen: 1.652 ug/L
RT: 11.217 min Scan# 3165
Delta R.T. -0.000 min
Lab File: VV030671.D
Acq: 19 Apr 2023 17:42

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion:146 Resp: 5563
Ion Ratio Lower Upper
146 100
111 45.6 26.5 49.1
148 69.8 44.7 83.1

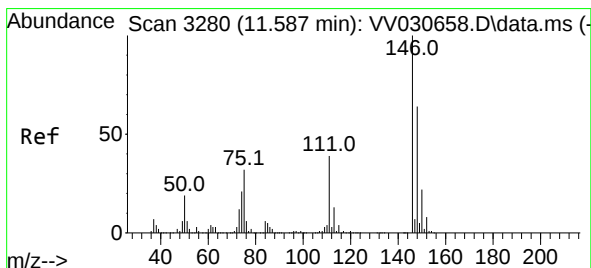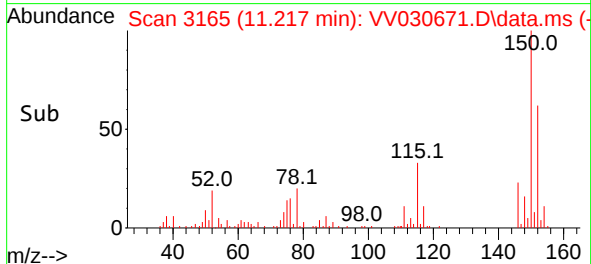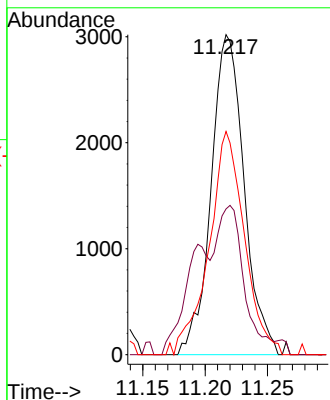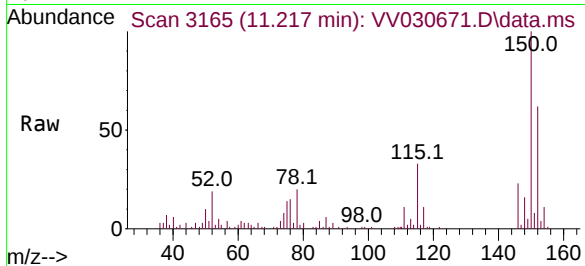

#67
1,2-Dichlorobenzene
Concen: 1.333 ug/L
RT: 11.590 min Scan# 3281
Delta R.T. 0.003 min
Lab File: VV030671.D
Acq: 19 Apr 2023 17:42

Tgt Ion:146 Resp: 4295
Ion Ratio Lower Upper
146 100
111 41.5 32.0 48.0
148 71.4 50.6 76.0

