




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030662.D
 Acq On : 19 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02360-20DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3DL

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:28:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 01:26:42 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2023
 Supervised By :Mahesh Dadoda 04/20/2023

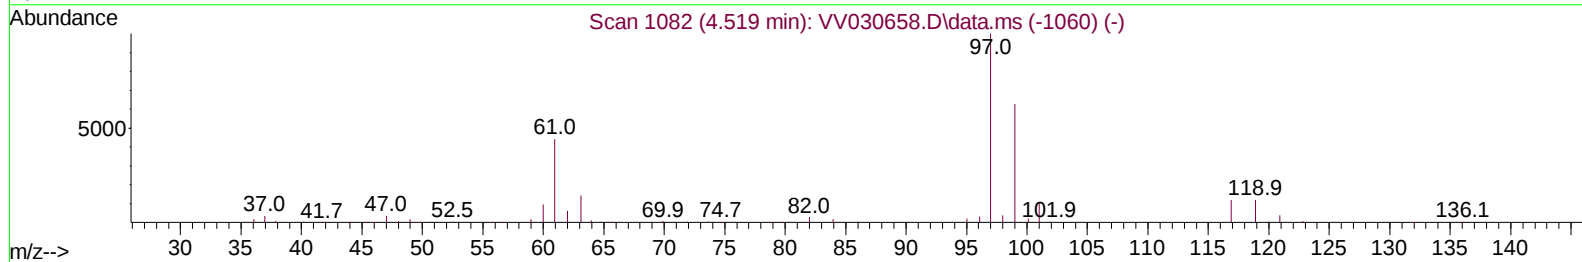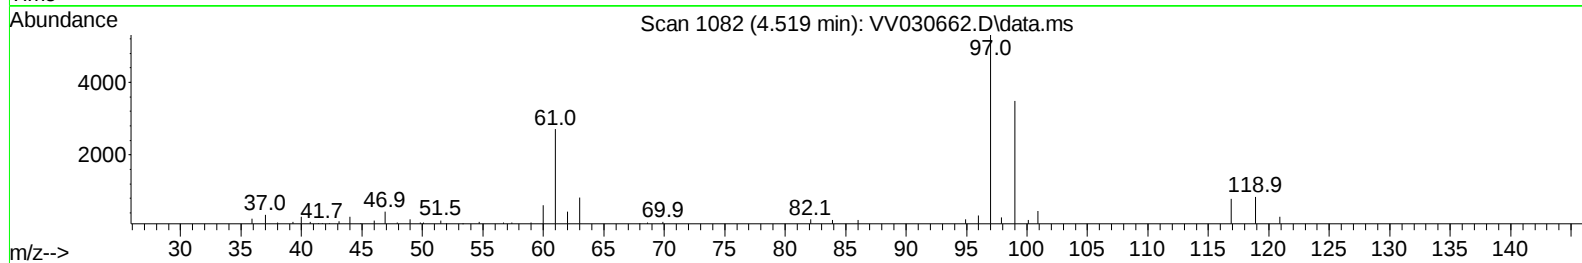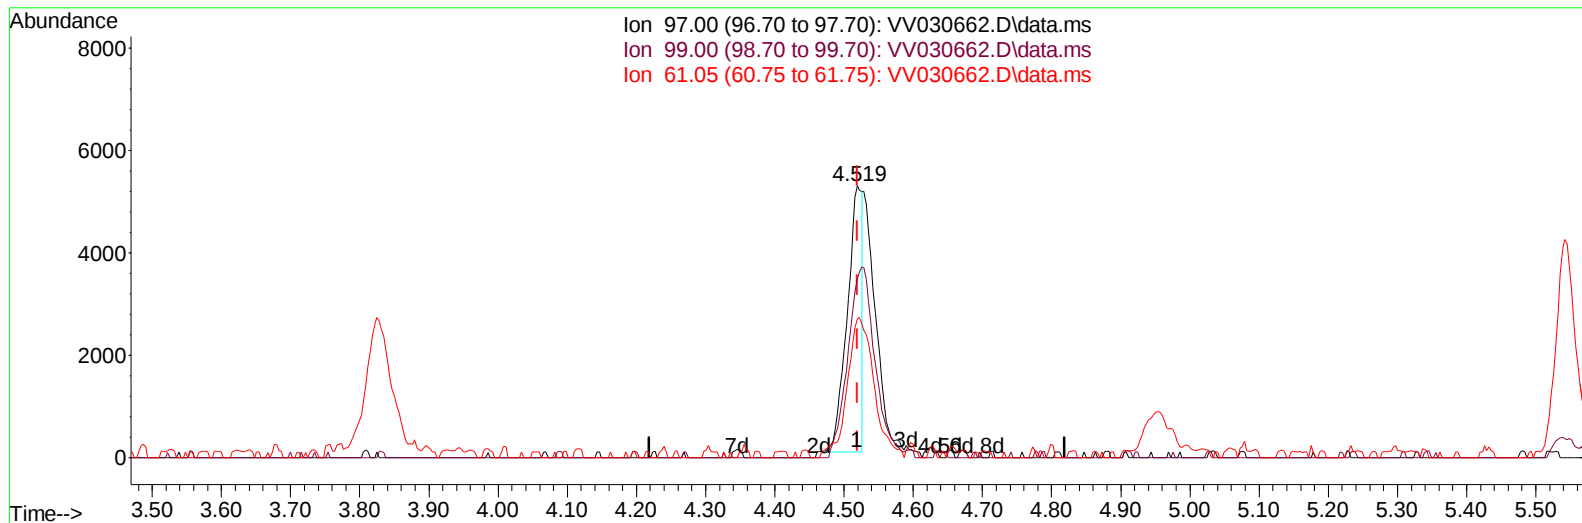

TIC: VV030662.D\data.ms

(30) 1,1,1-Trichloroethane (T)

4.519min (-0.000) 2.52 ug/L

response 7737

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.20	130.24#
61.05	46.30	94.82#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030662.D
 Acq On : 19 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02360-20DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3DL

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:28:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 01:26:42 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2023
 Supervised By :Mahesh Dadoda 04/20/2023

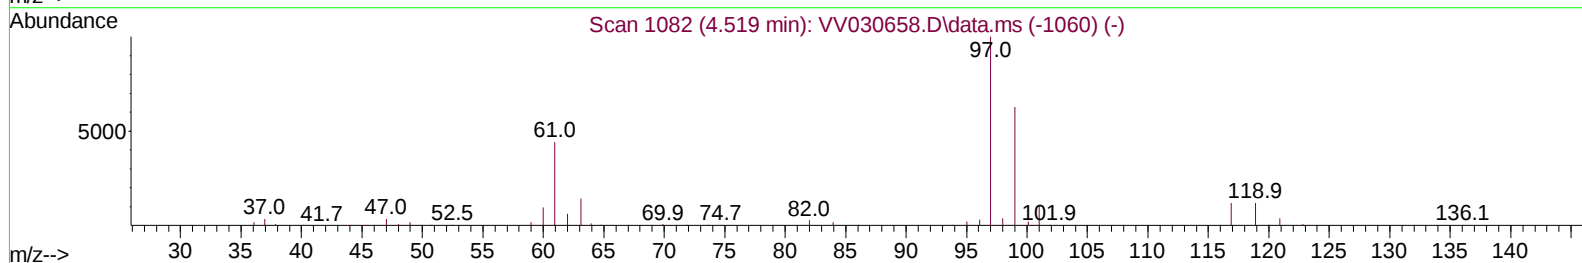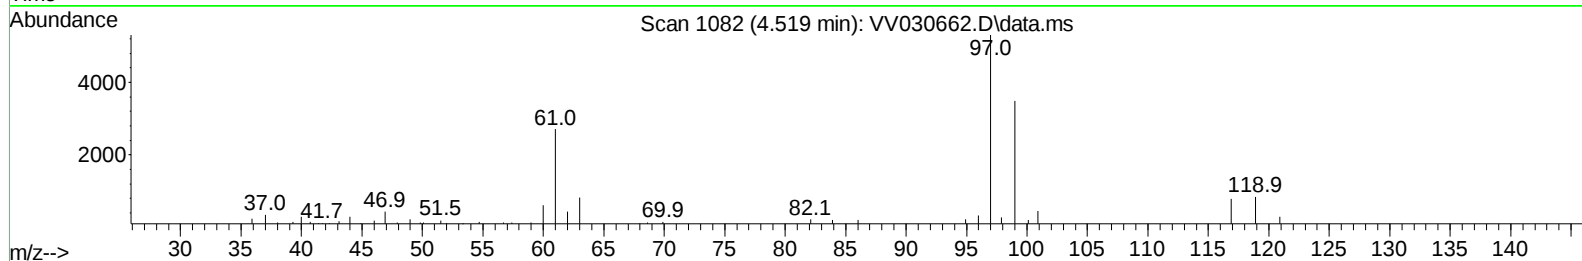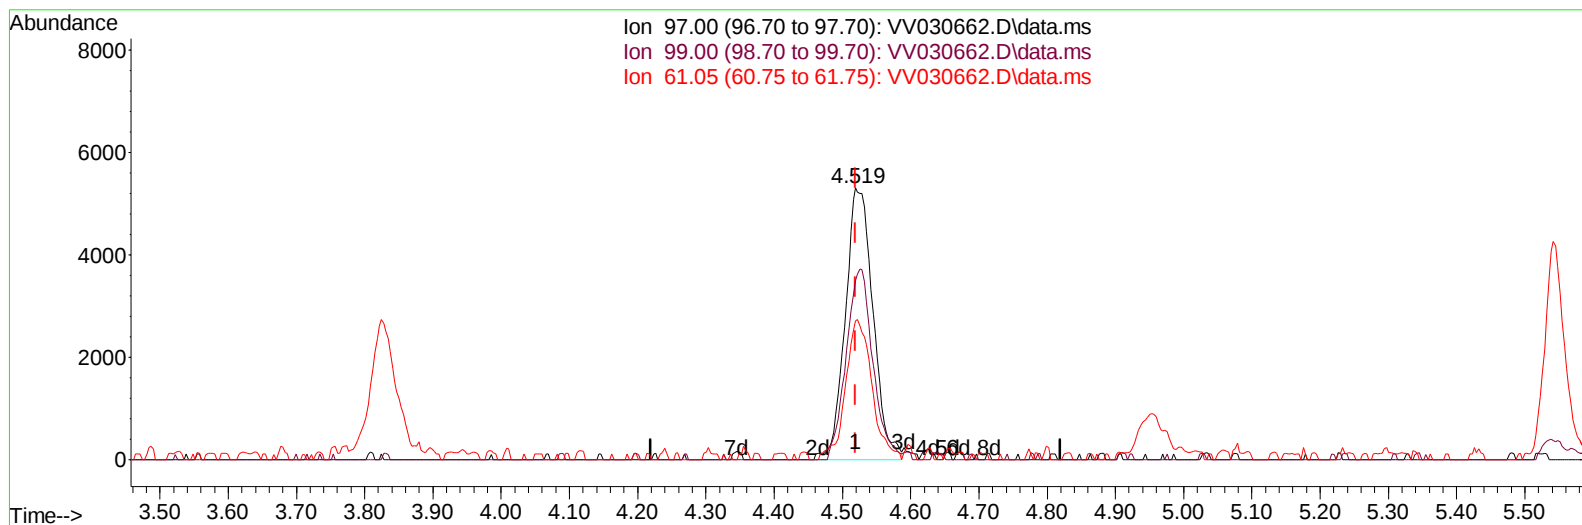

TIC: VV030662.D\data.ms

(30) 1,1,1-Trichloroethane (T)

4.519min (-0.000) 4.87 ug/L m

response 14931

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.20	67.49
61.05	46.30	49.13
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030662.D
 Acq On : 19 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02360-20DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3DL

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:28:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 01:26:42 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2023
 Supervised By :Mahesh Dadoda 04/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	228139	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	218219	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	102758	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	55256	33.039	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	66.080%	
7) Chloroethane-d5	1.535	69	50374	35.943	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	71.880%	
11) 1,1-Dichloroethene-d2	2.066	65	29165	36.772	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.540%	
21) 2-Butanone-d5	3.796	46	94754	103.150	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	103.150%	
24) Chloroform-d	4.259	84	133928	44.188	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.380%	
26) 1,2-Dichloroethane-d4	4.950	65	93063	47.759	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.520%	
32) Benzene-d6	4.969	84	236020	45.746	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.500%	
36) 1,2-Dichloropropane-d6	5.998	67	77989	48.664	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.320%	
41) Toluene-d8	7.252	98	197702	40.813	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.620%	
43) trans-1,3-Dichloroprop...	7.561	79	35820	44.345	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.700%	
47) 2-Hexanone-d5	8.034	63	61018	96.649	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	96.650%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	112612	48.425	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	96.860%	
66) 1,2-Dichlorobenzene-d4	11.567	152	87675	53.680	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	107.360%	
Target Compounds						
12) 1,1-Dichloroethene	2.072	96	2230	1.396	ug/L	# 1
20) cis-1,2-Dichloroethene	3.825	96	4365	2.488	ug/L	85
30) 1,1,1-Trichloroethane	4.519	97	14931m	4.869	ug/L	
34) Trichloroethene	5.841	95	93842	54.444	ug/L	99
51) Chlorobenzene	8.821	112	13530	2.878	ug/L	99
65) 1,4-Dichlorobenzene	11.217	146	8400	2.483	ug/L	96
67) 1,2-Dichlorobenzene	11.586	146	6257	1.933	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030662.D
Acq On : 19 Apr 2023 14:12
Operator : SY/MD
Sample : 02360-20DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ3DL

Manual IntegrationsAPPROVED

Quant Time: Apr 20 01:28:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 01:26:42 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2023
Supervised By :Mahesh Dadoda 04/20/2023

