

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030659.D
 Acq On : 19 Apr 2023 12:30
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	155745	172463	16.79%	2.256%
2	1.535	148	154	167	rVB	134516	154662	15.05%	2.023%
3	2.063	309	318	332	rBV	271877	397157	38.66%	5.195%
4	2.391	418	420	431	rVB10	1595	1672	0.16%	0.022%
5	2.455	431	440	454	rVV10	5933	11499	1.12%	0.150%
6	2.513	456	458	461	rVB4	1894	891	0.09%	0.012%
7	2.542	461	467	468	rBV6	1032	866	0.08%	0.011%
8	2.632	491	495	497	rBV4	2610	1843	0.18%	0.024%
9	2.777	537	540	543	rVB6	2134	1159	0.11%	0.015%
10	2.806	543	549	553	rBV9	2236	2668	0.26%	0.035%
11	2.883	570	573	574	rBV3	1001	574	0.06%	0.008%
12	2.963	595	598	600	rBV4	1352	960	0.09%	0.013%
13	3.018	611	615	616	rBV4	1378	1023	0.10%	0.013%
14	3.072	630	632	634	rBV2	1137	701	0.07%	0.009%
15	3.121	643	647	651	rBV7	2193	2008	0.20%	0.026%
16	3.272	691	694	699	rVB6	1903	1812	0.18%	0.024%
17	3.310	704	706	707	rBV2	1070	429	0.04%	0.006%
18	3.346	713	717	718	rBV4	1327	914	0.09%	0.012%
19	3.394	725	732	735	rBV8	2435	2729	0.27%	0.036%
20	3.558	780	783	786	rBV5	1149	883	0.09%	0.012%
21	3.658	812	814	816	rVB3	1245	543	0.05%	0.007%
22	3.699	824	827	829	rBV4	1747	968	0.09%	0.013%
23	3.712	829	831	834	rBV4	1288	754	0.07%	0.010%
24	3.796	847	857	883	rBV2	56780	163643	15.93%	2.141%
25	4.256	988	1000	1022	rVB	158072	395169	38.47%	5.169%
26	4.609	1104	1110	1112	rVB6	1637	1736	0.17%	0.023%
27	4.629	1112	1116	1119	rBV5	1205	1066	0.10%	0.014%
28	4.754	1152	1155	1157	rBV3	1812	1119	0.11%	0.015%
29	4.815	1173	1174	1177	rBV3	1261	790	0.08%	0.010%
30	4.895	1197	1199	1201	rBV3	1134	458	0.04%	0.006%
31	4.963	1203	1220	1245	rVV2	388445	1027346	100.00%	13.439%
32	5.539	1388	1399	1419	rBV	293627	598168	58.22%	7.825%
33	5.995	1529	1541	1562	rBV	221966	451275	43.93%	5.903%
34	6.297	1633	1635	1636	rBV2	1745	624	0.06%	0.008%
35	6.458	1682	1685	1687	rBV4	1095	787	0.08%	0.010%
36	6.664	1747	1749	1750	rBV3	1080	499	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030659.D
 Acq On : 19 Apr 2023 12:30
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.825	1798	1799	1801	rBV2	1357	660	0.06%	0.009%
38	6.918	1817	1828	1848	rBV	119148	227833	22.18%	2.980%
39	7.249	1919	1931	1952	rBV	439196	780302	75.95%	10.207%
40	7.558	2018	2027	2042	rBV	84548	151338	14.73%	1.980%
41	7.947	2145	2148	2149	rBV3	1596	820	0.08%	0.011%
42	8.030	2162	2174	2205	rBV	189898	395137	38.46%	5.169%
43	8.555	2333	2337	2338	rBV4	1359	931	0.09%	0.012%
44	8.667	2371	2372	2375	rBV2	1385	764	0.07%	0.010%
45	8.789	2398	2410	2435	rBV	439117	800249	77.89%	10.468%
46	9.111	2507	2510	2512	rBV3	1358	646	0.06%	0.008%
47	9.181	2529	2532	2533	rBV3	1494	857	0.08%	0.011%
48	9.217	2540	2543	2545	rBV4	1494	900	0.09%	0.012%
49	9.265	2556	2558	2559	rBV2	1543	514	0.05%	0.007%
50	9.349	2580	2584	2585	rBV3	1771	1222	0.12%	0.016%
51	9.513	2631	2635	2636	rBV4	2353	1736	0.17%	0.023%
52	9.757	2707	2711	2713	rBV5	2150	1554	0.15%	0.020%
53	9.966	2773	2776	2777	rBV3	1627	834	0.08%	0.011%
54	9.995	2783	2785	2786	rBV3	1121	625	0.06%	0.008%
55	10.159	2826	2836	2856	rVB	268345	435977	42.44%	5.703%
56	10.378	2900	2904	2905	rBV4	1199	767	0.07%	0.010%
57	10.423	2914	2918	2921	rVB5	1620	931	0.09%	0.012%
58	10.439	2921	2923	2925	rBV3	1331	683	0.07%	0.009%
59	10.667	2993	2994	2997	rVB3	1421	608	0.06%	0.008%
60	10.680	2997	2998	3001	rBV3	1011	580	0.06%	0.008%
61	10.702	3001	3005	3007	rBV4	2281	1642	0.16%	0.021%
62	10.728	3011	3013	3017	rVB4	1776	934	0.09%	0.012%
63	10.767	3021	3025	3026	rBV4	1729	1177	0.11%	0.015%
64	10.831	3041	3045	3047	rBV5	1731	1211	0.12%	0.016%
65	11.069	3115	3119	3122	rBV6	1522	1533	0.15%	0.020%
66	11.130	3132	3138	3140	rBV6	3080	3508	0.34%	0.046%
67	11.194	3147	3158	3180	rBV	412223	686835	66.86%	8.985%
68	11.400	3220	3222	3224	rBV3	1491	785	0.08%	0.010%
69	11.426	3228	3230	3233	rBV4	1395	843	0.08%	0.011%
70	11.522	3257	3260	3261	rBV2	1768	1044	0.10%	0.014%
71	11.567	3263	3274	3290	rVV	415486	691970	67.36%	9.052%
72	11.805	3346	3348	3351	rVB3	927	415	0.04%	0.005%
73	11.895	3372	3376	3377	rBV3	1525	1053	0.10%	0.014%
74	12.416	3534	3538	3540	rBV5	1510	1122	0.11%	0.015%
75	12.487	3558	3560	3563	rBV4	1829	1049	0.10%	0.014%
76	12.574	3585	3587	3588	rBV	1171	550	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030659.D
 Acq On : 19 Apr 2023 12:30
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.648	3606	3610	3612	rBV5	1266	841	0.08%	0.011%
78	12.712	3624	3630	3634	rVB7	1897	2013	0.20%	0.026%
79	12.734	3634	3637	3641	rBV6	1407	1157	0.11%	0.015%
80	12.908	3687	3691	3693	rBV4	1673	1404	0.14%	0.018%
81	13.001	3716	3720	3724	rBV7	2998	2443	0.24%	0.032%
82	13.021	3724	3726	3730	rBV4	1496	1113	0.11%	0.015%
83	13.059	3736	3738	3743	rBV6	1675	1464	0.14%	0.019%
84	13.210	3778	3785	3794	rVV6	5673	10034	0.98%	0.131%
85	13.268	3801	3803	3806	rBV4	1372	780	0.08%	0.010%
86	13.342	3824	3826	3830	rBV5	1775	1201	0.12%	0.016%
87	13.368	3830	3834	3836	rBV5	1604	1238	0.12%	0.016%
88	13.525	3881	3883	3885	rVB2	1316	633	0.06%	0.008%
89	13.574	3896	3898	3900	rBV3	1441	818	0.08%	0.011%
90	13.609	3904	3909	3912	rBV6	2631	2530	0.25%	0.033%
91	13.670	3925	3928	3929	rBV3	1725	964	0.09%	0.013%
92	13.693	3929	3935	3936	rVV5	3253	2963	0.29%	0.039%
93	13.779	3960	3962	3964	rBV3	1834	991	0.10%	0.013%
94	13.860	3985	3987	3990	rBV4	1508	1091	0.11%	0.014%
95	13.988	4025	4027	4031	rVV5	1505	1194	0.12%	0.016%
96	14.246	4106	4107	4108	rBV	1089	410	0.04%	0.005%
97	14.300	4122	4124	4128	rBV5	1329	945	0.09%	0.012%
98	14.410	4156	4158	4160	rBV3	1514	956	0.09%	0.013%
99	14.651	4229	4233	4236	rBV6	2381	2240	0.22%	0.029%
100	15.493	4493	4495	4497	rBV3	2118	1123	0.11%	0.015%




Sum of corrected areas: 7644543

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030659.D
Acq On : 19 Apr 2023 12:30
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

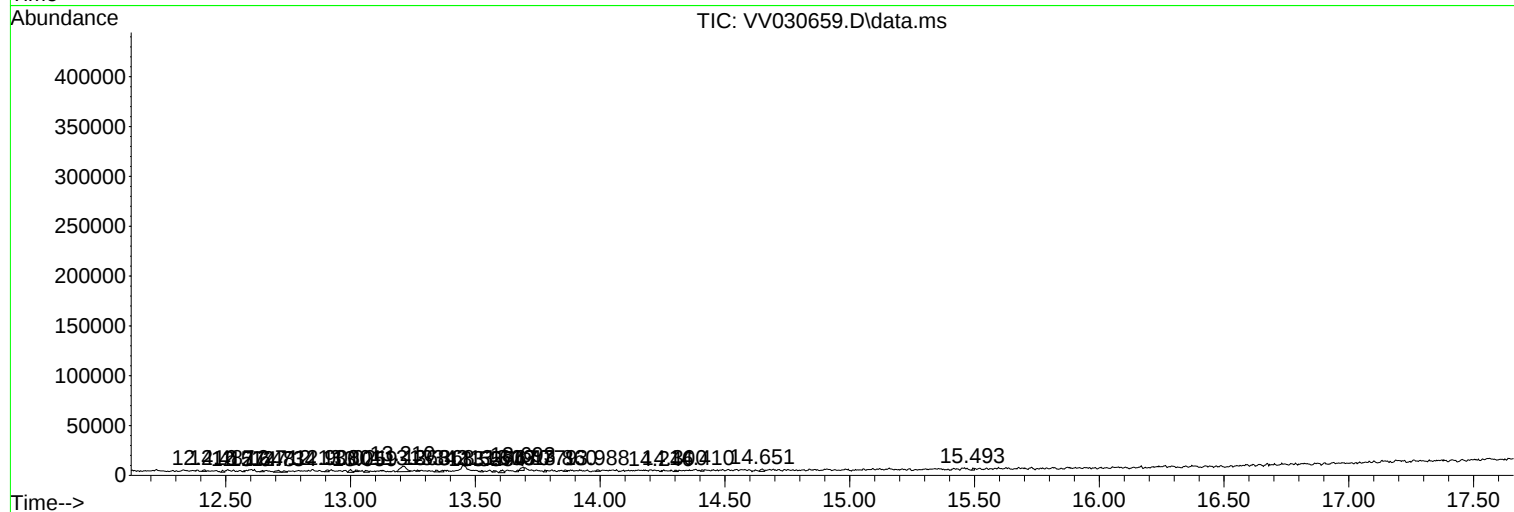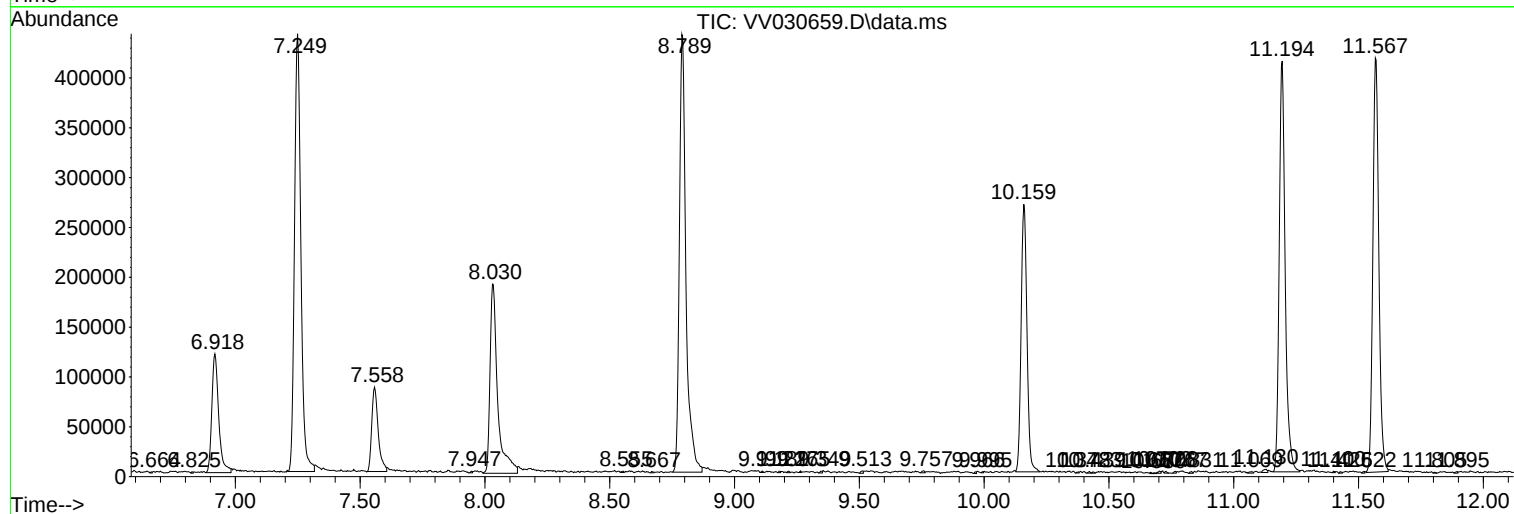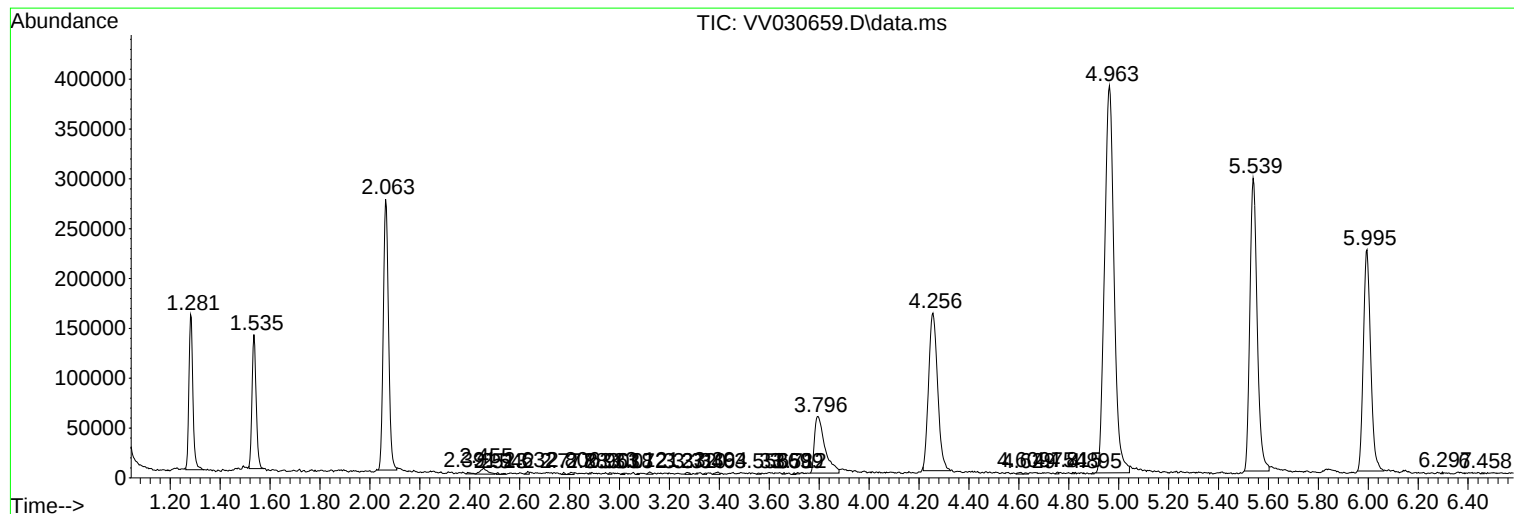

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030659.D
Acq On : 19 Apr 2023 12:30
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030659.D
Acq On : 19 Apr 2023 12:30
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------